

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
 Data File : VD078052.D
 Acq On : 22 Dec 2023 05:13
 Operator : RP/MD
 Sample : 05877-20
 Misc : 5.28G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 COM57

Quant Time: Dec 22 07:53:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	148573	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	274677	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	253629	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	99704	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	74114	42.333	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	84.660%
35) Dibromofluoromethane	7.810	113	85089	44.225	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	88.440%
50) Toluene-d8	10.269	98	344886	44.756	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	89.520%
62) 4-Bromofluorobenzene	12.575	95	93111	40.415	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	80.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
Data File : VD078052.D
Acq On : 22 Dec 2023 05:13
Operator : RP/MD
Sample : 05877-20
Misc : 5.28G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
COM57

Quant Time: Dec 22 07:53:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration




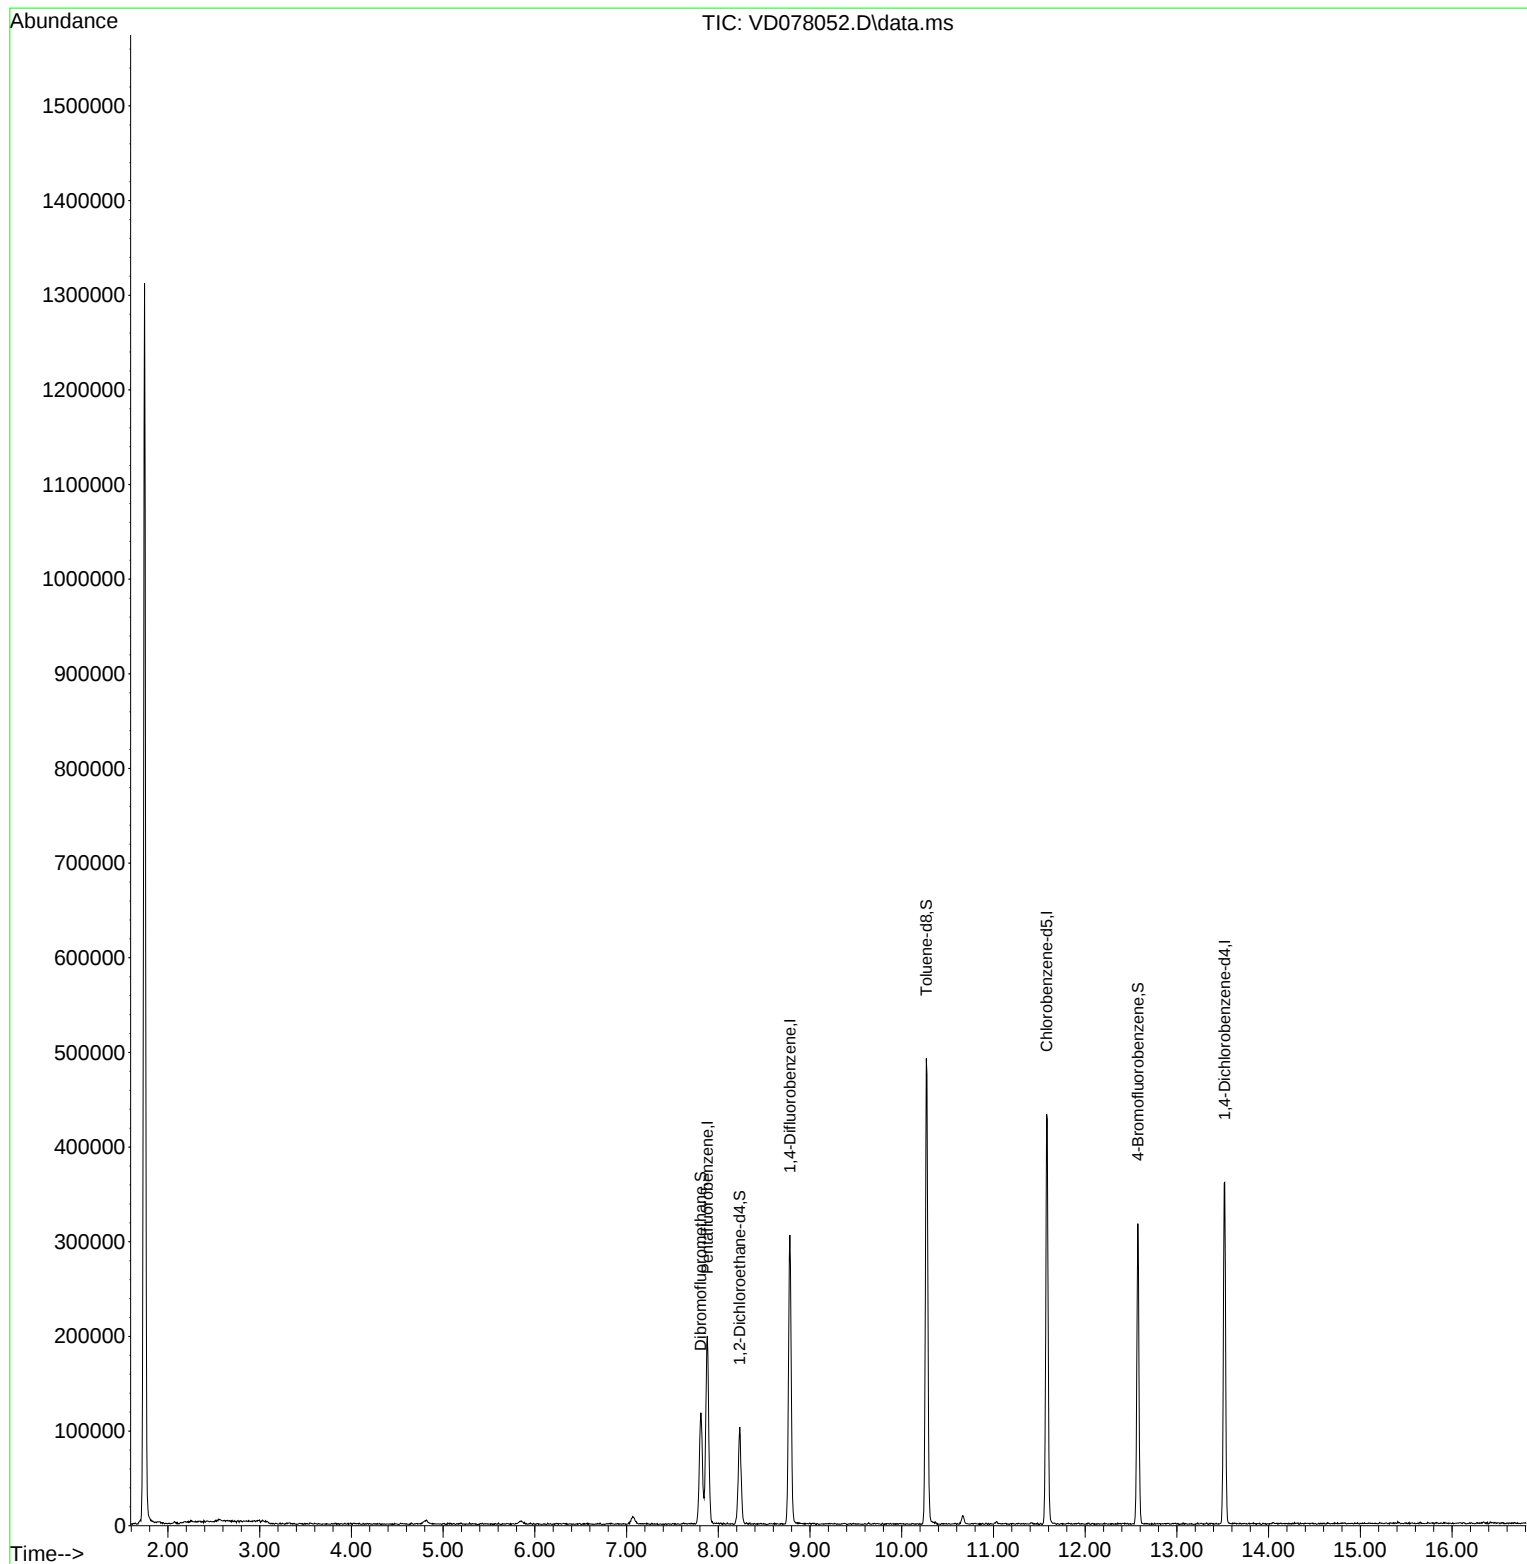


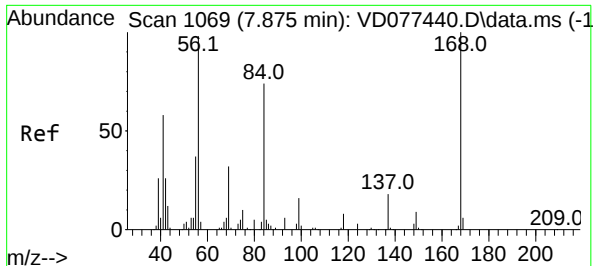

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 110
Delta R.T. 0.006 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13




Instrument :
MSVOA_D
ClientSampleId :
COM57


Tgt Ion:168 Resp: 148573
Ion Ratio Lower Upper
168 100
99 54.3 36.7 55.1

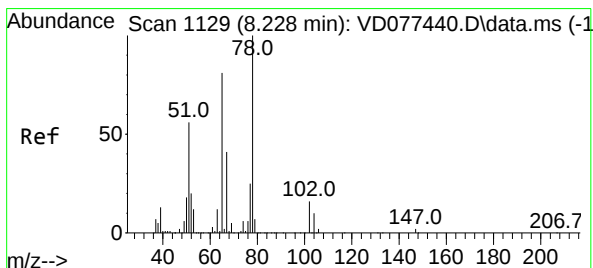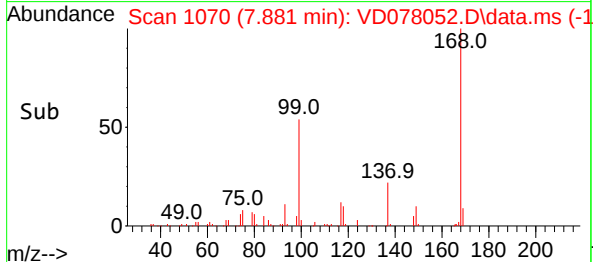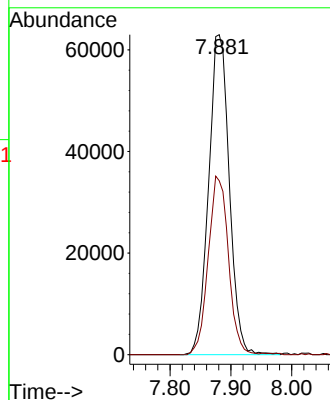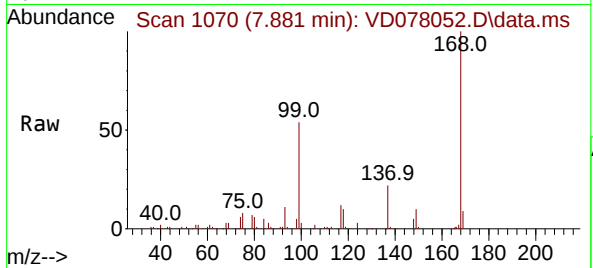

#33
1,2-Dichloroethane-d4
Concen: 42.333 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13

Tgt Ion: 65 Resp: 74114
Ion Ratio Lower Upper
65 100
67 54.8 0.0 115.0

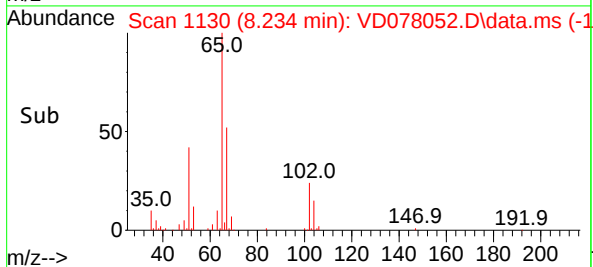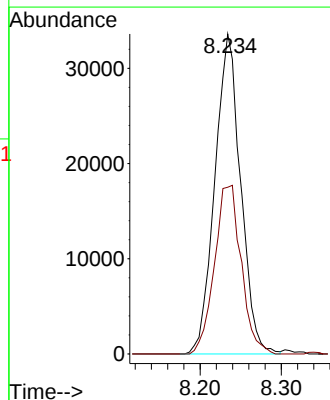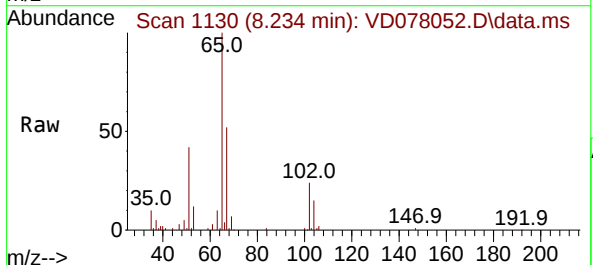

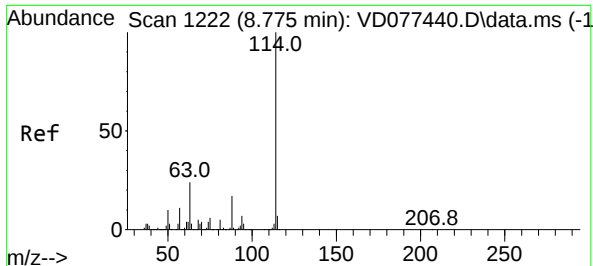

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 11

Delta R.T. 0.006 min

Lab File: VD078052.D

Acq: 22 Dec 2023 05:13

Instrument :

MSVOA_D

ClientSampleId :

COM57




Tgt Ion:114 Resp: 274677

Ion Ratio Lower Upper

114 100

63 17.8 0.0 33.4

88 13.1 0.0 26.2

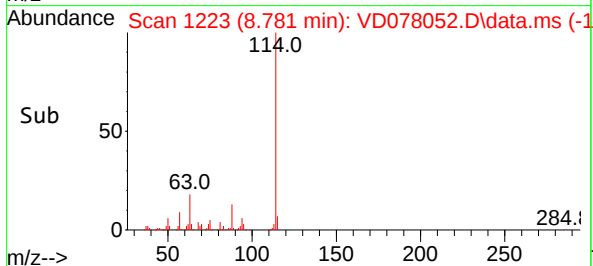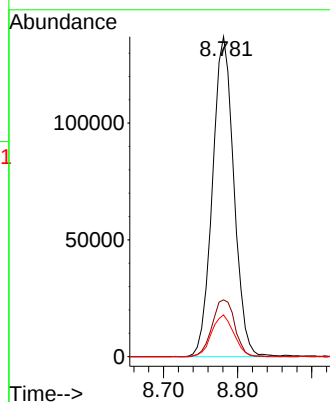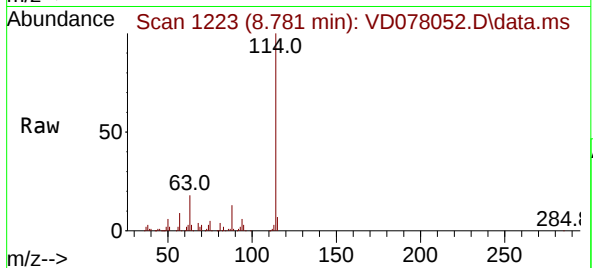

#35

Dibromofluoromethane

Concen: 44.225 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078052.D

Acq: 22 Dec 2023 05:13




Tgt Ion:113 Resp: 85089


Ion Ratio Lower Upper

113 100

111 102.1 84.7 127.1

192 18.2 16.8 25.2


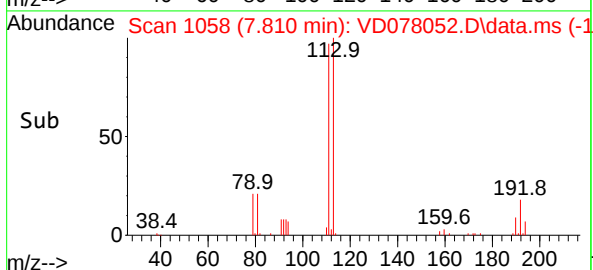
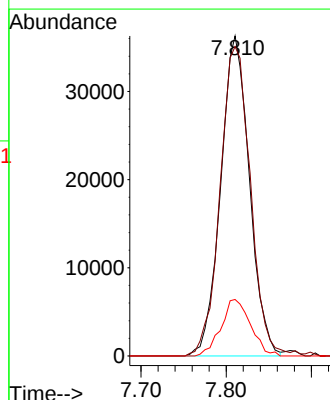
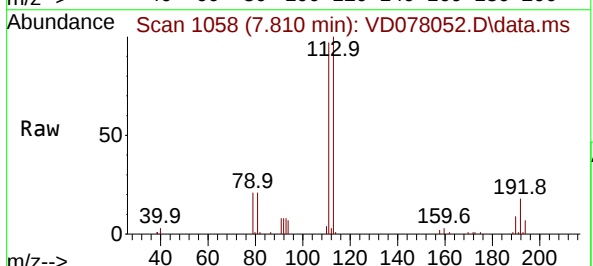


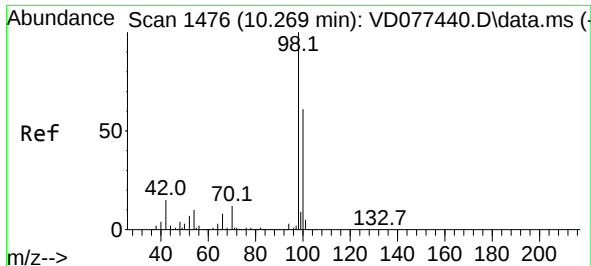

#50
Toluene-d8
Concen: 44.756 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13




Instrument :
MSVOA_D
ClientSampleId :
COM57


Tgt Ion: 98 Resp: 344886
Ion Ratio Lower Upper
98 100
100 64.0 50.3 75.5

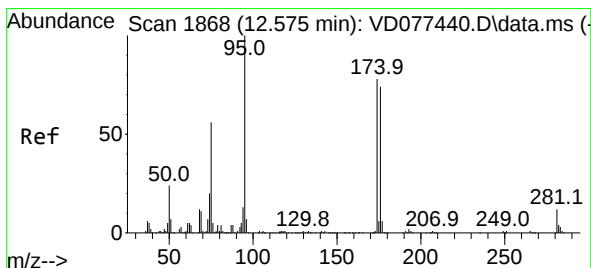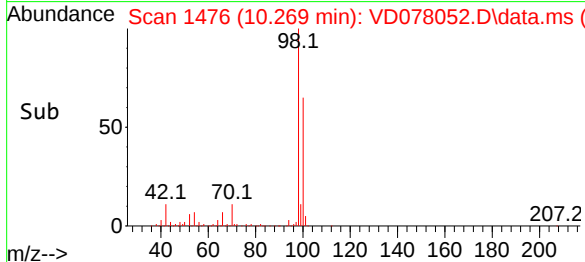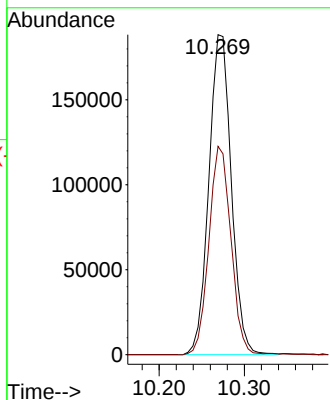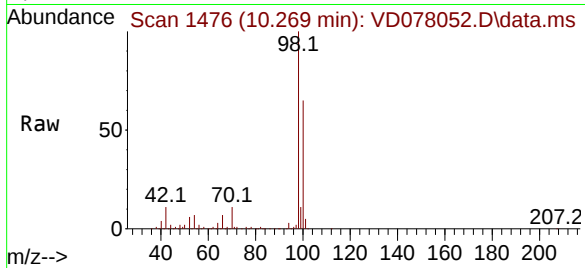

#62
4-Bromofluorobenzene
Concen: 40.415 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13

Tgt Ion: 95 Resp: 93111
Ion Ratio Lower Upper
95 100
174 87.3 0.0 201.8
176 85.0 0.0 191.8


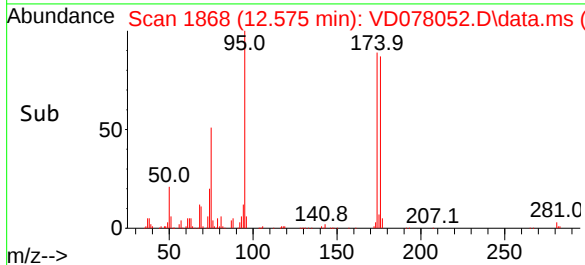
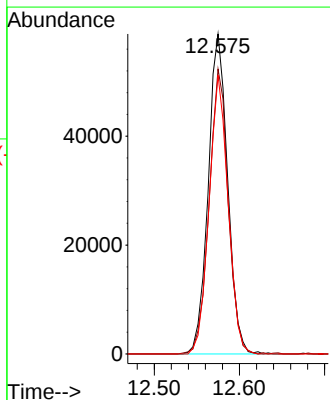
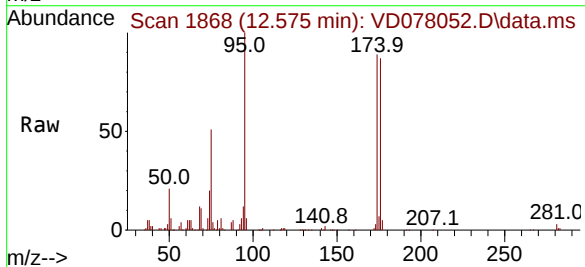


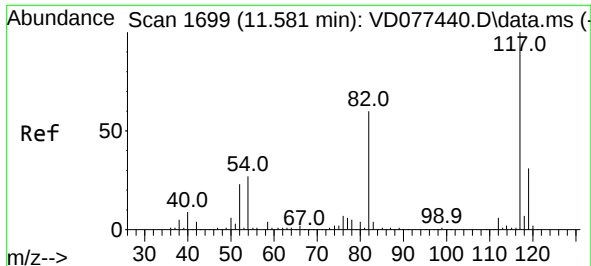

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13

Instrument :
MSVOA_D
ClientSampleId :
COM57

Tgt Ion:117 Resp: 253629
Ion Ratio Lower Upper
117 100
82 52.9 38.3 57.5
119 32.7 25.0 37.4

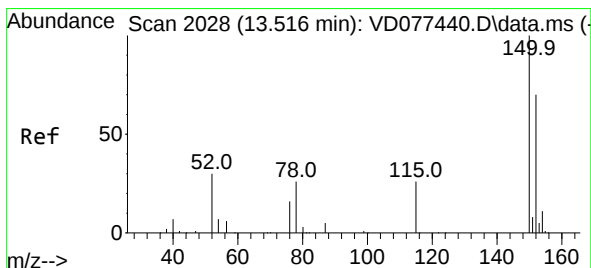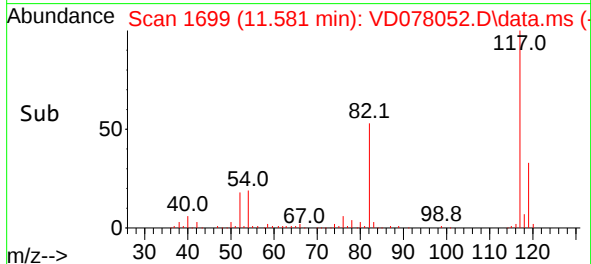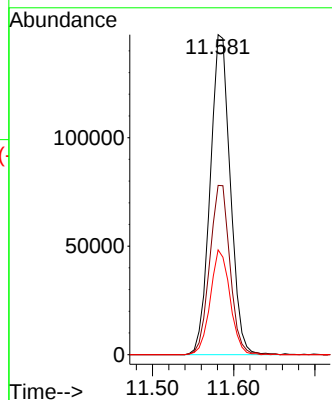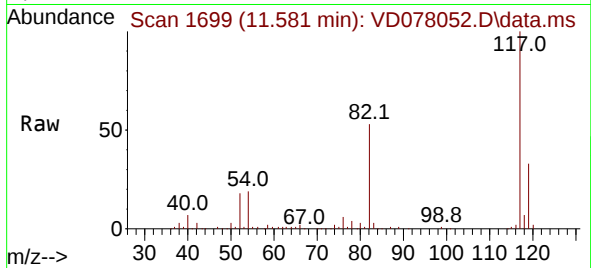

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. 0.006 min
Lab File: VD078052.D
Acq: 22 Dec 2023 05:13

Tgt Ion:152 Resp: 99704
Ion Ratio Lower Upper
152 100
115 57.6 27.1 81.3
150 155.6 0.0 353.6

