
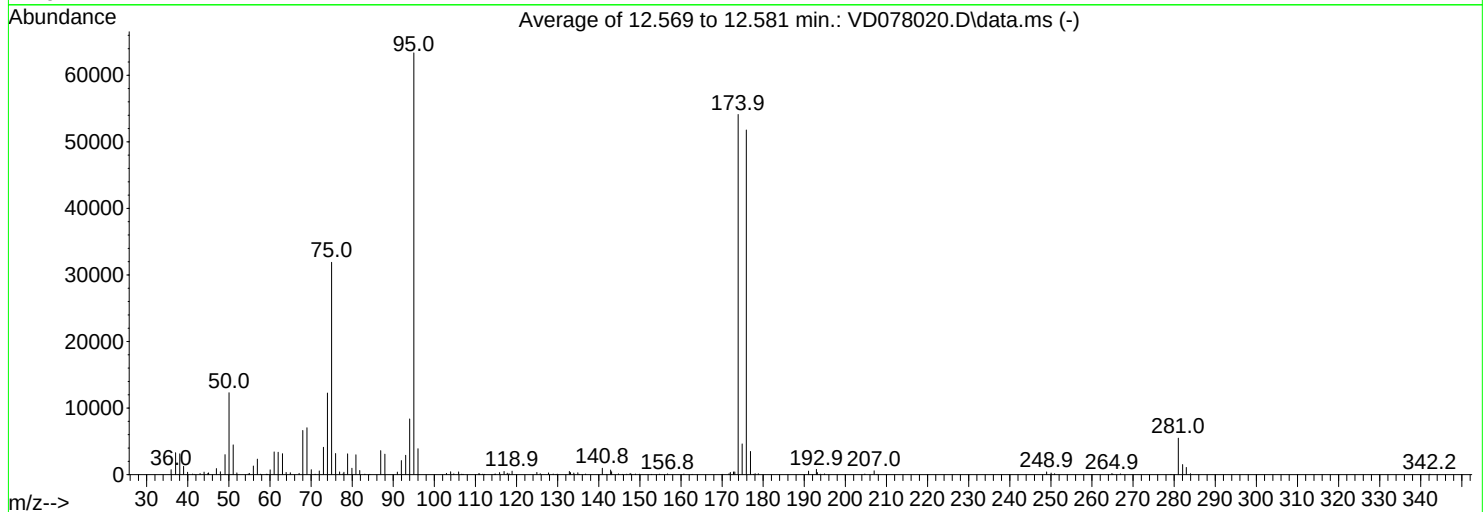


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
Data File : VD078020.D
Acq On : 21 Dec 2023 09:22
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

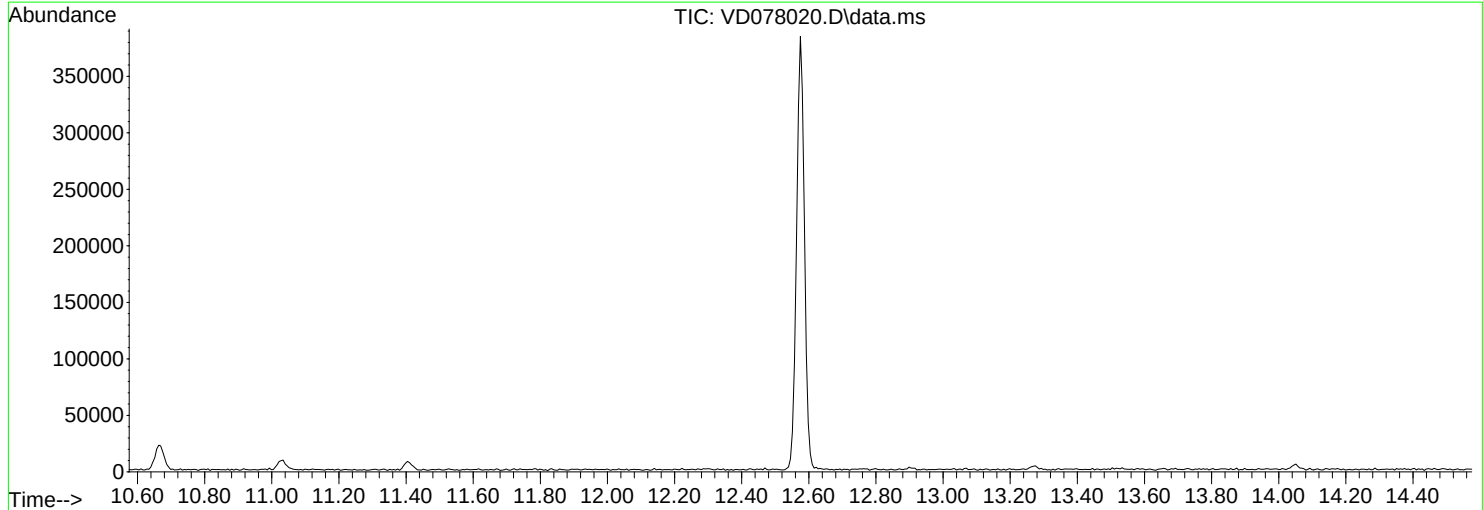

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	12316	PASS
75	95	30	60	50.4	31907	PASS
95	95	100	100	100.0	63368	PASS
96	95	5	9	6.2	3901	PASS
173	174	0.00	2	0.7	404	PASS
174	95	50	100	85.4	54109	PASS
175	174	5	9	8.5	4614	PASS
176	174	95	101	95.7	51779	PASS
177	176	5	9	6.7	3480	PASS