
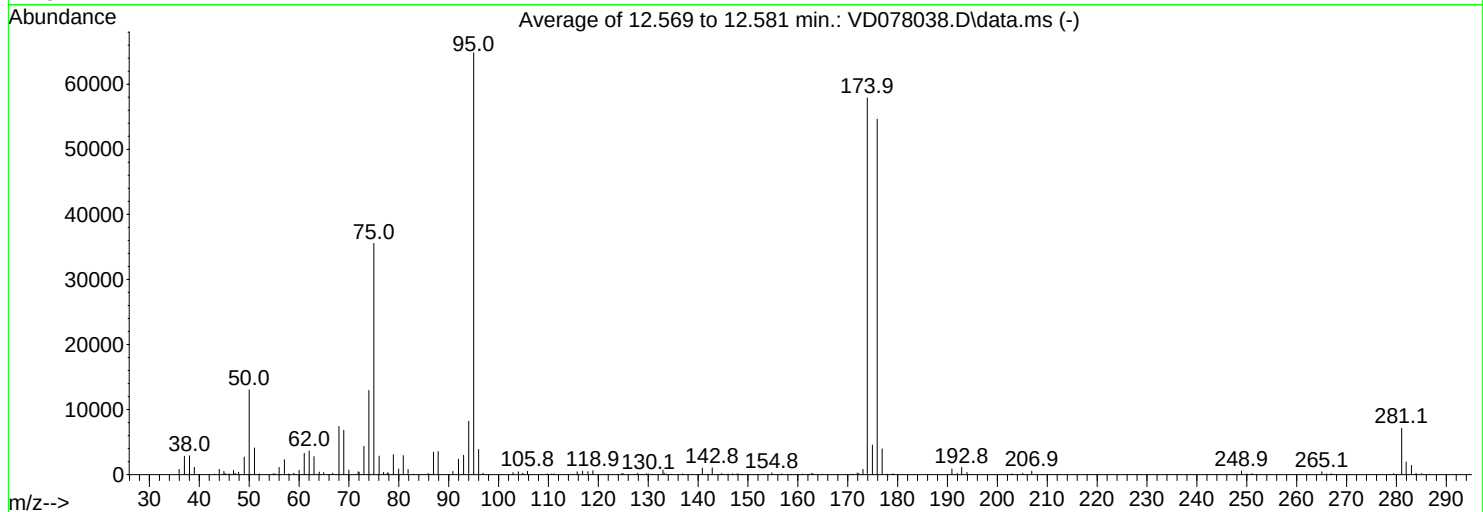


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122123\
Data File : VD078038.D
Acq On : 21 Dec 2023 21:09
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Title : SW846 8260
Last Update : Thu Dec 14 14:48:10 2023

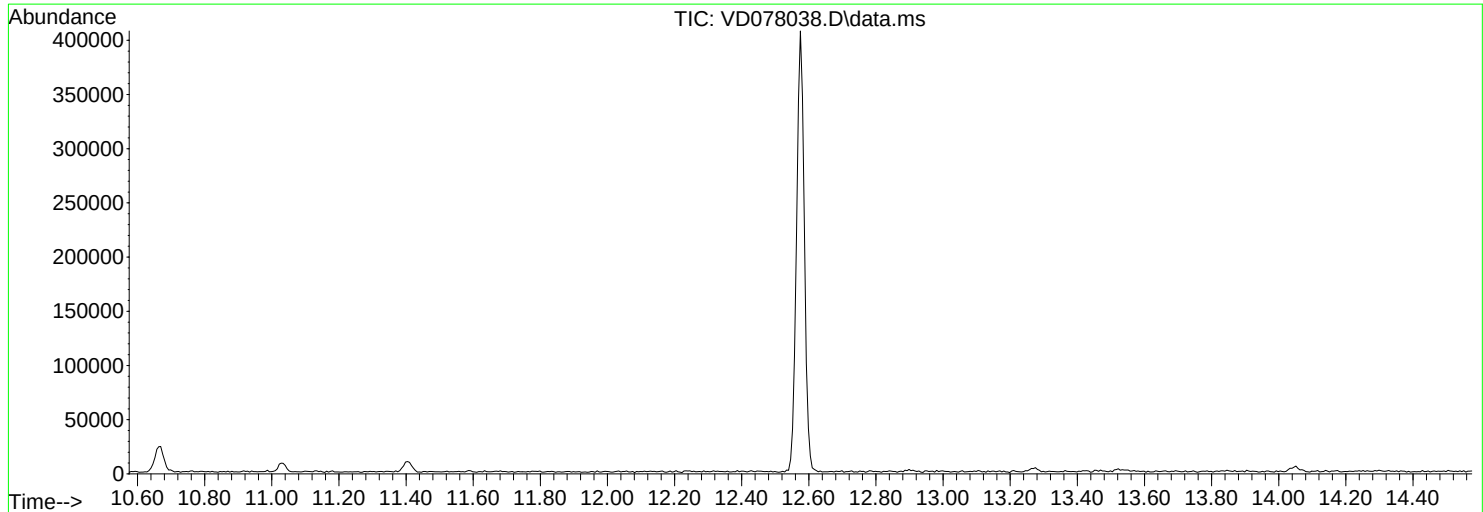

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	13027	PASS
75	95	30	60	54.8	35528	PASS
95	95	100	100	100.0	64829	PASS
96	95	5	9	5.9	3853	PASS
173	174	0.00	2	1.4	813	PASS
174	95	50	100	89.3	57888	PASS
175	174	5	9	7.9	4553	PASS
176	174	95	101	94.4	54648	FAIL*
177	176	5	9	7.2	3959	PASS