


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122218\
 Data File : VD060699.D
 Acq On : 22 Dec 2018 10:06
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA_D/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
 Title : SW846 8260
 Last Update : Fri Dec 21 17:37:47 2018

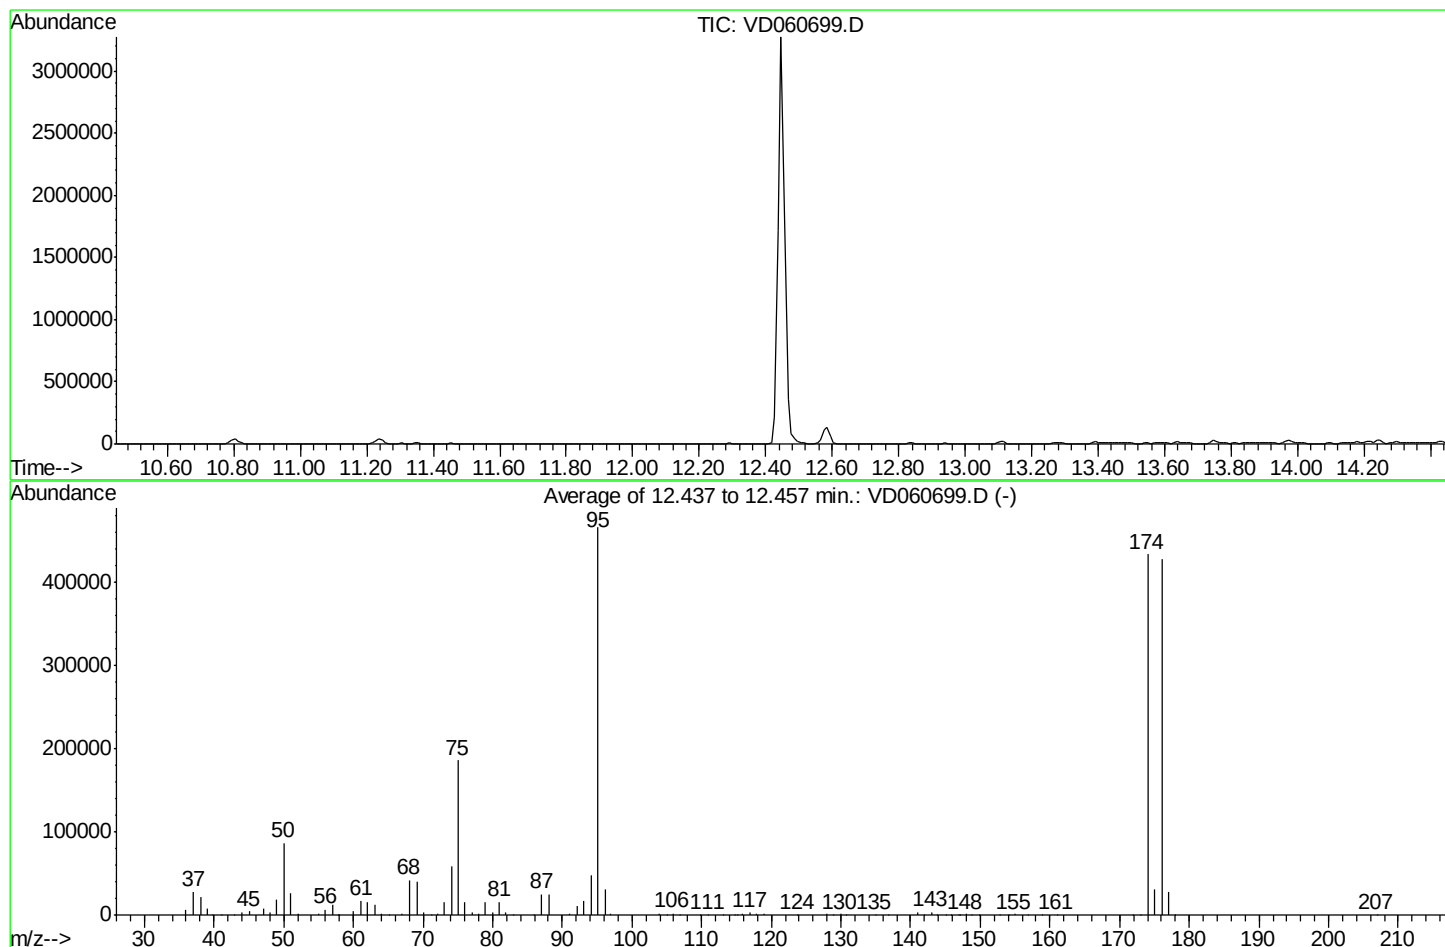

AutoFind: Scans 1139, 1140, 1141; Background Corrected with Scan 1134

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	86789	PASS
75	95	30	60	39.8	185306	PASS
95	95	100	100	100.0	465472	PASS
96	95	5	9	6.5	30456	PASS
173	174	0.00	2	0.1	586	PASS
174	95	50	100	93.0	432896	PASS
175	174	5	9	7.2	31296	PASS
176	174	95	101	98.8	427882	PASS
177	176	5	9	6.4	27405	PASS