
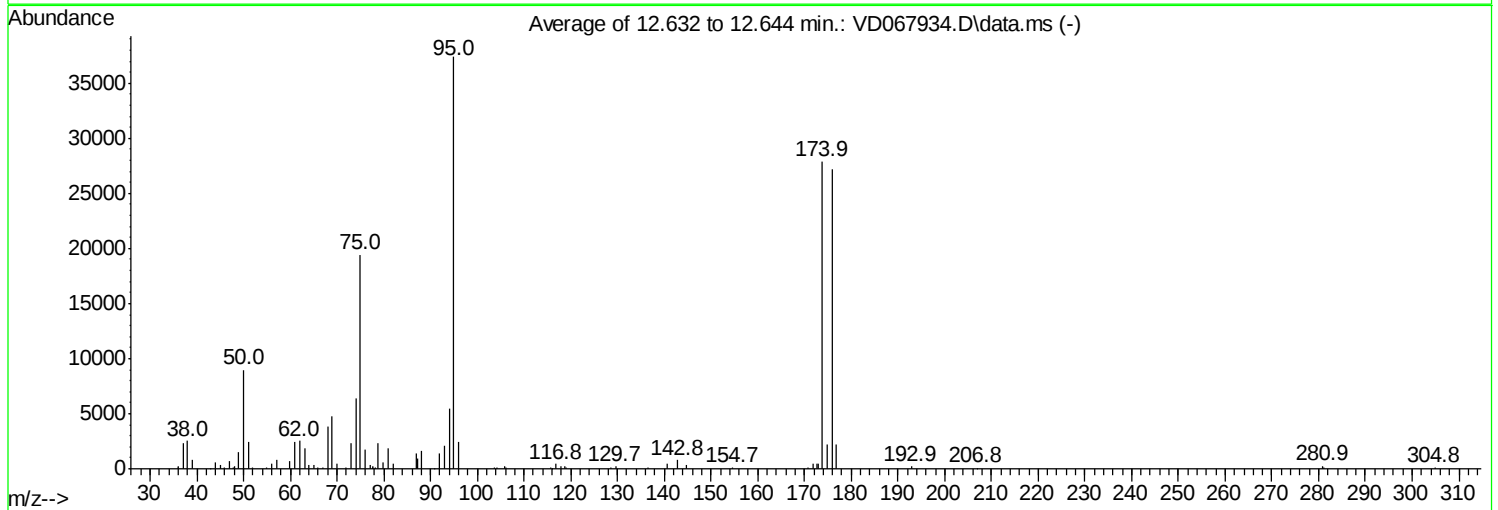


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122220\
 Data File : VD067934.D
 Acq On : 22 Dec 2020 14:11
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122220S.M
 Title : Sw846 8260
 Last Update : Wed Dec 23 07:34:16 2020

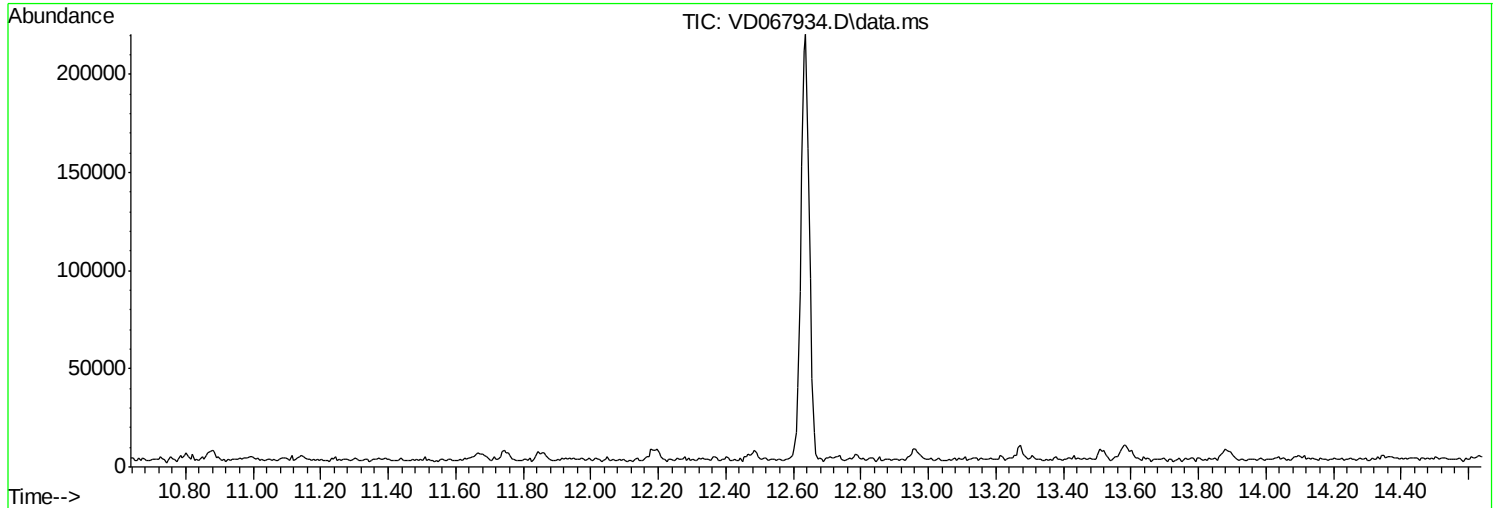

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1813

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	8972	PASS
75	95	30	60	51.9	19423	PASS
95	95	100	100	100.0	37397	PASS
96	95	5	9	6.6	2473	PASS
173	174	0.00	2	1.5	431	PASS
174	95	50	100	74.4	27840	PASS
175	174	5	9	8.0	2219	PASS
176	174	95	101	97.8	27229	PASS
177	176	5	9	8.3	2248	PASS