


Tert butyl alcohol


Response Ratio

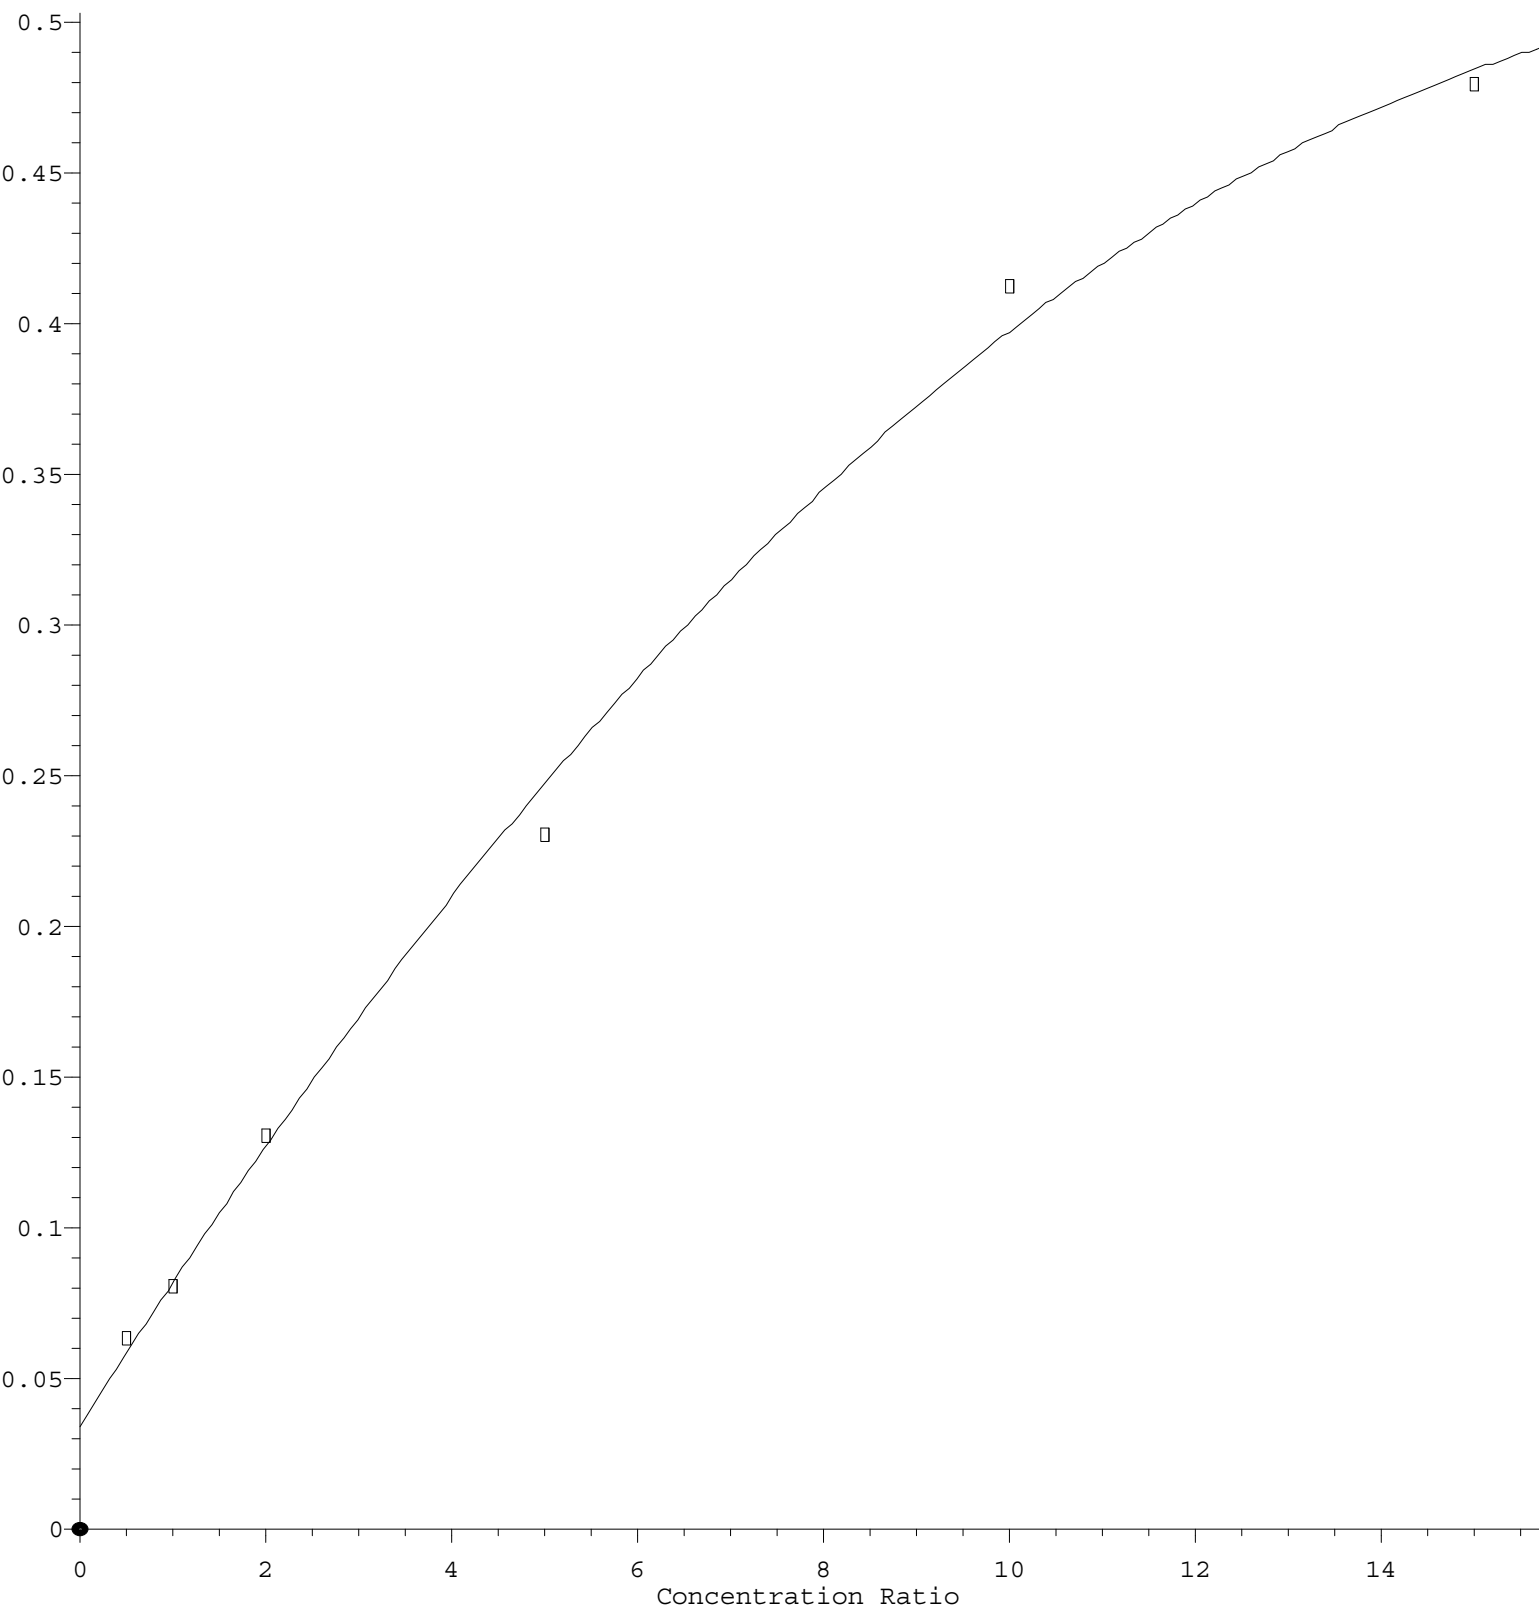

$R = -1.263e-003 A^2 + 4.895e-002 A + 3.429e-002$
 Coef of Det (r^2) = 0.996306 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D122221S.M
 Calibration Table Last Updated: Thu Dec 23 08:20:24 2021

Methylene Chloride

Response Ratio

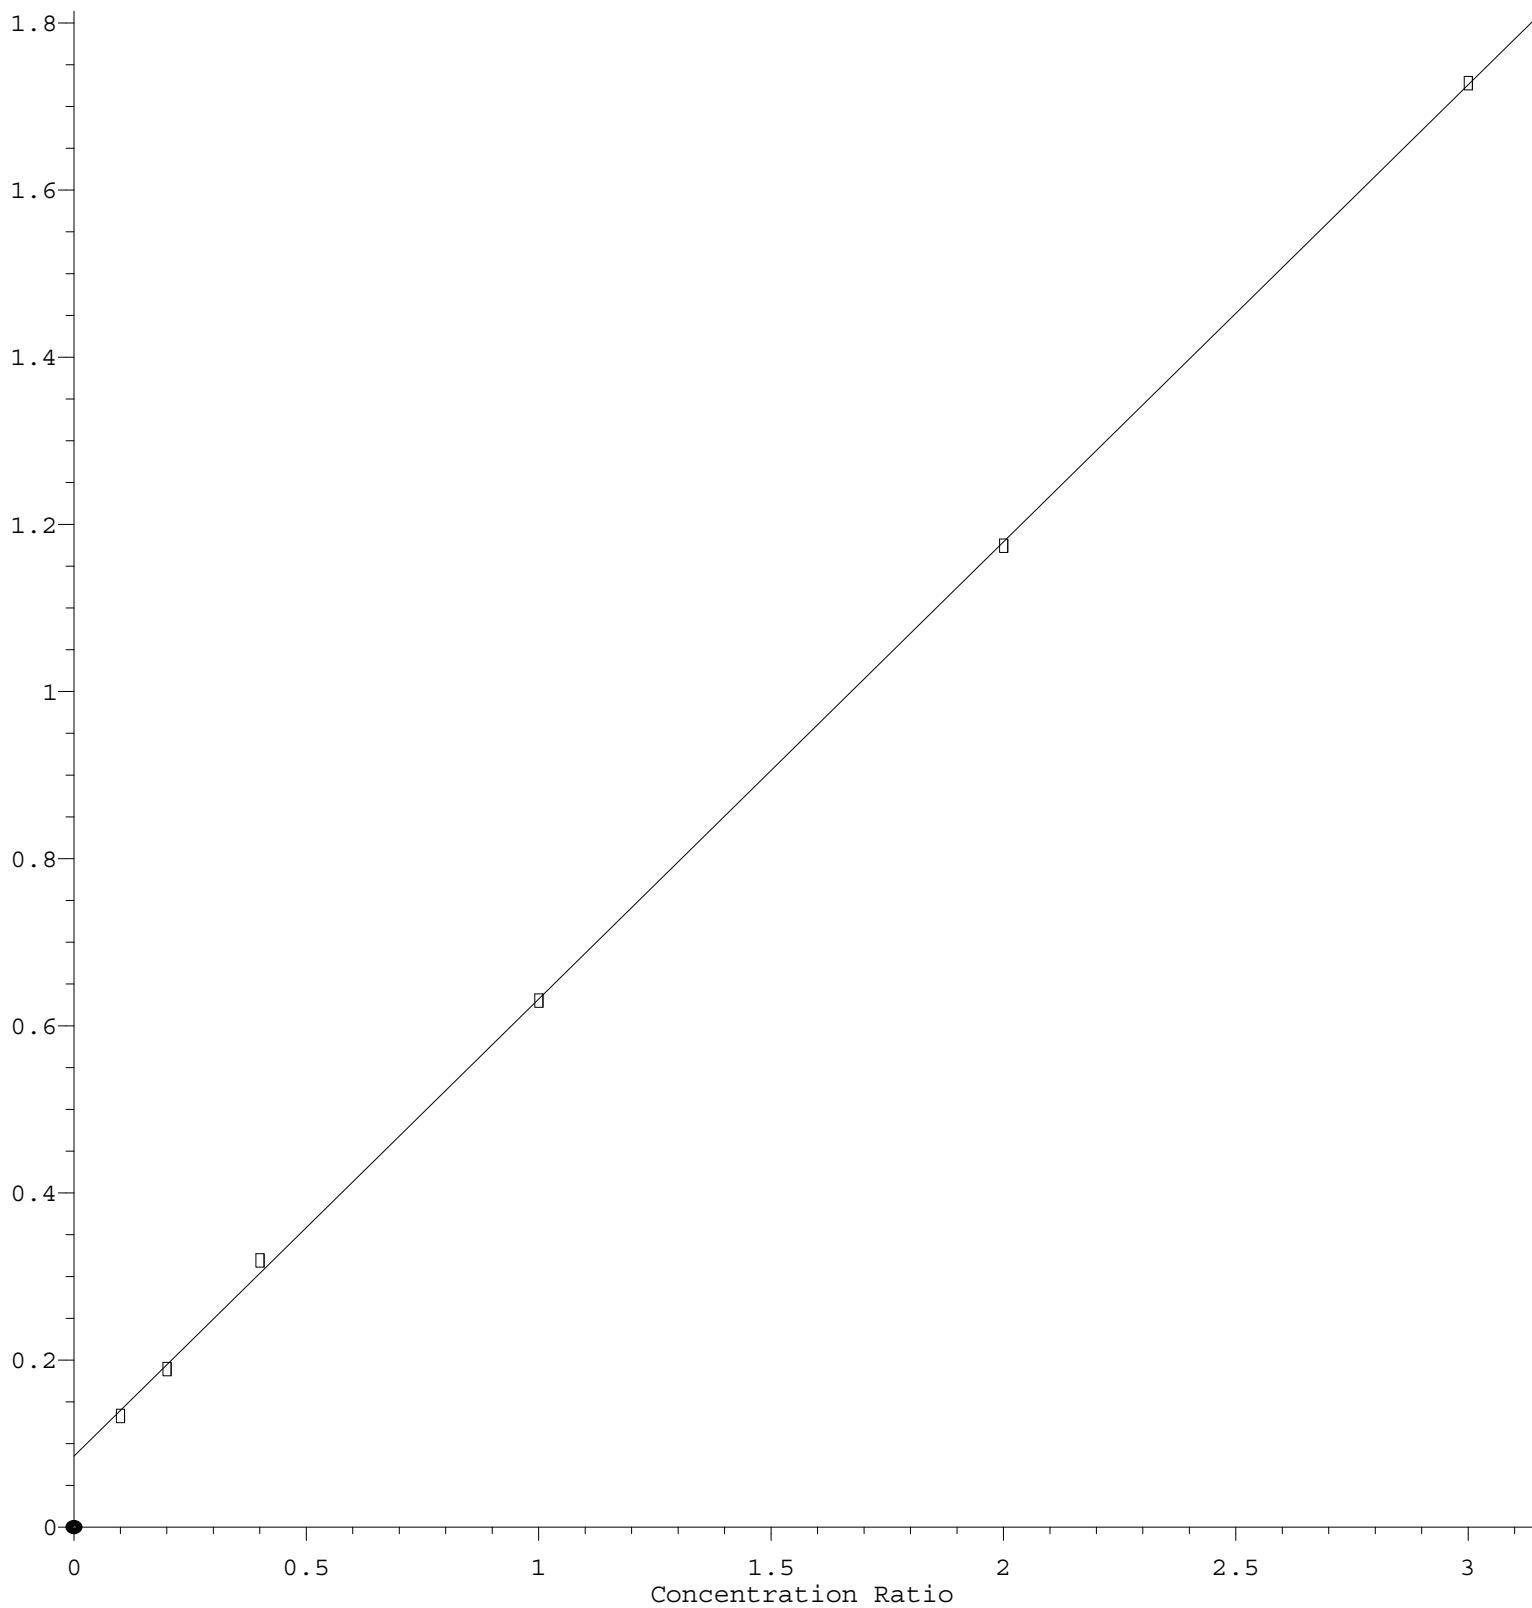

$$\text{Response} = 5.470\text{e-}001 * \text{Amt} + 8.477\text{e-}002$$

Coef of Det (r^2) = 0.999834 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D122221S.M

Calibration Table Last Updated: Thu Dec 23 08:20:24 2021