

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122223\
 Data File : VD078071.D
 Acq On : 22 Dec 2023 18:29
 Operator : RP/MD
 Sample : 05879-12
 Misc : 4.12G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 COM08

Quant Time: Dec 23 03:40:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 14:48:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.881	168	153090	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.781	114	273073	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	245986	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	83387	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	68445	37.942	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	75.880%
35) Dibromofluoromethane	7.810	113	82447	43.103	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	86.200%
50) Toluene-d8	10.269	98	341559	44.584	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	89.160%
62) 4-Bromofluorobenzene	12.575	95	83148	36.302	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	72.600%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122223\
Data File : VD078071.D
Acq On : 22 Dec 2023 18:29
Operator : RP/MD
Sample : 05879-12
Misc : 4.12G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
COM08

Quant Time: Dec 23 03:40:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D120823S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 14:48:10 2023
Response via : Initial Calibration



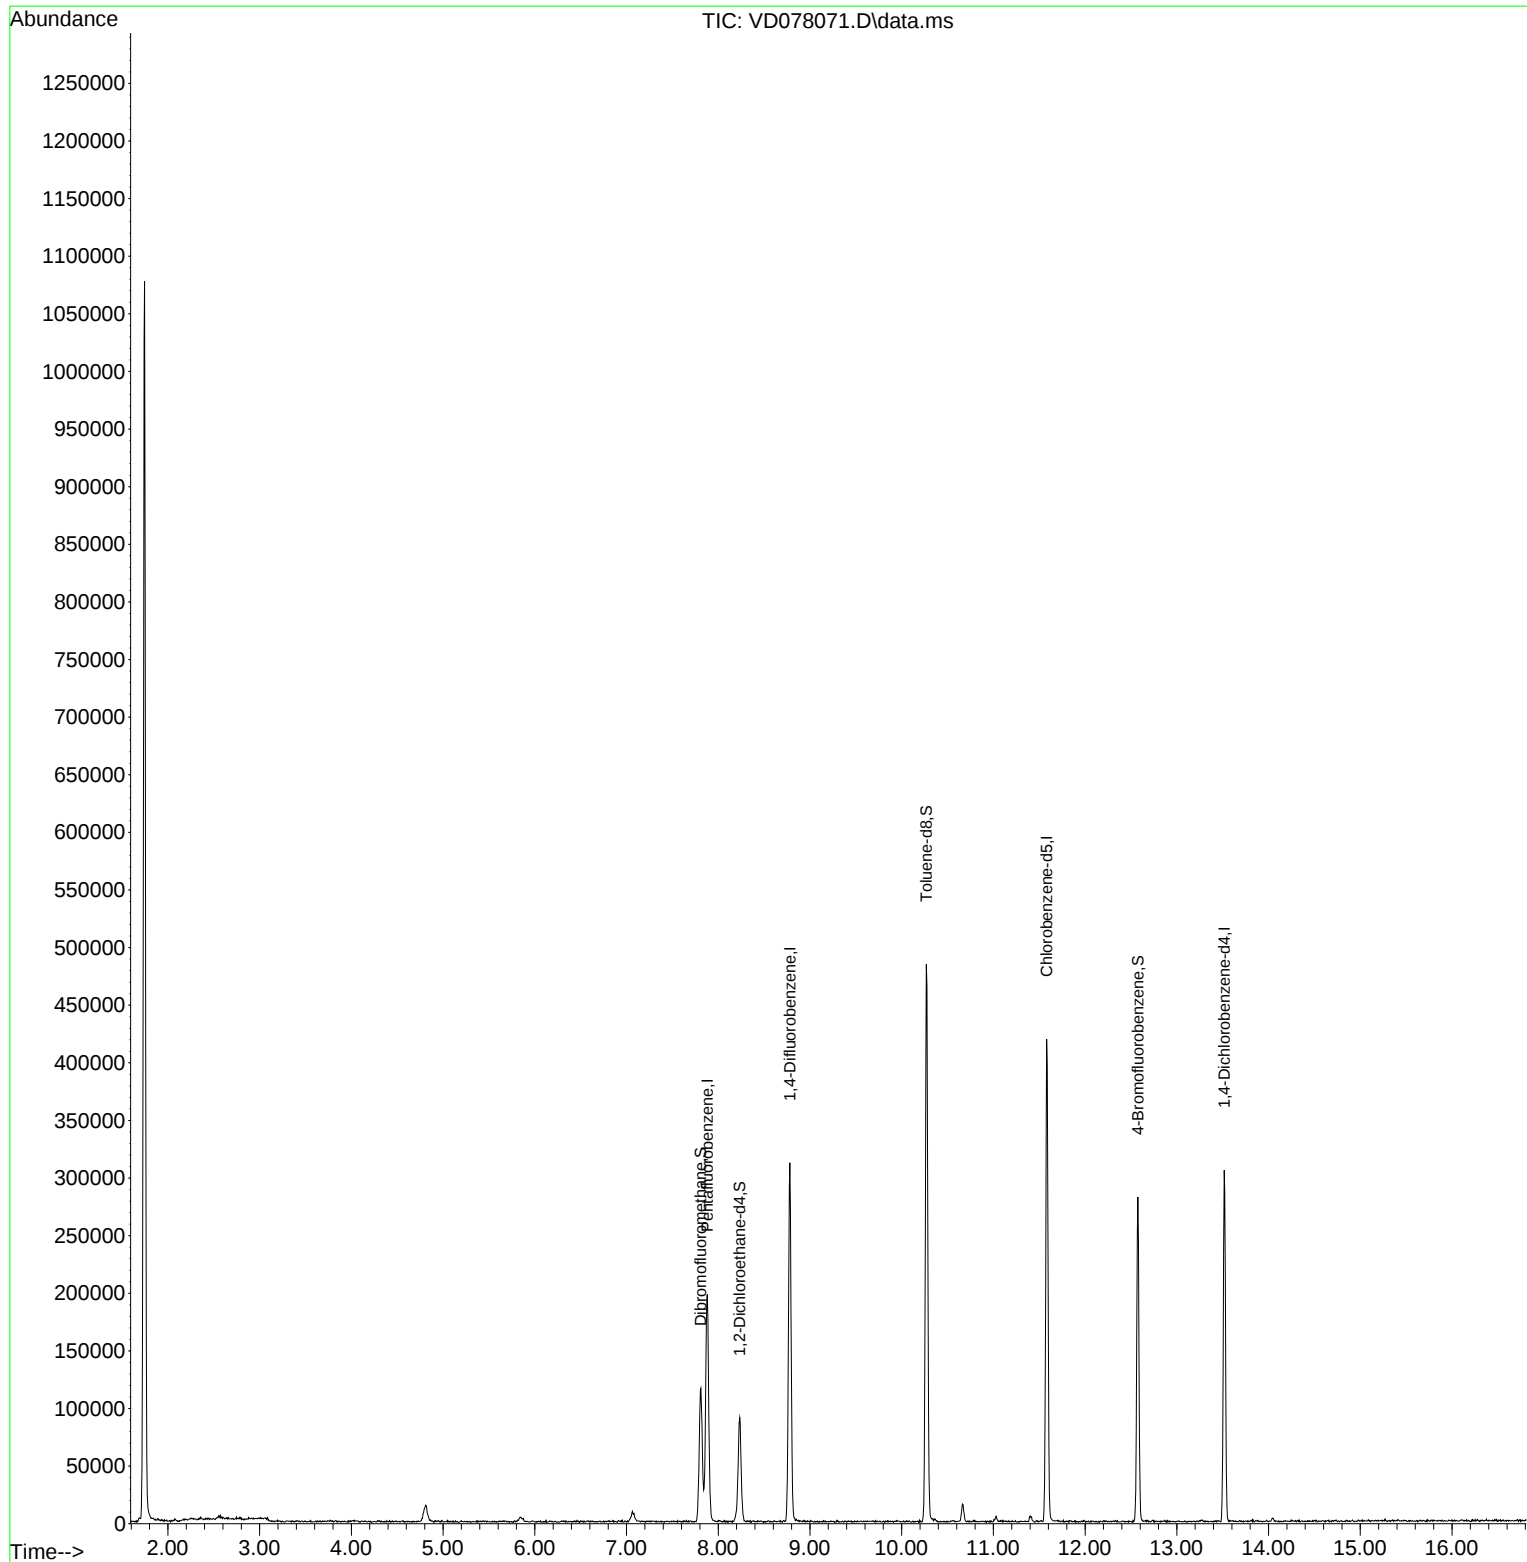


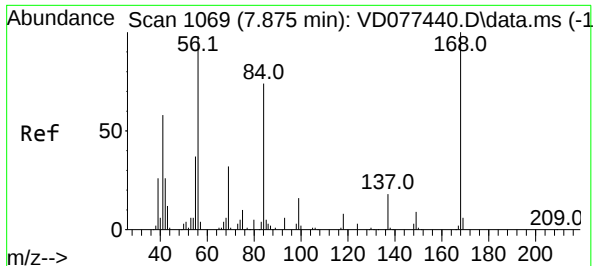

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29




Instrument :
MSVOA_D
ClientSampleId :
COM08


Tgt Ion:168 Resp: 153090
Ion Ratio Lower Upper
168 100
99 52.9 36.7 55.1

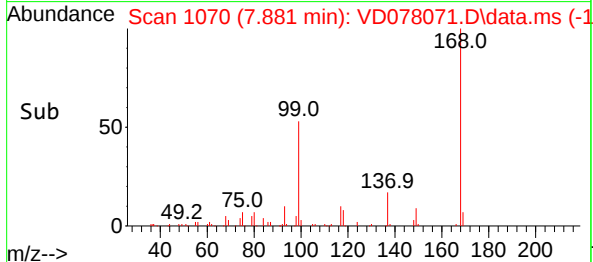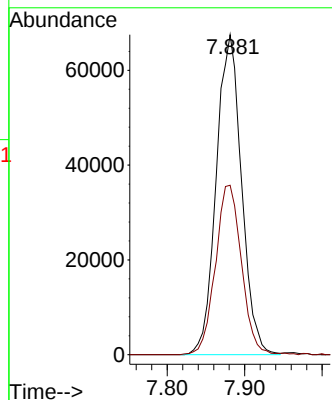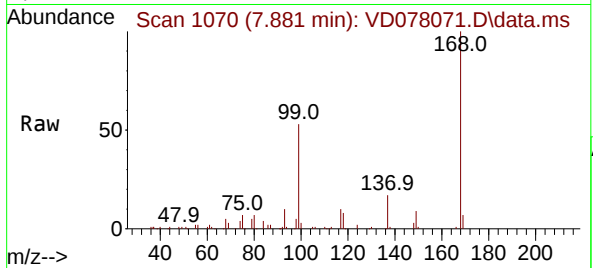

#33
1,2-Dichloroethane-d4
Concen: 37.942 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29

Tgt Ion: 65 Resp: 68445
Ion Ratio Lower Upper
65 100
67 53.0 0.0 115.0

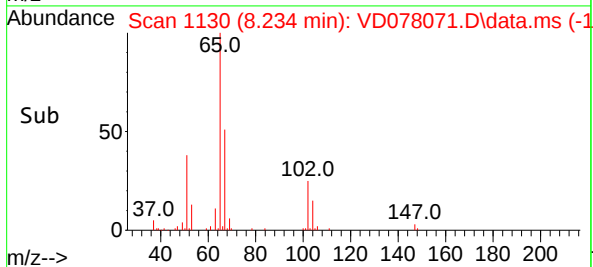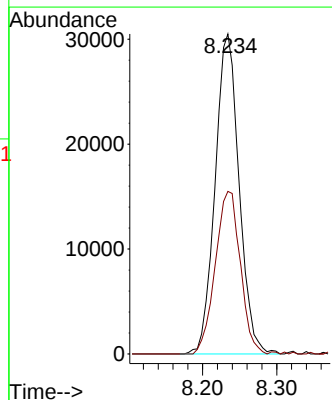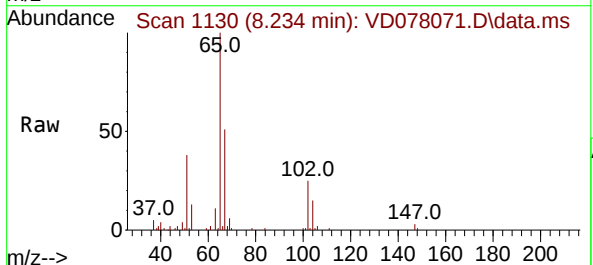

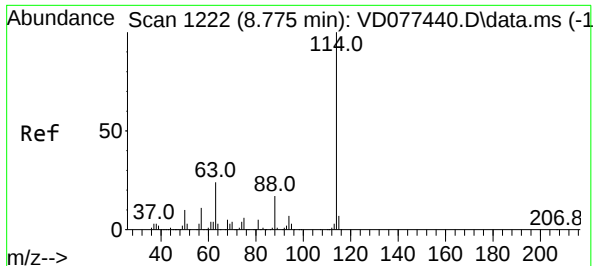

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.781 min Scan# 1

Delta R.T. 0.006 min

Lab File: VD078071.D

Acq: 22 Dec 2023 18:29

Instrument :

MSVOA_D

ClientSampleId :

COM08




Tgt Ion:114 Resp: 273073

Ion Ratio Lower Upper

114 100

63 19.2 0.0 33.4

88 14.3 0.0 26.2

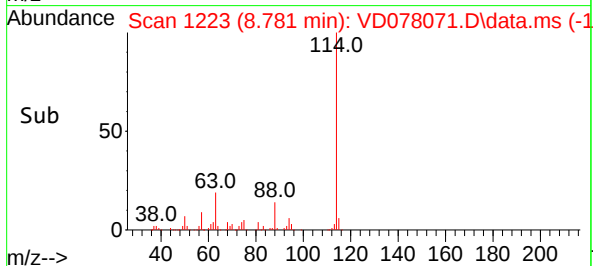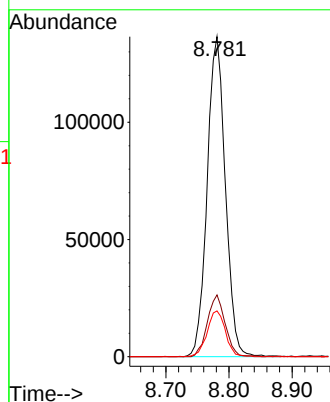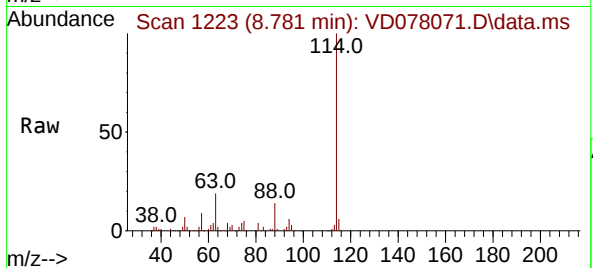

#35

Dibromofluoromethane

Concen: 43.103 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD078071.D

Acq: 22 Dec 2023 18:29




Tgt Ion:113 Resp: 82447

Ion Ratio Lower Upper

113 100

111 103.8 84.7 127.1

192 19.6 16.8 25.2


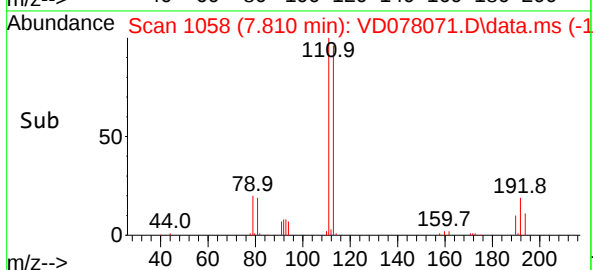
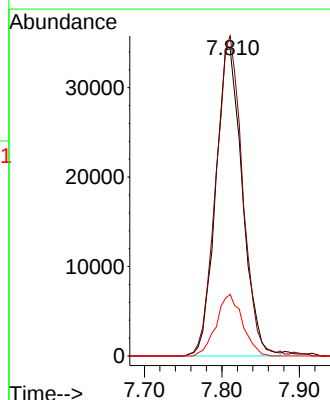
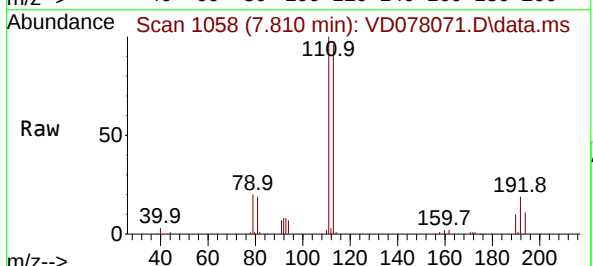




#50
Toluene-d8
Concen: 44.584 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29




Instrument :
MSVOA_D
ClientSampleId :
COM08


Tgt Ion: 98 Resp: 341559
Ion Ratio Lower Upper
98 100
100 63.8 50.3 75.5

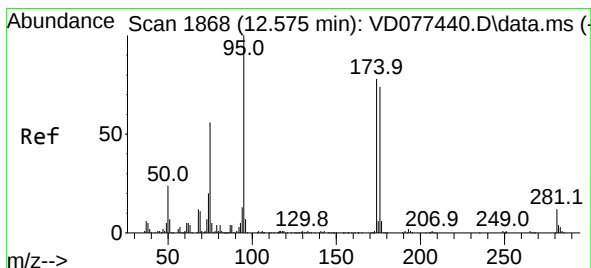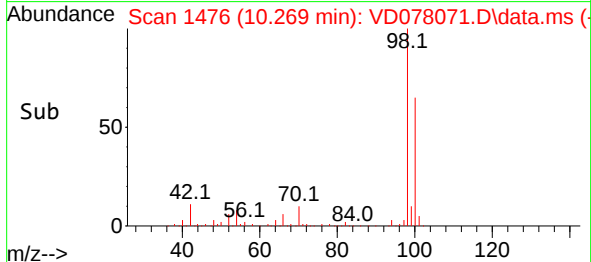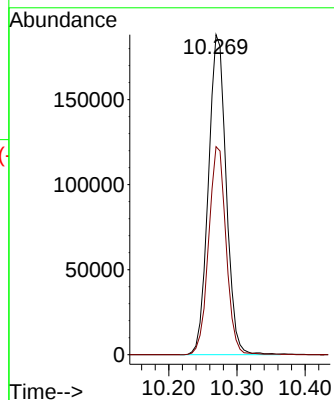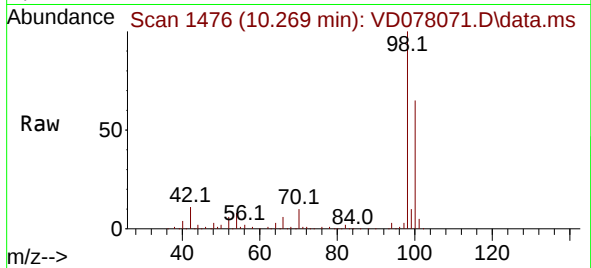

#62
4-Bromofluorobenzene
Concen: 36.302 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29

Tgt Ion: 95 Resp: 83148
Ion Ratio Lower Upper
95 100
174 90.2 0.0 201.8
176 85.1 0.0 191.8


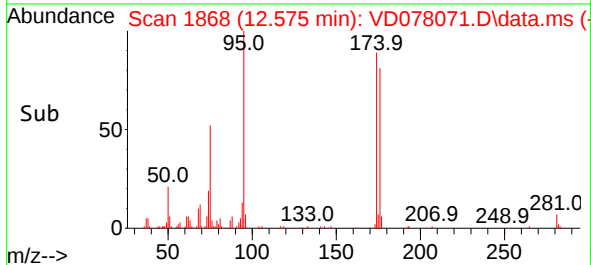
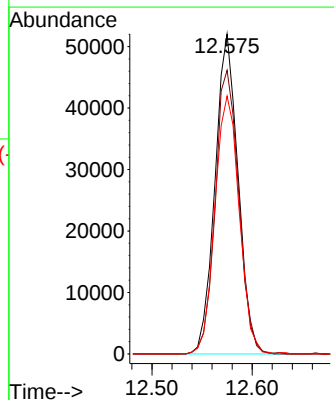
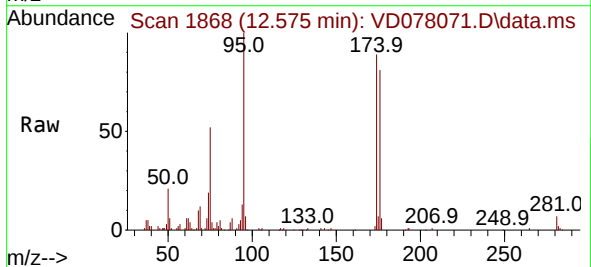


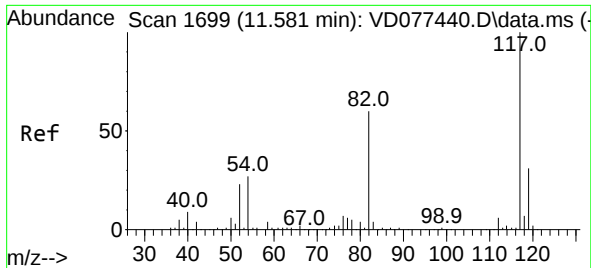

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29

Instrument :
MSVOA_D
ClientSampleId :
COM08

Tgt Ion:117 Resp: 245986
Ion Ratio Lower Upper
117 100
82 52.3 38.3 57.5
119 34.1 25.0 37.4

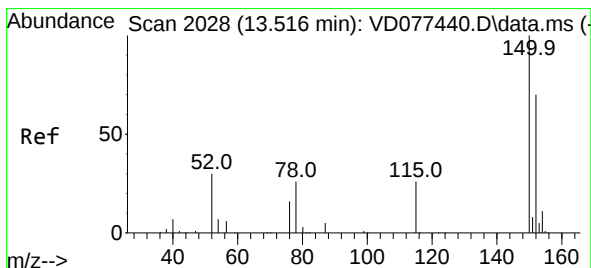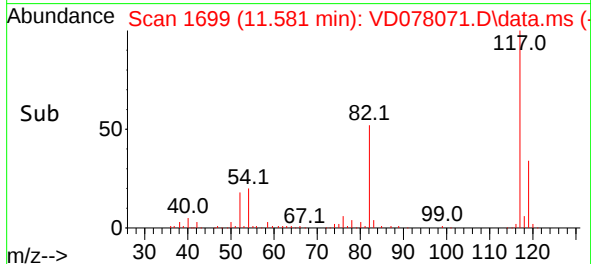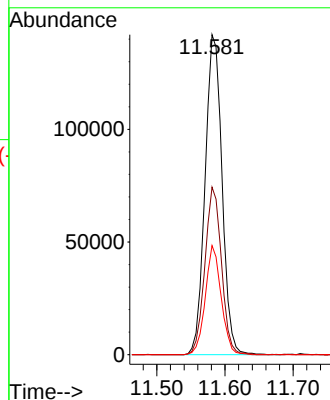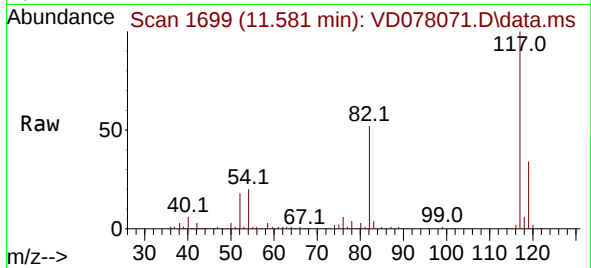

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.000 min
Lab File: VD078071.D
Acq: 22 Dec 2023 18:29

Tgt Ion:152 Resp: 83387
Ion Ratio Lower Upper
152 100
115 54.6 27.1 81.3
150 153.7 0.0 353.6

