
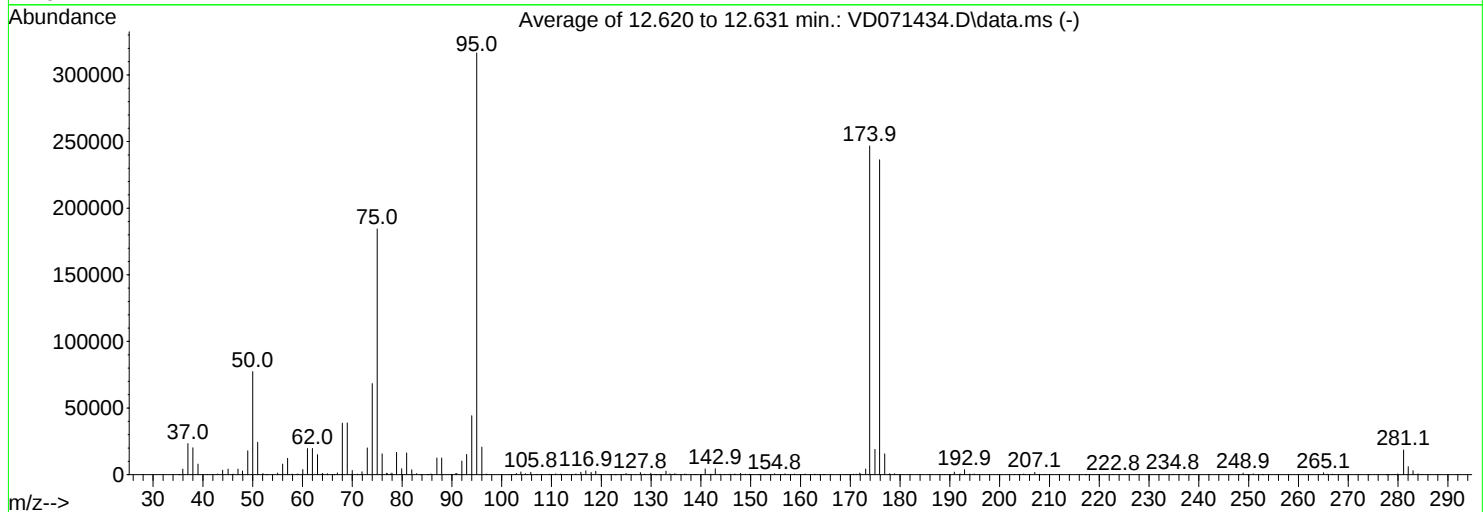


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD122321\  
 Data File : VD071434.D  
 Acq On : 23 Dec 2021 09:47  
 Operator : VA/SY  
 Sample : BFB  
 Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D122221S.M  
 Title : SW846 8260  
 Last Update : Thu Dec 23 08:20:24 2021

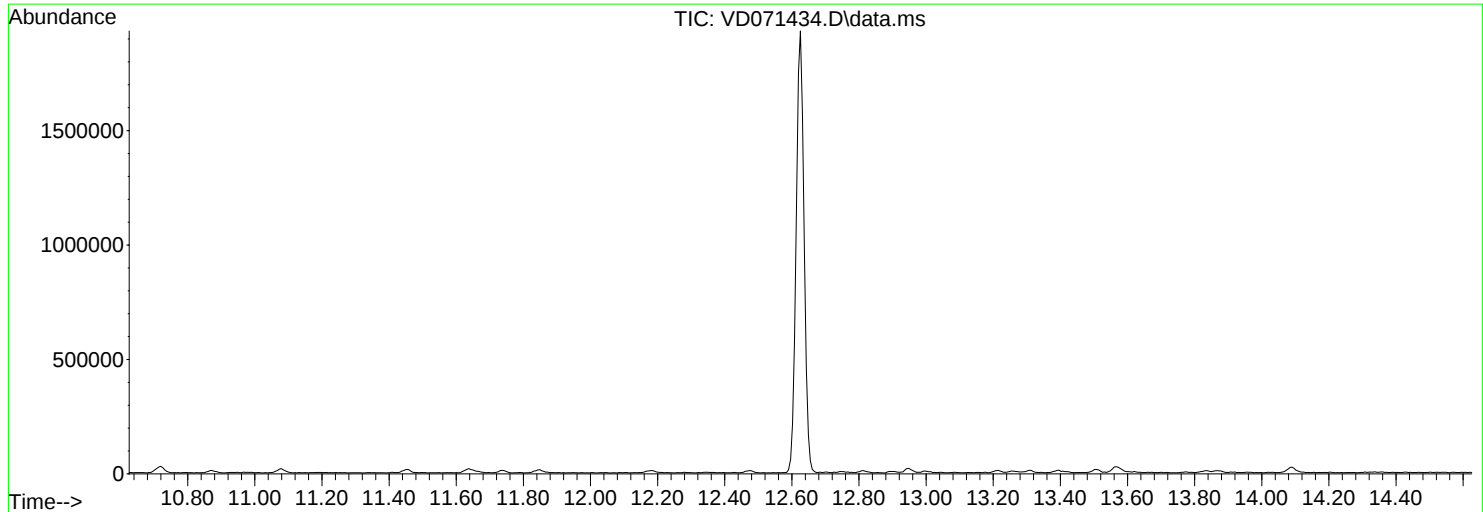

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 24.4         | 77371      | PASS                |
| 75             | 95              | 30              | 60              | 58.3         | 184533     | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 316608     | PASS                |
| 96             | 95              | 5               | 9               | 6.5          | 20685      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.7          | 4168       | PASS                |
| 174            | 95              | 50              | 100             | 77.9         | 246677     | PASS                |
| 175            | 174             | 5               | 9               | 7.7          | 19005      | PASS                |
| 176            | 174             | 95              | 101             | 95.8         | 236309     | PASS                |
| 177            | 176             | 5               | 9               | 6.6          | 15639      | PASS                |