

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122618\
 Data File : VD060715.D
 Acq On : 26 Dec 2018 15:11
 Operator : VA/AP
 Sample : J6579-01
 Misc : 5.92g/5ml/MSVOA D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TN-122618-C

Quant Time: Dec 27 02:48:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 21 17:37:47 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.40	168	1498705	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	7.42	114	2049264	50.00	ug/l	-0.02
63) Chlorobenzene-d5	11.27	117	1593579	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.36	152	700471	50.00	ug/l	-0.02
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.77	65	541506	52.28	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	104.56%	
35) Dibromofluoromethane	6.31	113	718482	47.90	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	95.80%	
50) Toluene-d8	9.43	98	1911128	42.70	ug/l	-0.03
Spiked Amount 50.000			Recovery	=	85.40%	
62) 4-Bromofluorobenzene	12.41	95	626644	39.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	79.96%	
Target Compounds						
16) Acetone	3.16	43	27244	15.063	ug/l #	90
20) Methylene Chloride	3.72	84	129428	6.890	ug/l	93
52) Toluene	9.53	92	151662	4.438	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD122618\
Data File : VD060715.D
Acq On : 26 Dec 2018 15:11
Operator : VA/AP
Sample : J6579-01
Misc : 5.92g/5ml/MSVOA D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TN-122618-C

Quant Time: Dec 27 02:48:56 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
Quant Title : SW846 8260
QLast Update : Fri Dec 21 17:37:47 2018
Response via : Initial Calibration

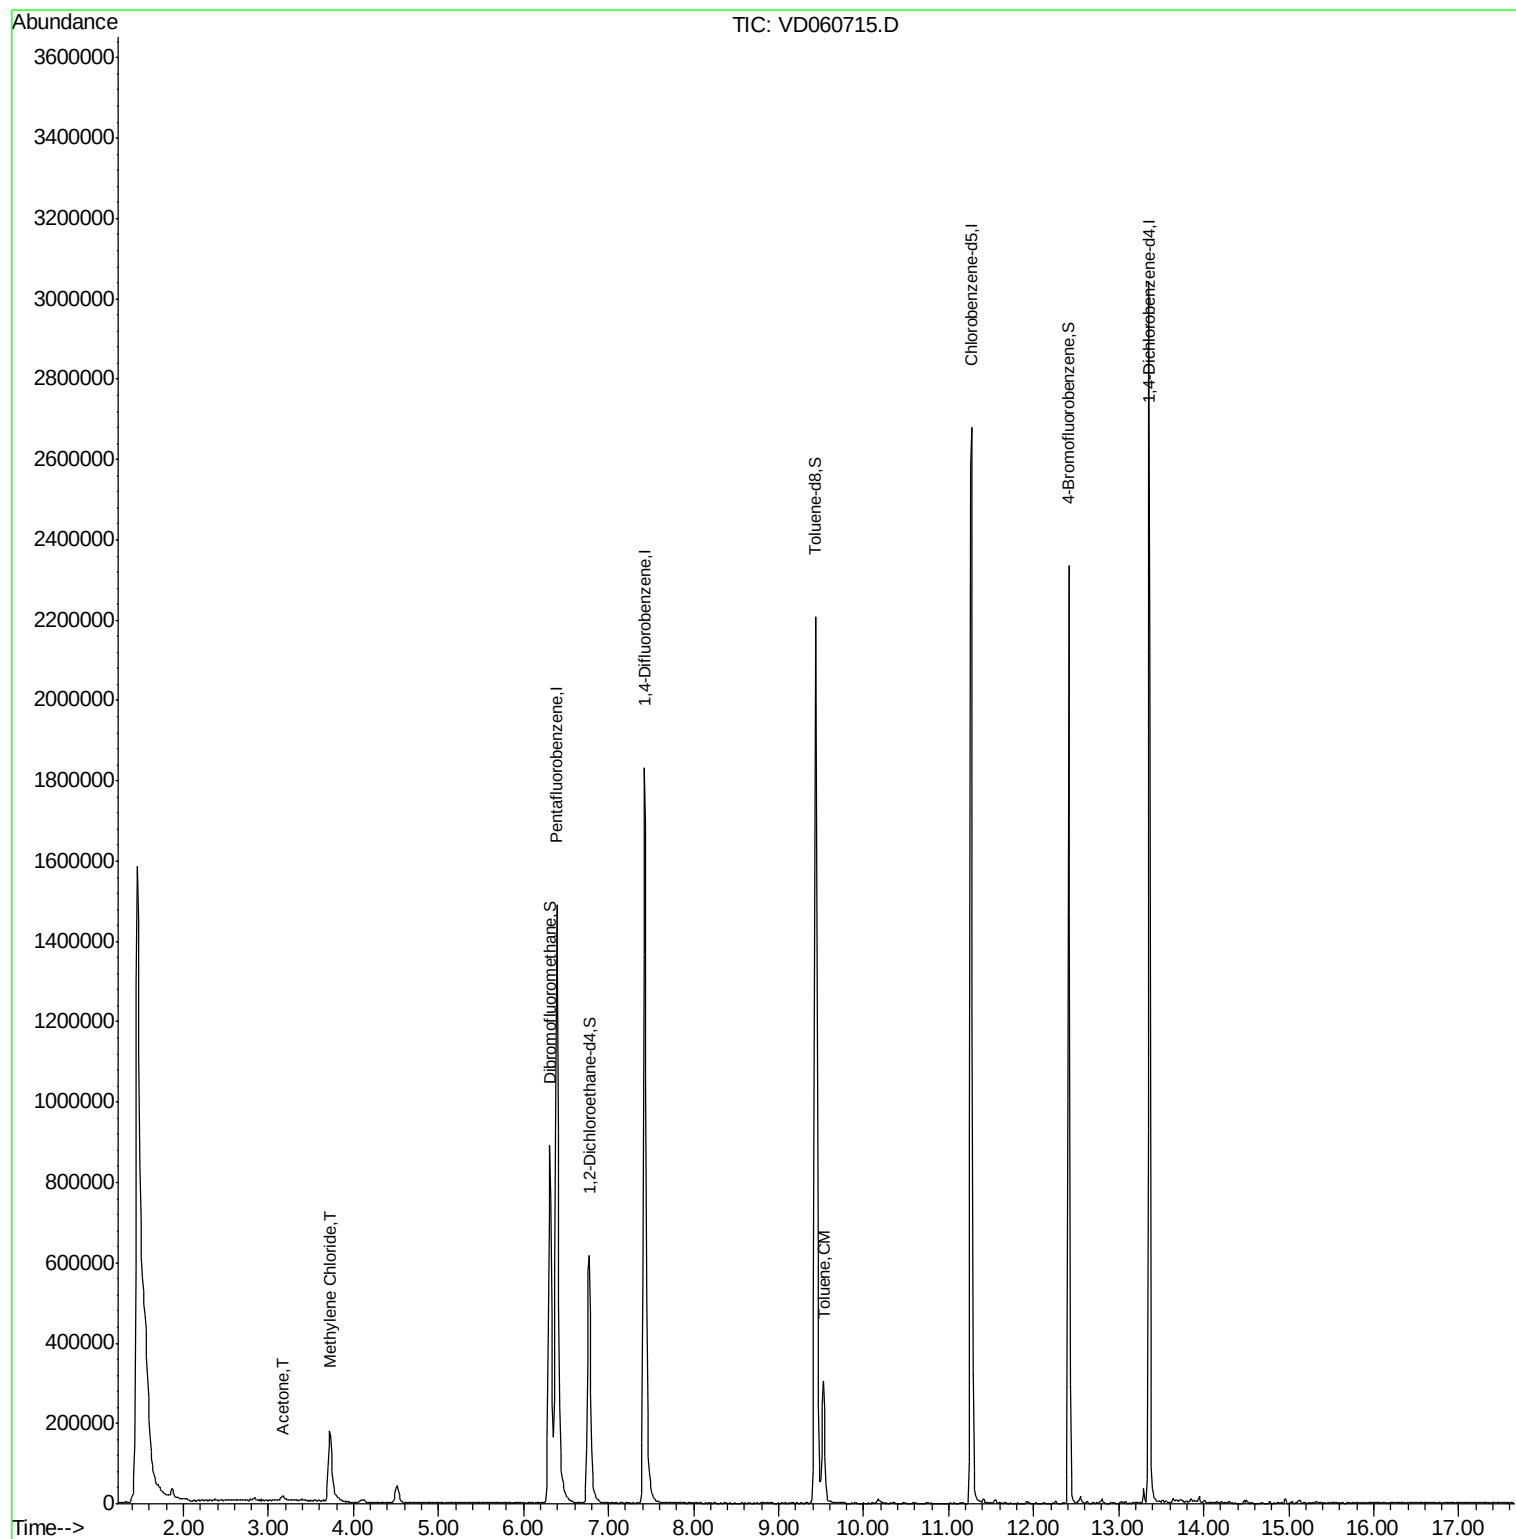

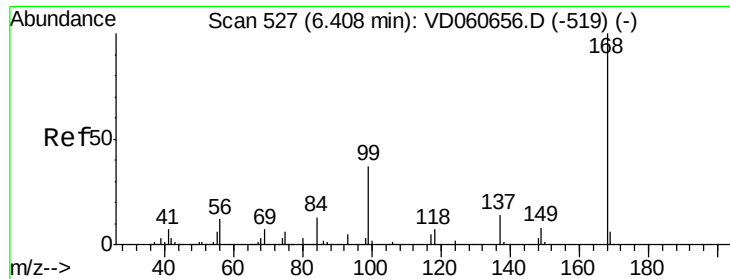

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 6.40 min Scan# 526

Delta R.T. -0.01 min

Lab File: VD060715.D

Acq: 26 Dec 2018 15:11

Instrument :

MSVOA_D

ClientSampleId :


TN-122618-C

Tot Ion:168 Resp: 1498705

Ion Ratio Lower Upper

168 100

99 45.1 38.7 58.1

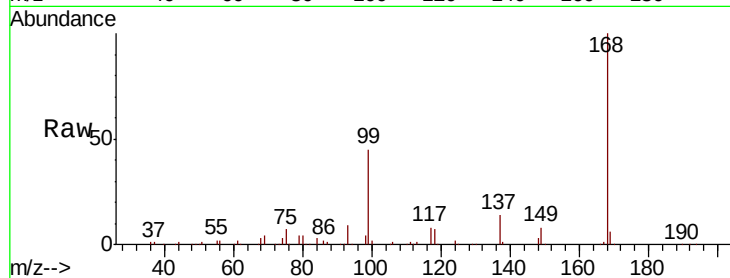

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

6.40

500000

400000



300000

200000

100000

0

Time--> 6.20 6.30 6.40 6.50 6.60

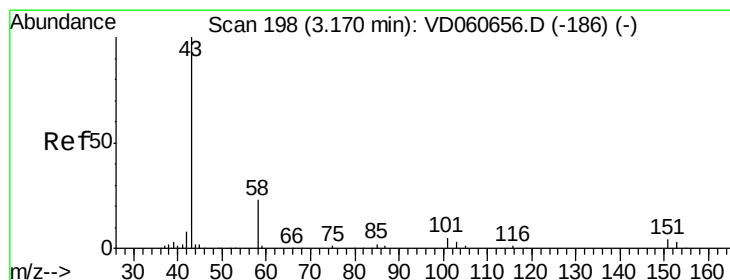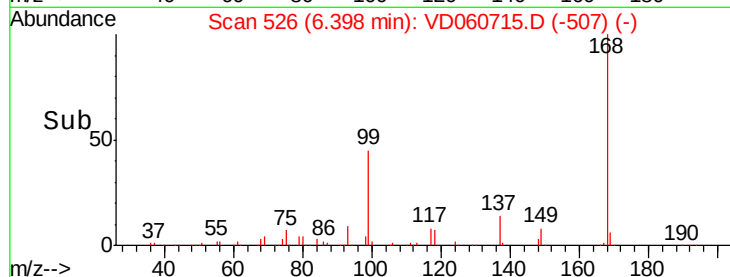

#16

Acetone

Concen: 15.063 ug/l

RT: 3.16 min Scan# 197

Delta R.T. -0.01 min

Lab File: VD060715.D


Acq: 26 Dec 2018 15:11

Tgt Ion: 43 Resp: 27244

Ion Ratio Lower Upper

43 100

58 17.8 18.2 27.2#

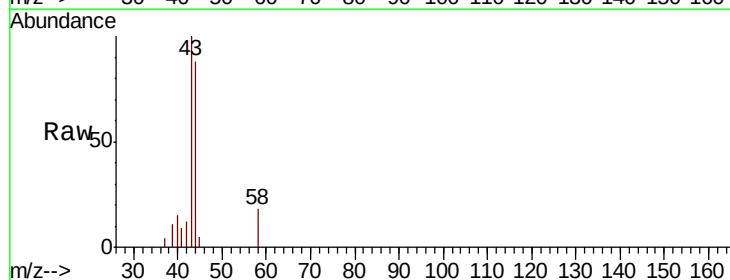

Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC

8000


6000


4000

2000

0

Time--> 3.10 3.20 3.30

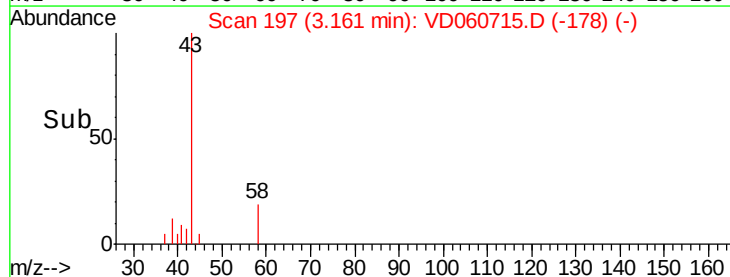

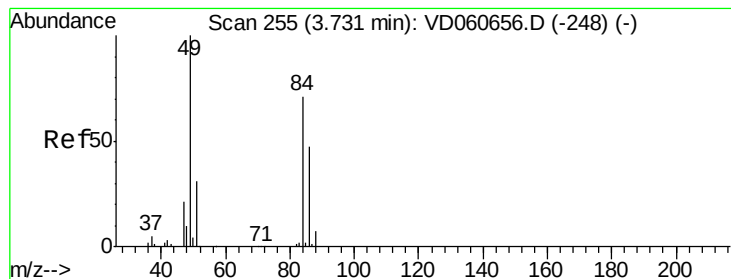

#20

Methylene Chloride

Concen: 6.890 ug/l

RT: 3.72 min Scan# 254

Delta R.T. -0.01 min

Lab File: VD060715.D

Acq: 26 Dec 2018 15:11

Instrument :

MSVOA_D

ClientSampleId :

TN-122618-C

Tot Ion: 84 Resp: 129428


Ion Ratio Lower Upper

84 100

49 156.3 113.6 170.4

51 44.2 34.7 52.1

86 67.9 52.8 79.2



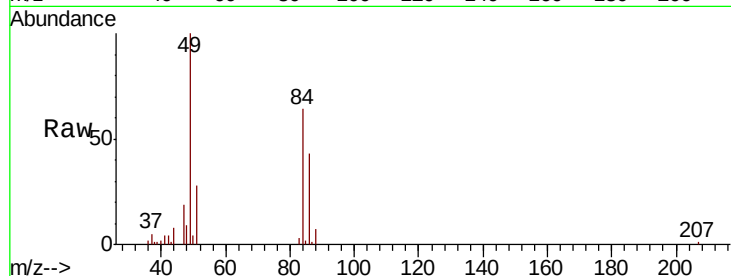


Abundance Ion 83.95 (83.65 to 84.65): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC

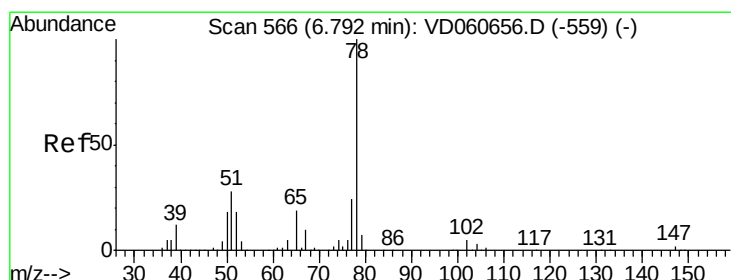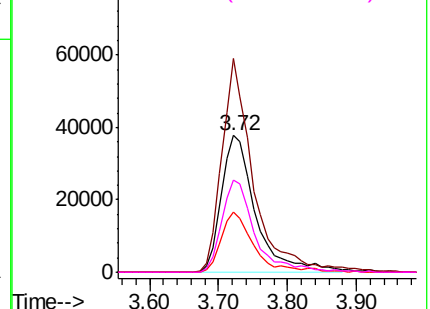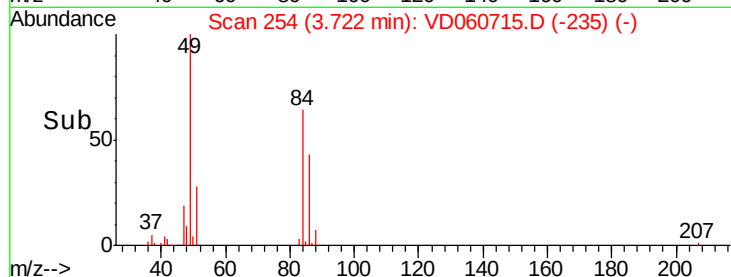

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 6.77 min Scan# 564

Delta R.T. -0.02 min

Lab File: VD060715.D


Acq: 26 Dec 2018 15:11

Tgt Ion: 65 Resp: 541506

Ion Ratio Lower Upper



65 100


67 51.0 0.0 105.4

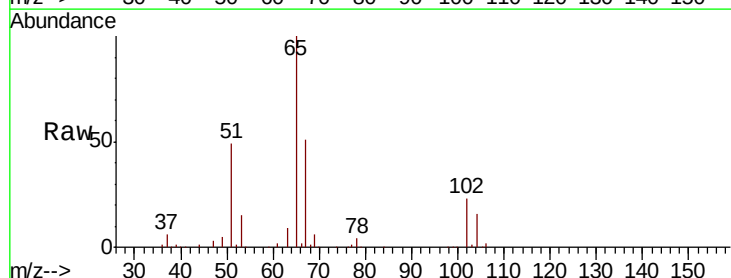

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC



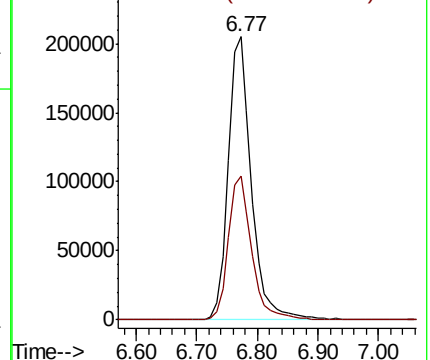
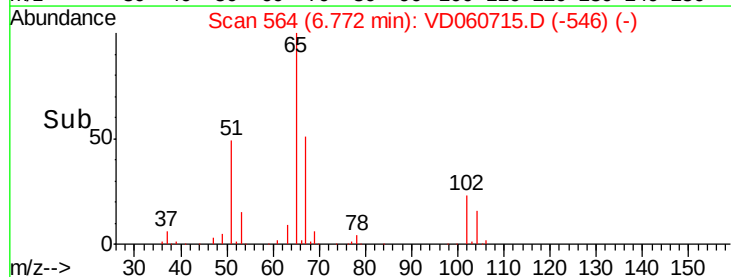


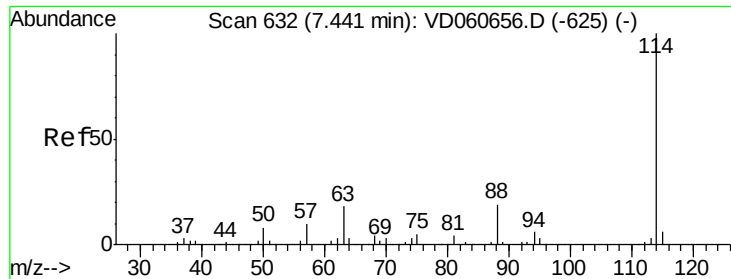

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 7.42 min Scan# 630
 Delta R.T. -0.02 min
 Lab File: VD060715.D
 Acq: 26 Dec 2018 15:11




Instrument :
 MSVOA_D
 ClientSampleId :
 TN-122618-C


Tot Ion:114 Resp: 2049264
 Ion Ratio Lower Upper
 114 100
 63 18.0 0.0 36.2
 88 19.0 0.0 37.0

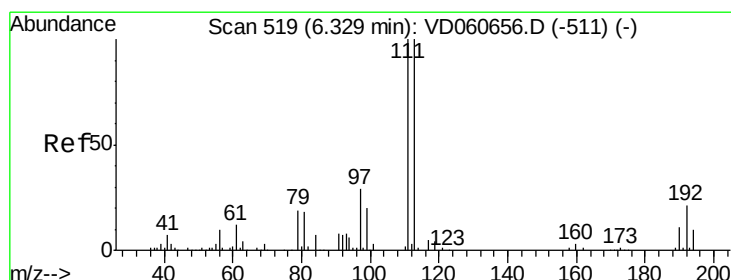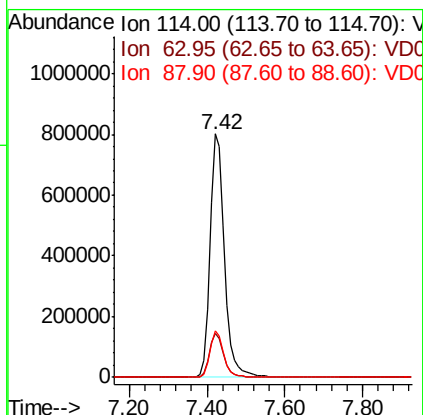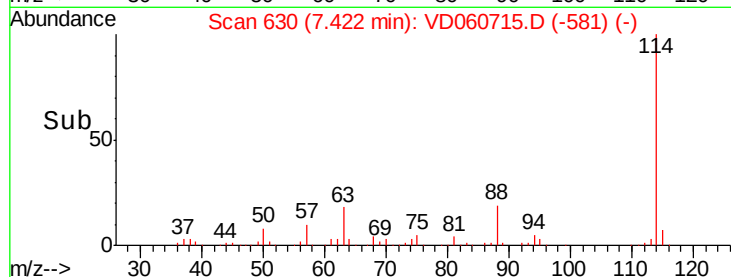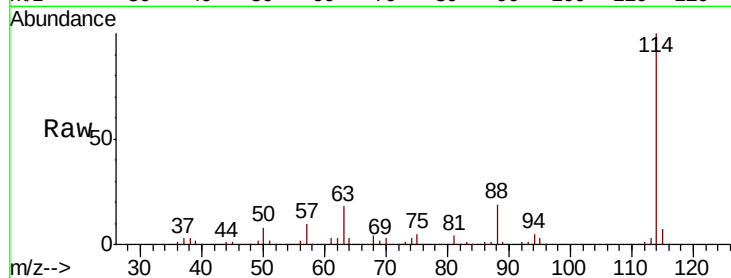

#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.31 min Scan# 517
 Delta R.T. -0.02 min
 Lab File: VD060715.D
 Acq: 26 Dec 2018 15:11

Tgt Ion:113 Resp: 718482
 Ion Ratio Lower Upper
 113 100
 111 103.5 80.0 120.0
 192 21.2 16.6 25.0

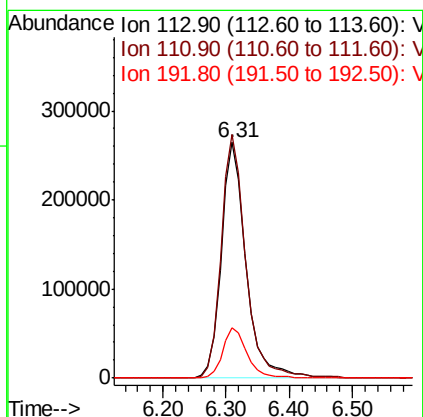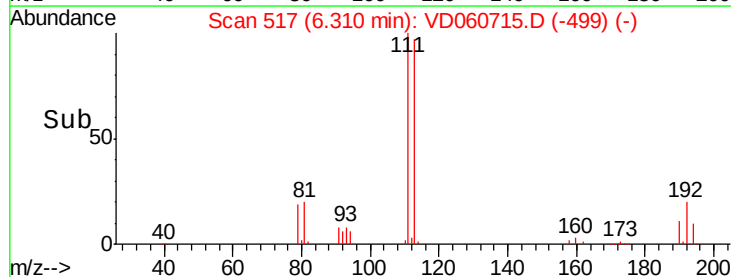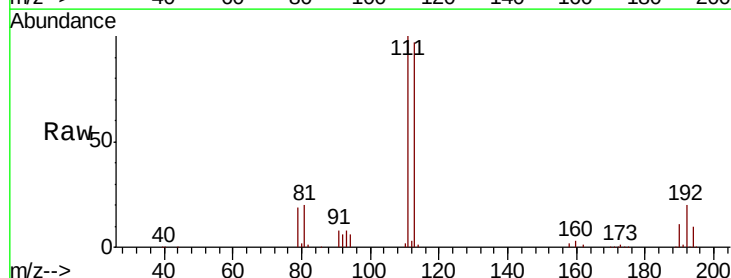


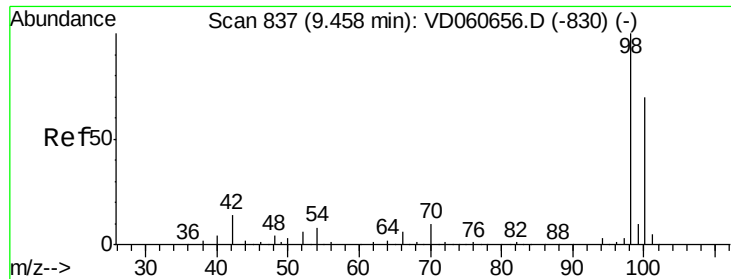




#50
Toluene-d8
Concen: N.D. ug/l
RT: 9.43 min Scan# 834
Delta R.T. -0.03 min
Lab File: VD060715.D
Acq: 26 Dec 2018 15:11

Instrument :
MSVOA_D
ClientSampleId :
TN-122618-C

Tot Ion: 98 Resp: 1911128
Ion Ratio Lower Upper
98 100
100 68.2 55.8 83.8

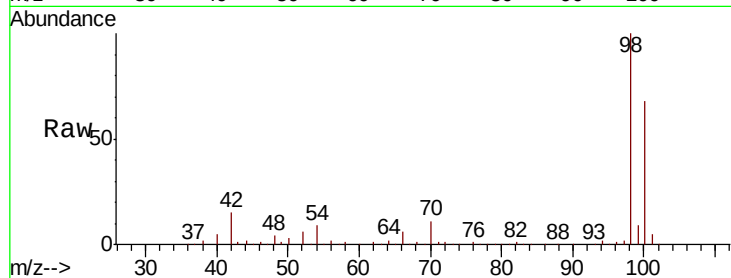


Abundance Ion 98.05 (97.75 to 98.75): VDC
Ion 100.05 (99.75 to 100.75): VDC

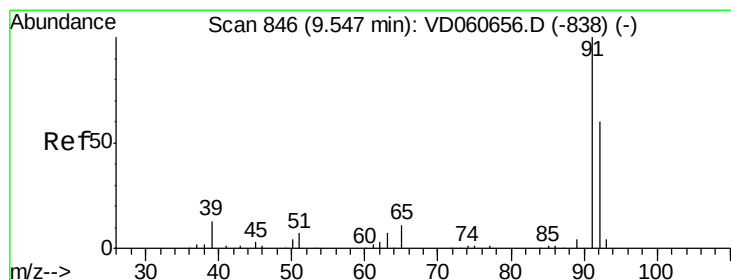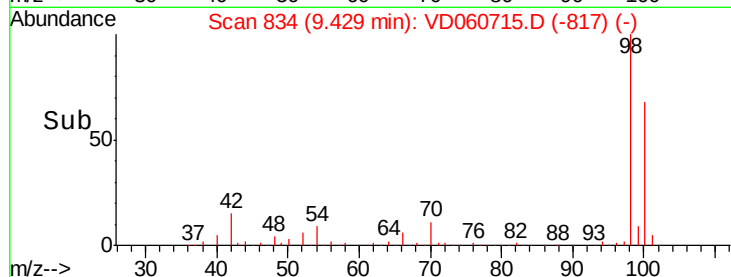
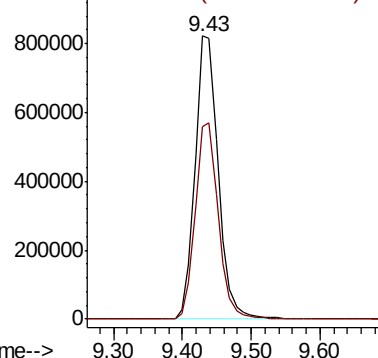



#52
Toluene
Concen: 4.438 ug/l
RT: 9.53 min Scan# 844
Delta R.T. -0.02 min
Lab File: VD060715.D
Acq: 26 Dec 2018 15:11

Tgt Ion: 92 Resp: 151662
Ion Ratio Lower Upper
92 100
91 171.2 132.6 199.0

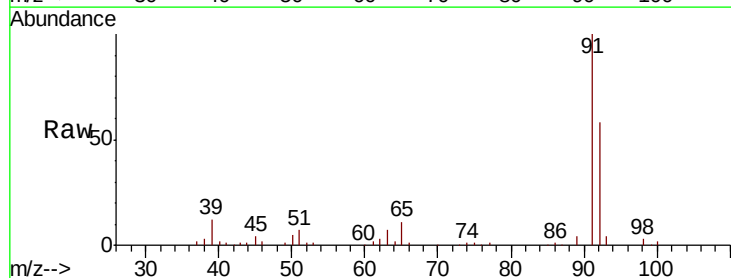

Abundance Ion 92.00 (91.70 to 92.70): VDC
Ion 91.00 (90.70 to 91.70): VDC



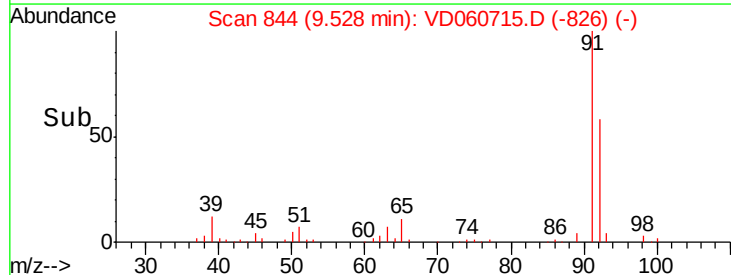
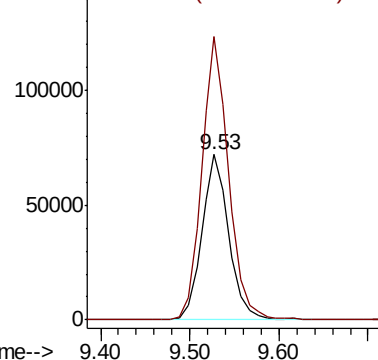


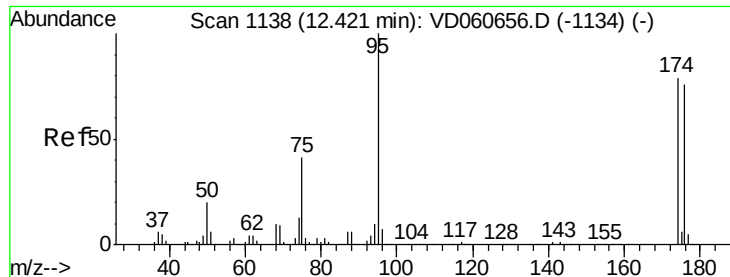

#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 12.41 min Scan# 1137
Delta R.T. -0.01 min
Lab File: VD060715.D
Acq: 26 Dec 2018 15:11




Instrument :
MSVOA_D
ClientSampleId :
TN-122618-C


Tot Ion: 95 Resp: 626644
Ion Ratio Lower Upper
95 100
174 89.2 0.0 158.2
176 86.4 0.0 152.4

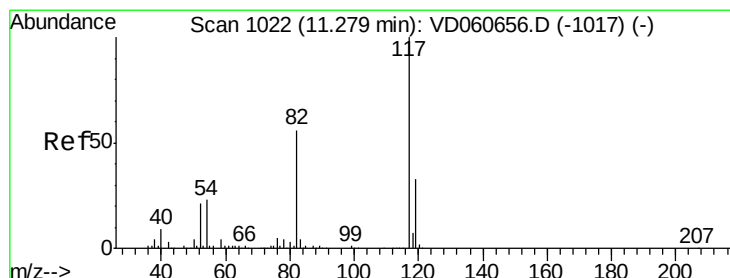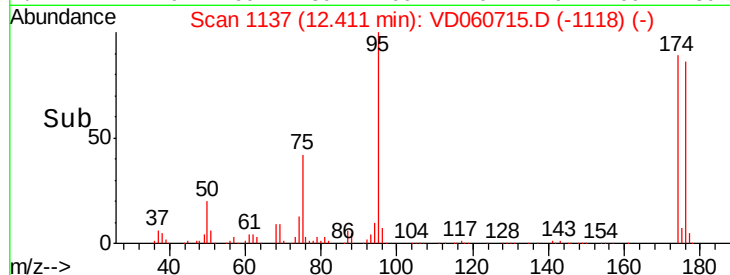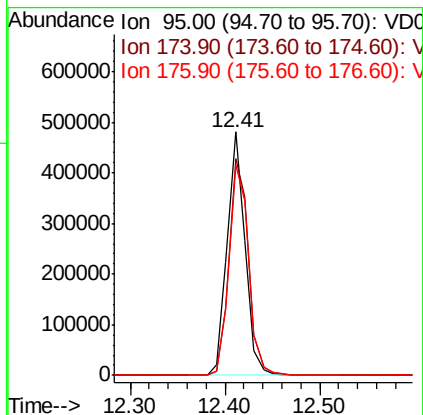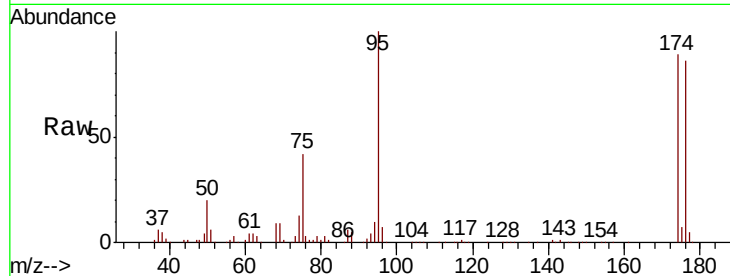

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.27 min Scan# 1021
Delta R.T. -0.01 min
Lab File: VD060715.D
Acq: 26 Dec 2018 15:11

Tgt Ion: 117 Resp: 1593579
Ion Ratio Lower Upper
117 100
82 51.3 44.5 66.7
119 32.6 26.3 39.5

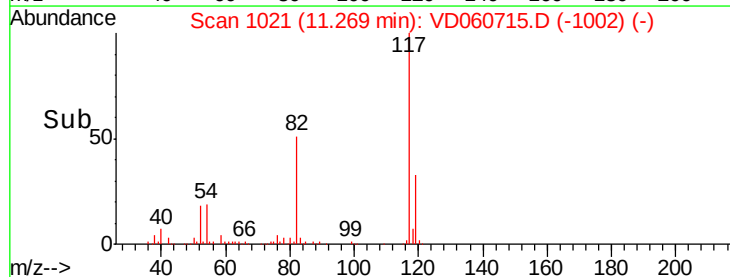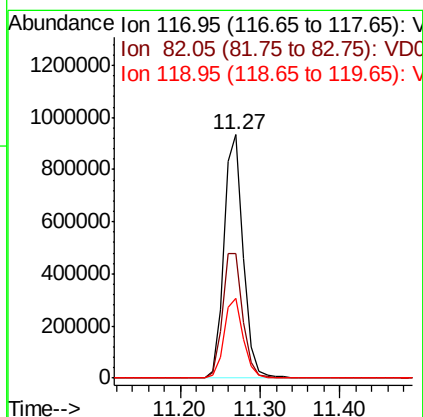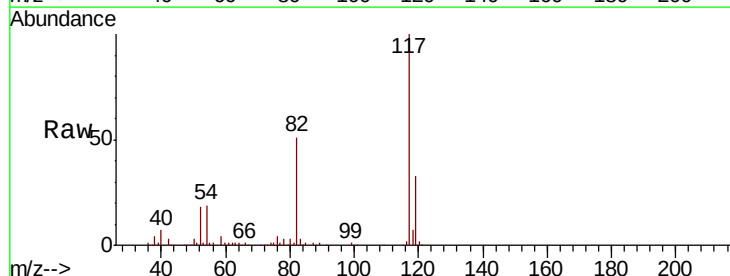


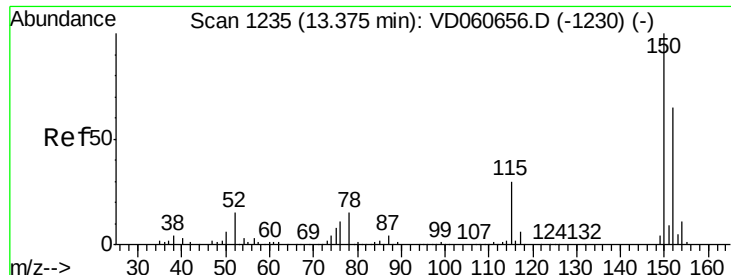

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.36 min Scan# 1233
 Delta R.T. -0.02 min
 Lab File: VD060715.D
 Acq: 26 Dec 2018 15:11

Instrument :
 MSVOA_D
 ClientSampleId :
 TN-122618-C

Tot Ion	Ratio	Lower	Upper
152	100		
115	54.0	24.1	72.3
150	154.3	0.0	315.0

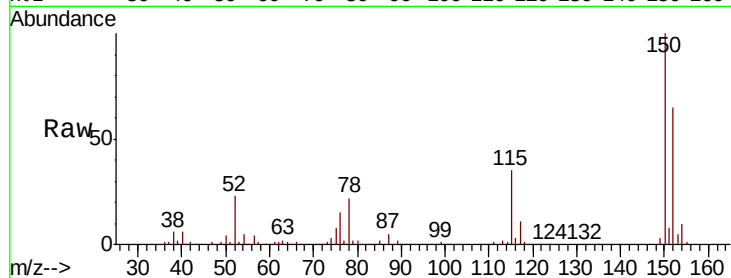

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 115.00 (114.70 to 115.70): V

Ion 149.90 (149.60 to 150.60): V

