


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122618\
Data File : VD060708.D
Acq On : 26 Dec 2018 9:51
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
Title : SW846 8260
Last Update : Fri Dec 21 17:37:47 2018

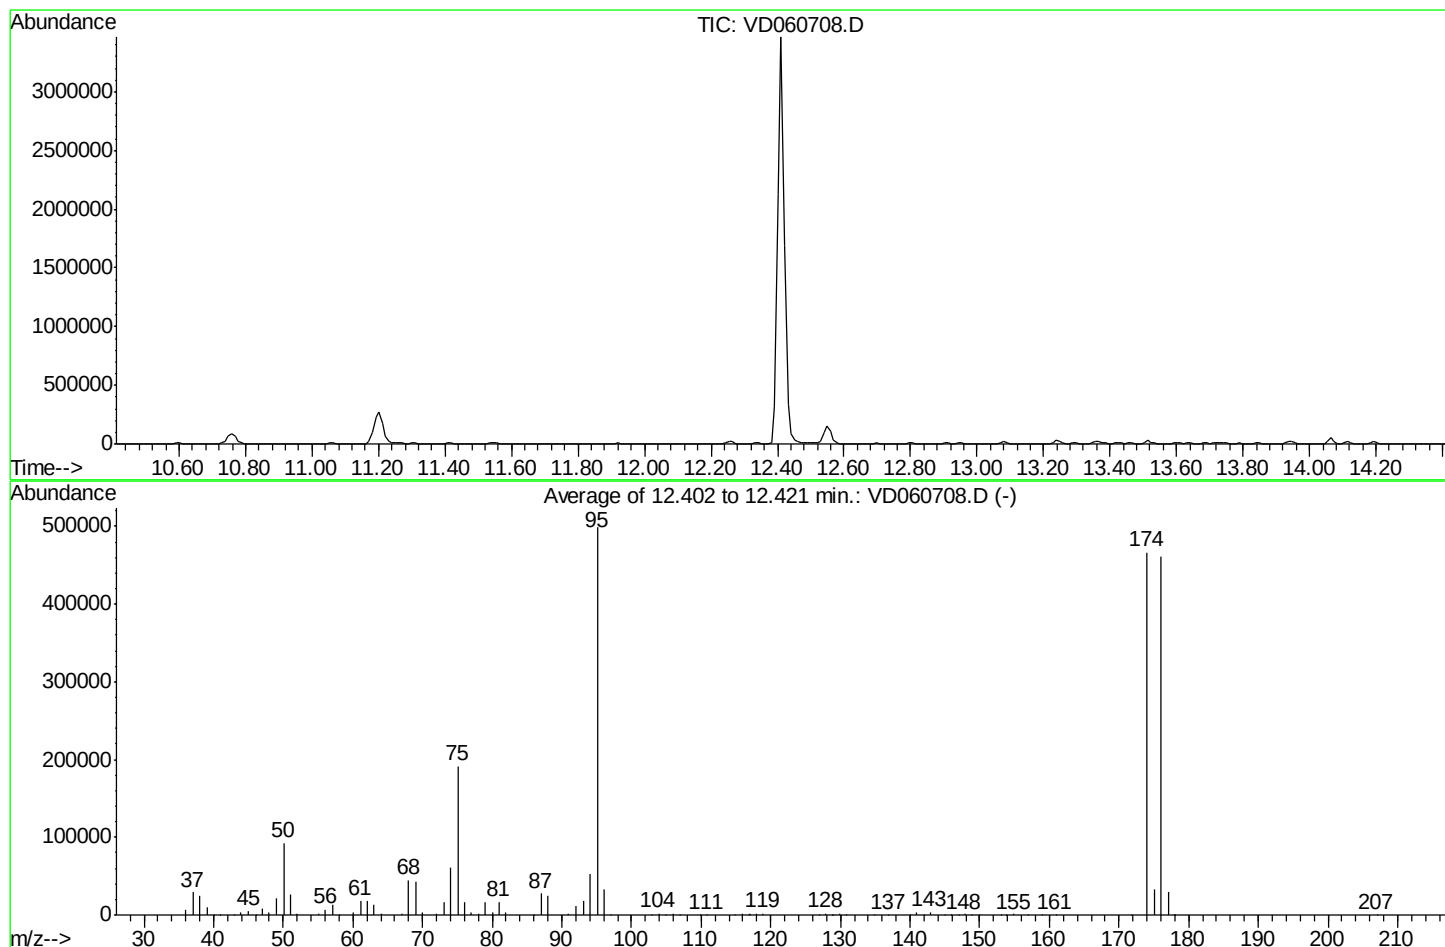

AutoFind: Scans 1136, 1137, 1138; Background Corrected with Scan 1131

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	92936	PASS
75	95	30	60	38.5	191912	PASS
95	95	100	100	100.0	498794	PASS
96	95	5	9	6.6	33133	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.6	466858	PASS
175	174	5	9	7.0	32536	PASS
176	174	95	101	98.7	460672	PASS
177	176	5	9	6.6	30434	PASS