

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122619\
 Data File : VD064590.D
 Acq On : 26 Dec 2019 10:40
 Operator : VA/SY
 Sample : VD1226SBL01
 Misc : 5.00G/5.00ml/MSVOA D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD1226SBL01

Quant Time: Dec 27 02:28:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 24 13:19:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.98	168	496881	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.87	114	780405	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	800483	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	411061	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.33	65	218137	49.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.58%	
35) Dibromofluoromethane	7.92	113	236103	49.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.62%	
50) Toluene-d8	10.34	98	951473	51.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.78%	
62) 4-Bromofluorobenzene	12.64	95	357173	61.60	ug/l	0.00
Spiked Amount	50.000		Recovery	=	123.20%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD122619\
Data File : VD064590.D
Acq On : 26 Dec 2019 10:40
Operator : VA/SY
Sample : VD1226SBL01
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD1226SBL01

Quant Time: Dec 27 02:28:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 24 13:19:06 2019
Response via : Initial Calibration

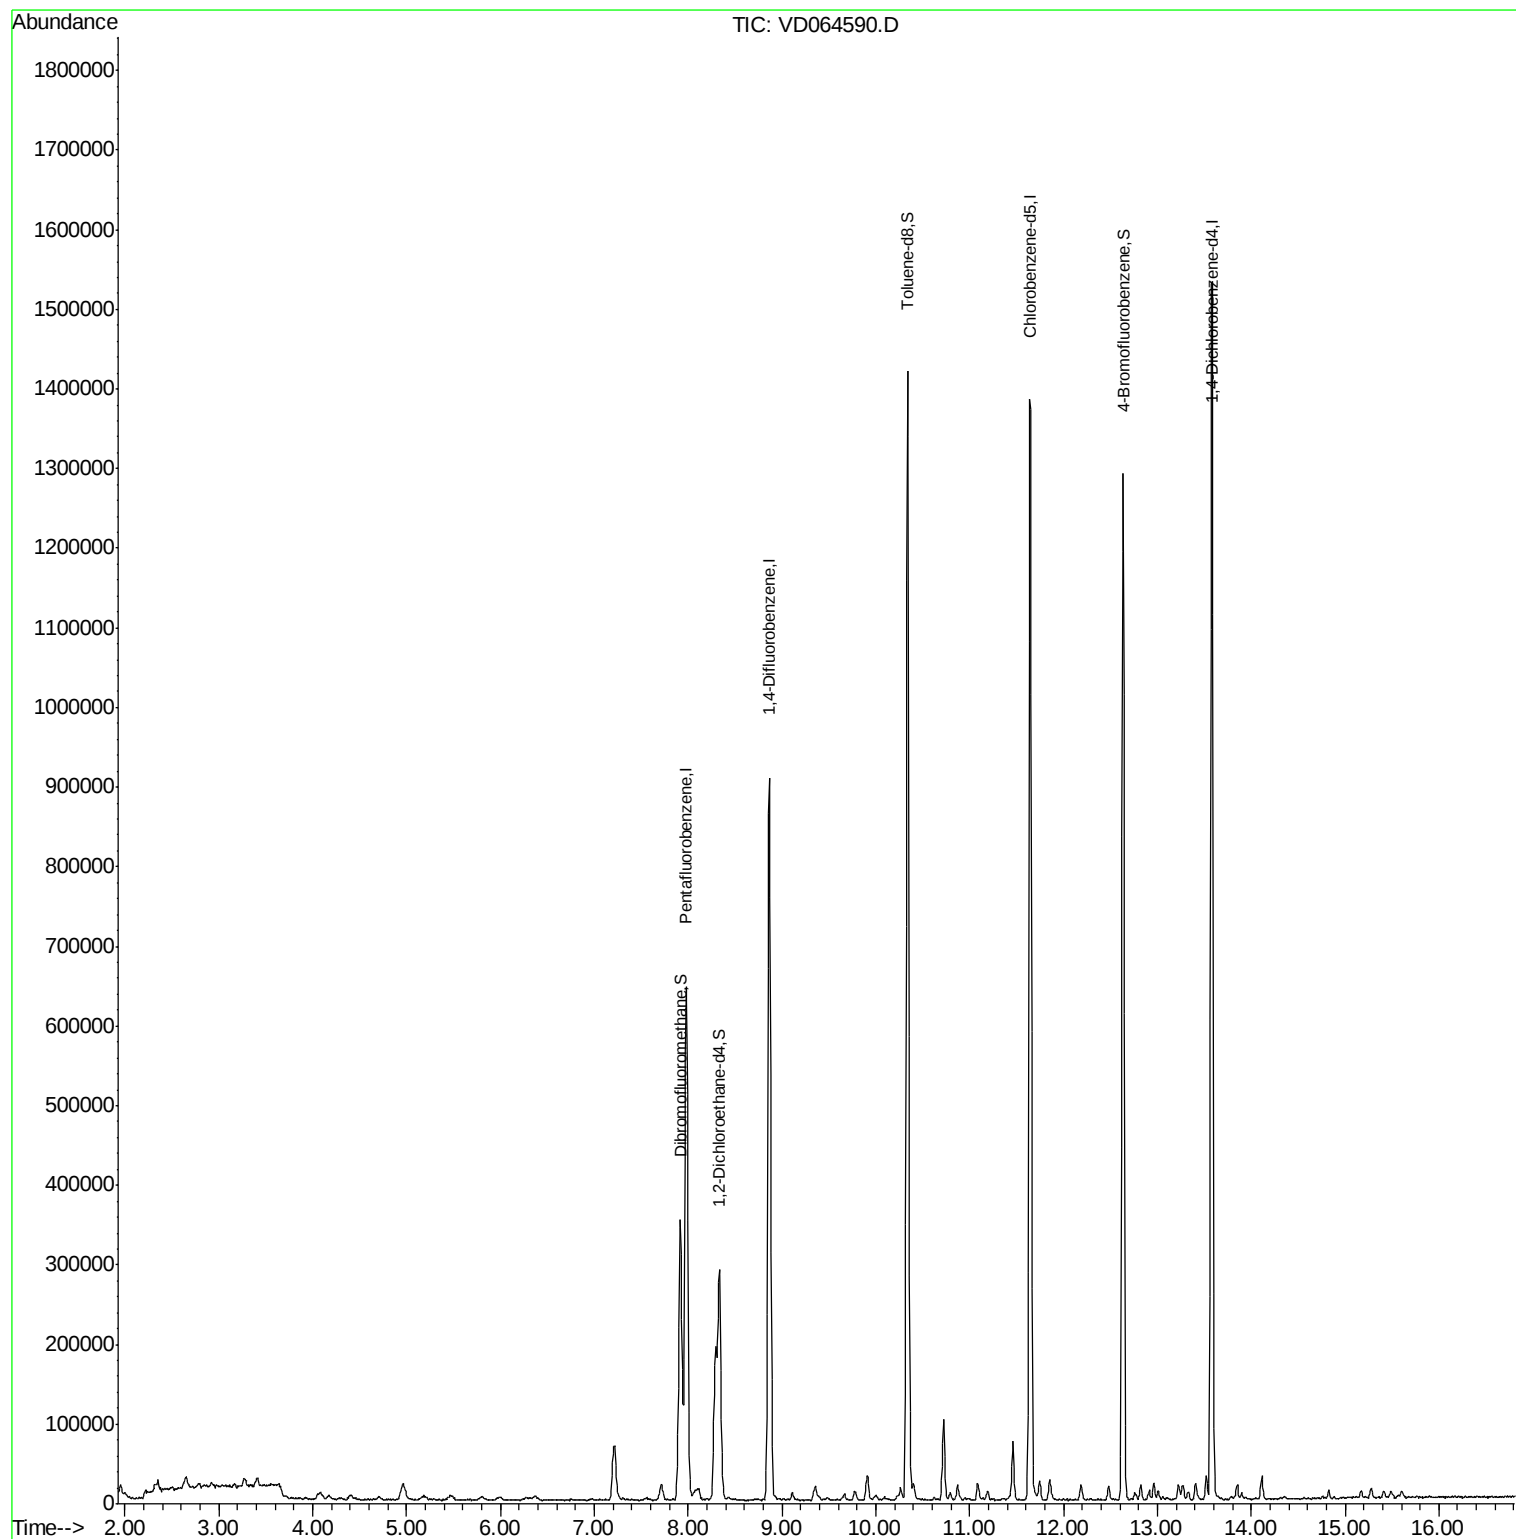

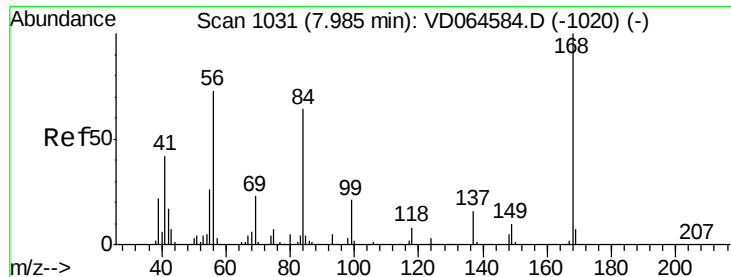

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.98 min Scan# 1030

Delta R.T. -0.01 min

Lab File: VD064590.D

Acq: 26 Dec 2019 10:40

Instrument :

MSVOA_D

ClientSampleId :


VD1226SBL01

Tot Ion:168 Resp: 496881

Ion Ratio Lower Upper

168 100

99 50.4 41.8 62.6

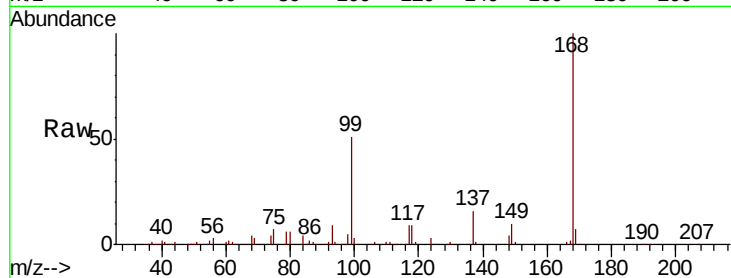

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VDC

7.98

250000

200000



150000

100000

50000

0

Time-->

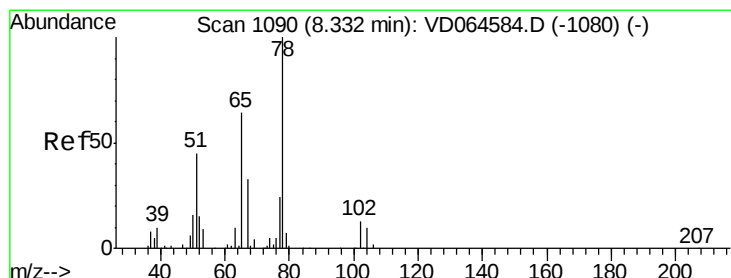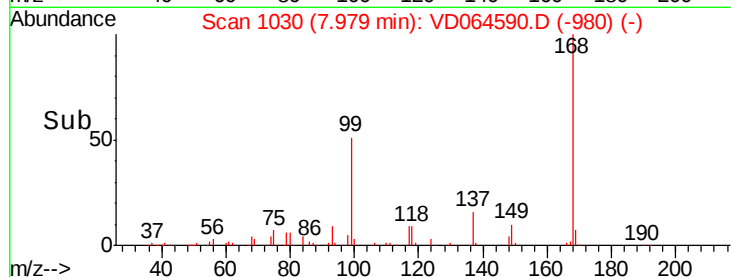

#33

1,2-Dichloroethane-d4

Concen: 49.787 ug/l

RT: 8.33 min Scan# 1090

Delta R.T. 0.00 min

Lab File: VD064590.D


Acq: 26 Dec 2019 10:40

Tgt Ion: 65 Resp: 218137

Ion Ratio Lower Upper

65 100

67 51.5 0.0 106.2

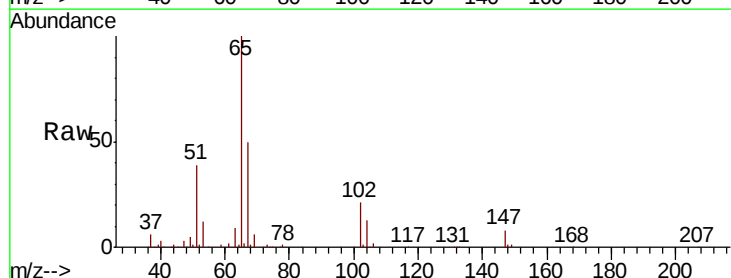

Abundance Ion 64.90 (64.60 to 65.60): VDC

Ion 66.90 (66.60 to 67.60): VDC

8.33

100000

80000


60000


40000

20000

0

Time-->

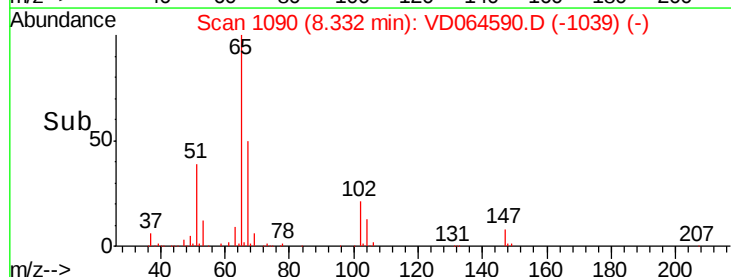

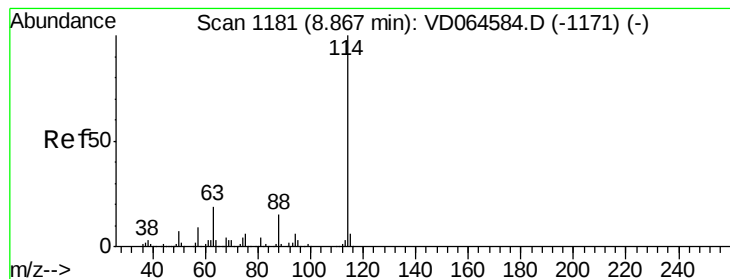

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.87 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VD064590.D

Acq: 26 Dec 2019 10:40

Instrument :

MSVOA_D

ClientSampleId :

VD1226SBL01


Tot Ion:114 Resp: 780405

Ion Ratio Lower Upper

114 100

63 19.5 0.0 38.0




88 14.0 0.0 29.2

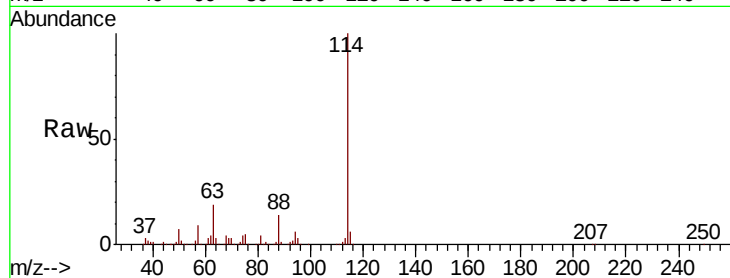

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): V

Ion 87.90 (87.60 to 88.60): V

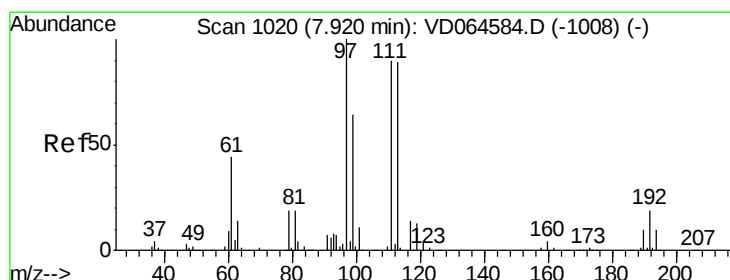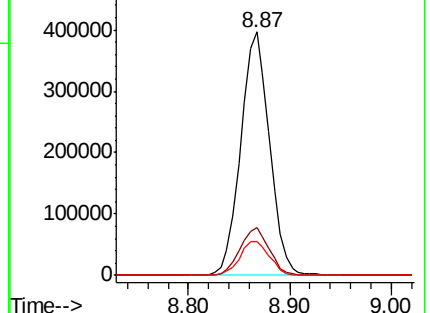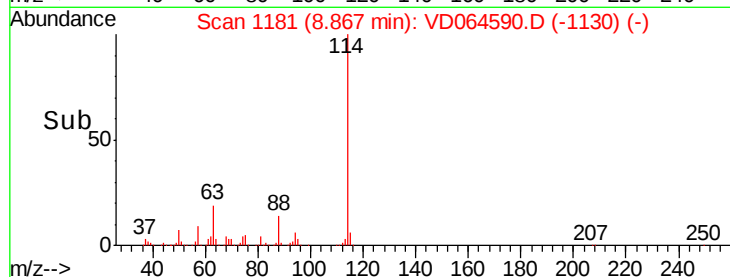

#35

Dibromofluoromethane

Concen: 49.312 ug/l

RT: 7.92 min Scan# 1020

Delta R.T. 0.00 min

Lab File: VD064590.D

Acq: 26 Dec 2019 10:40


Tgt Ion:113 Resp: 236103

Ion Ratio Lower Upper

113 100

111 103.8 80.6 121.0



192 23.1 17.9 26.9

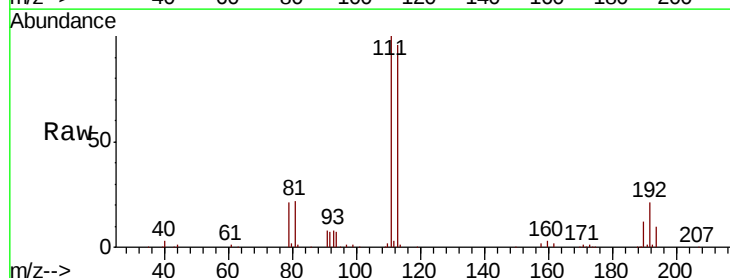


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



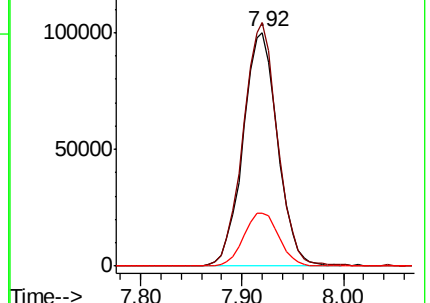
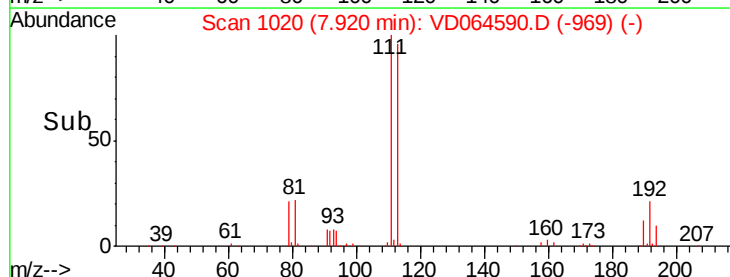


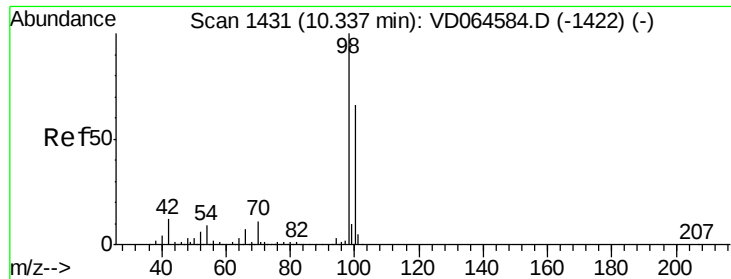

#50
Toluene-d8
Concen: 51.888 ug/l
RT: 10.34 min Scan# 1431
Delta R.T. 0.00 min
Lab File: VD064590.D
Acq: 26 Dec 2019 10:40




Instrument :
MSVOA_D
ClientSampleId :
VD1226SBL01


Tot Ion: 98 Resp: 951473
Ion Ratio Lower Upper
98 100
100 65.5 51.7 77.5

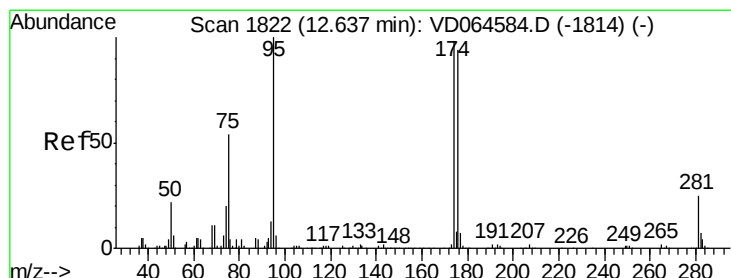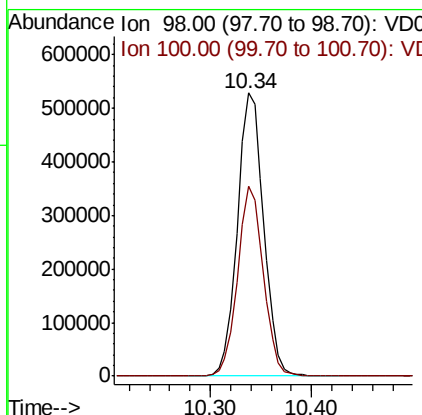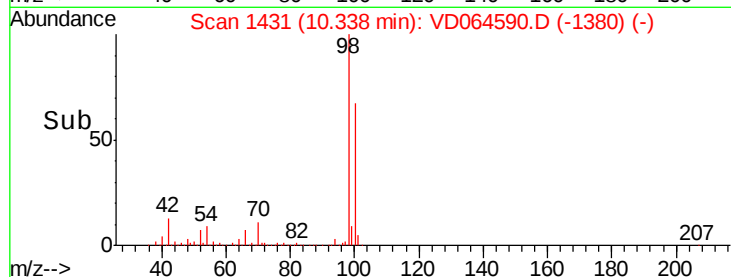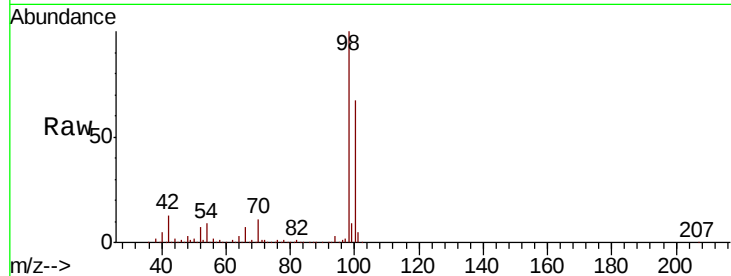

#62
4-Bromofluorobenzene
Concen: 61.598 ug/l
RT: 12.64 min Scan# 1822
Delta R.T. 0.00 min
Lab File: VD064590.D
Acq: 26 Dec 2019 10:40

Tgt Ion: 95 Resp: 357173
Ion Ratio Lower Upper
95 100
174 96.7 0.0 193.2
176 93.0 0.0 184.2


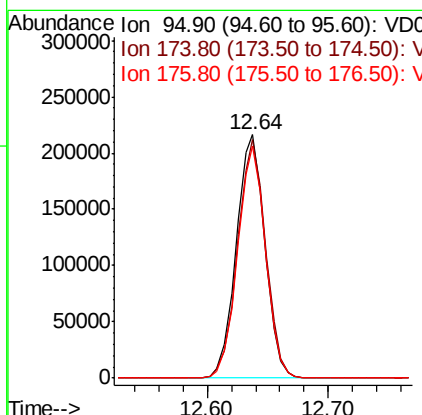
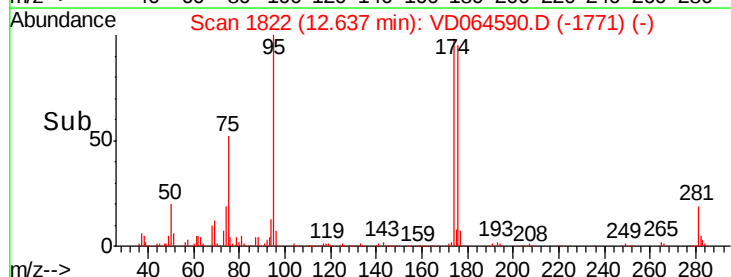
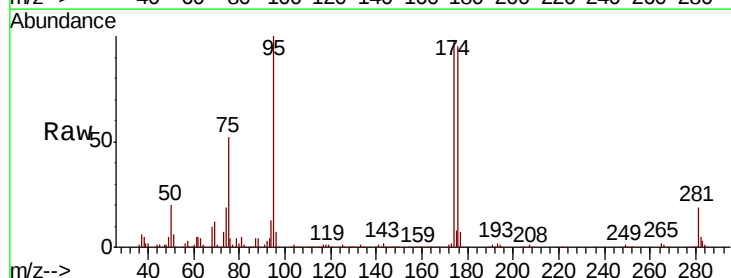


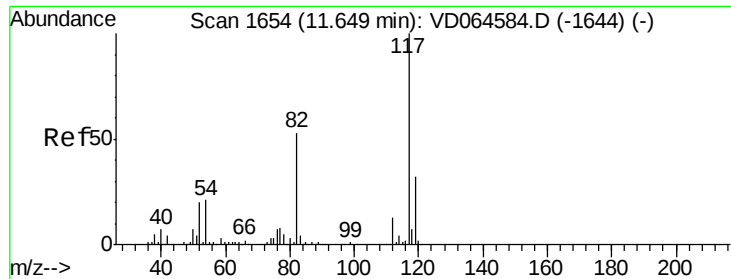

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.64 min Scan# 1653
Delta R.T. -0.01 min
Lab File: VD064590.D
Acq: 26 Dec 2019 10:40

Instrument :
MSVOA_D
ClientSampleId :
VD1226SBL01

Tot Ion:117 Resp: 800483
Ion Ratio Lower Upper
117 100
82 51.7 42.2 63.4
119 32.0 26.0 39.0

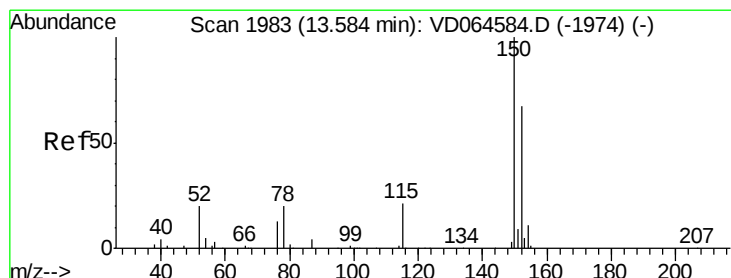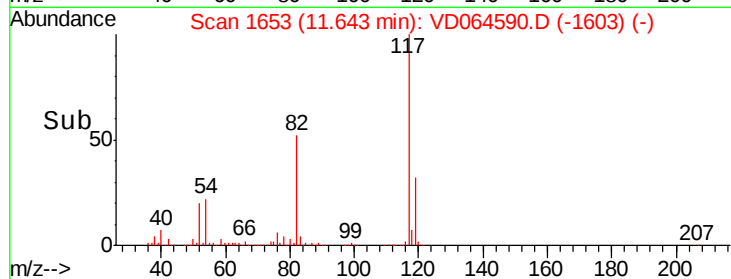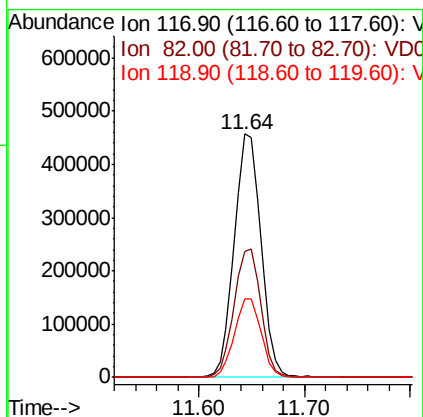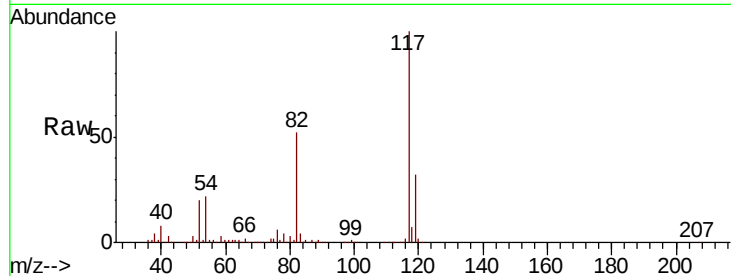

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.58 min Scan# 1983
Delta R.T. 0.00 min
Lab File: VD064590.D
Acq: 26 Dec 2019 10:40

Tgt Ion:152 Resp: 411061
Ion Ratio Lower Upper
152 100
115 56.1 27.8 83.4
150 159.4 0.0 351.4

