


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122619\
Data File : VD064612.D
Acq On : 26 Dec 2019 21:48
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Title : SW846 8260
Last Update : Tue Dec 24 13:19:06 2019

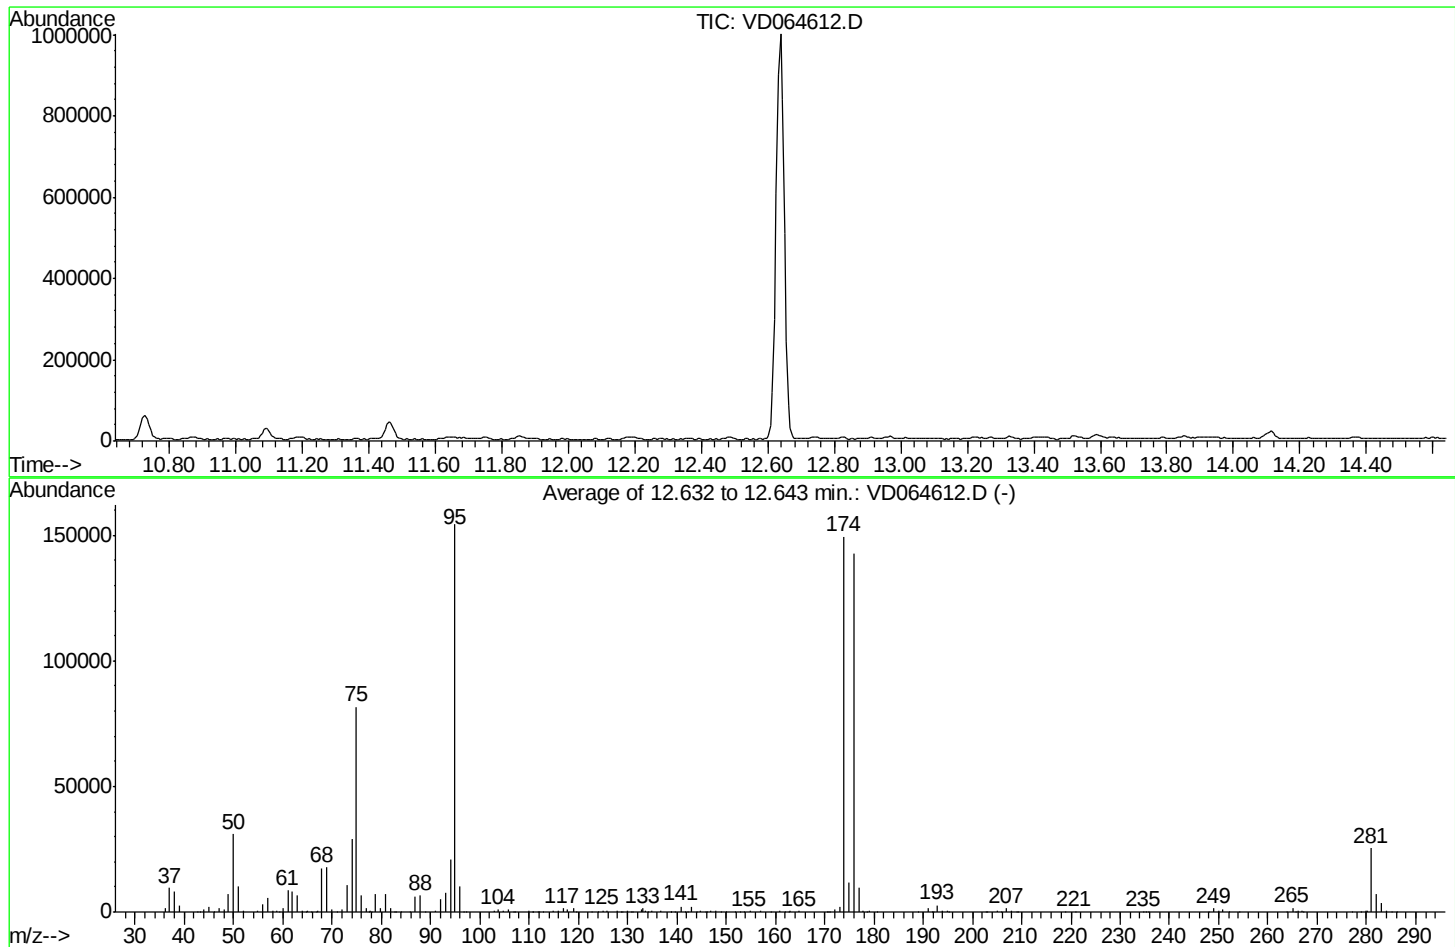

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	30917	PASS
75	95	30	60	52.9	81605	PASS
95	95	100	100	100.0	154389	PASS
96	95	5	9	6.6	10246	PASS
173	174	0.00	2	1.4	2127	PASS
174	95	50	100	96.9	149610	PASS
175	174	5	9	7.9	11814	PASS
176	174	95	101	95.5	142848	PASS
177	176	5	9	6.9	9792	PASS