
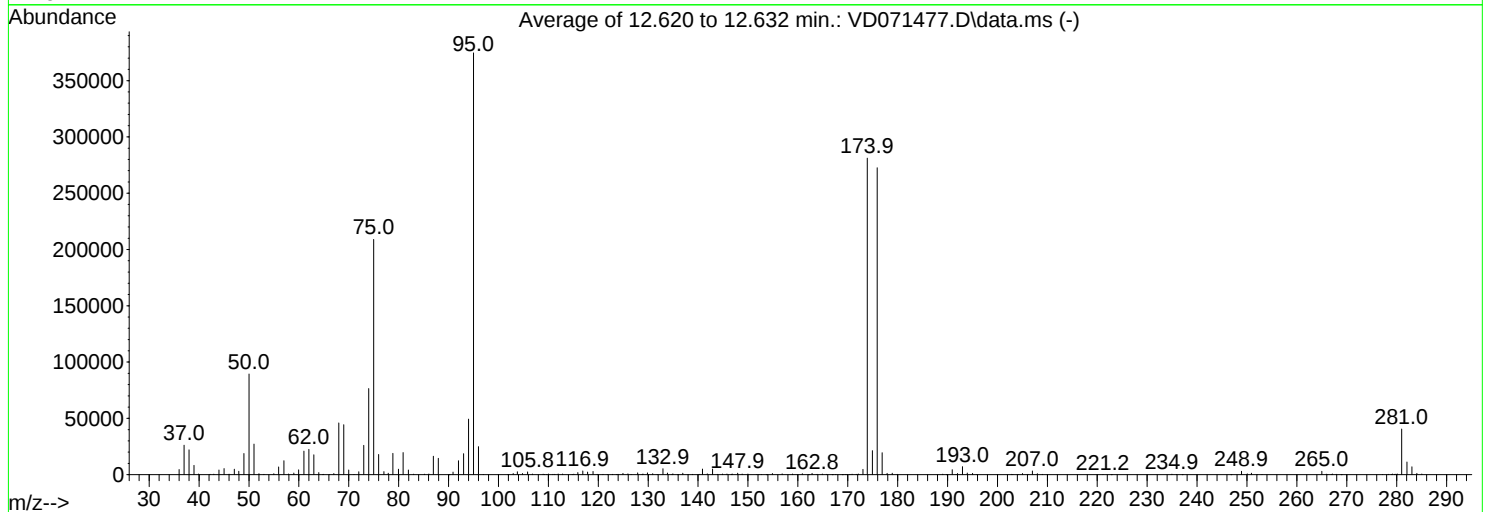


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122721\
Data File : VD071477.D
Acq On : 27 Dec 2021 09:15
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
Title : SW846 8260
Last Update : Thu Dec 23 08:20:24 2021

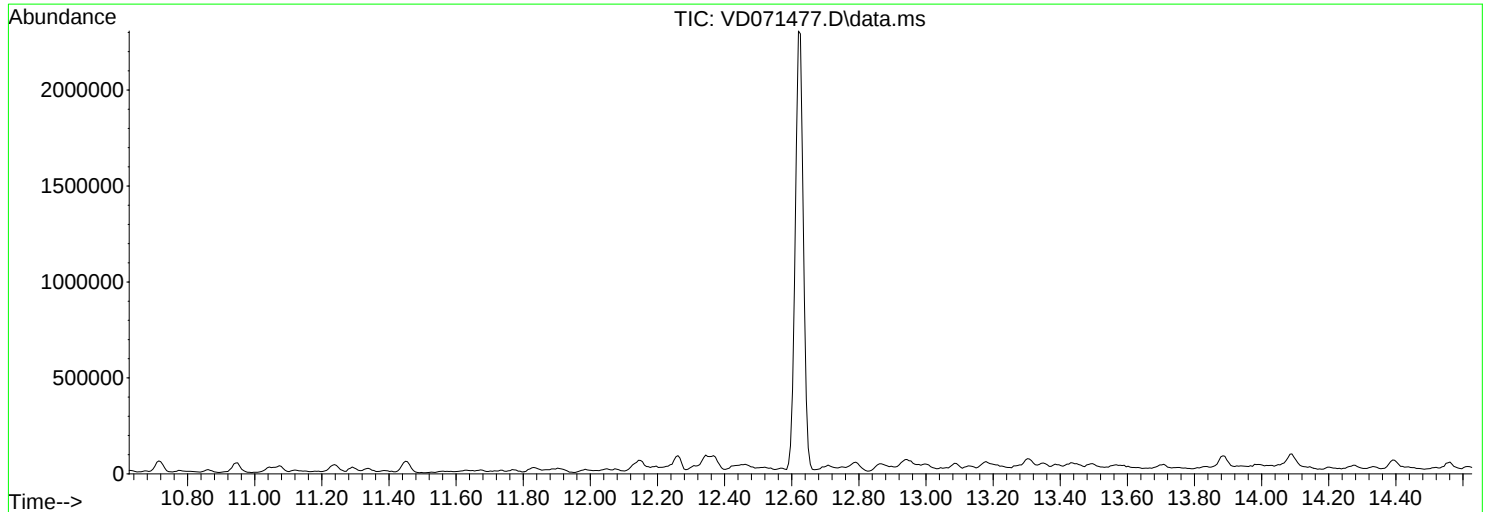

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1803

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	89475	PASS
75	95	30	60	55.8	208981	PASS
95	95	100	100	100.0	374698	PASS
96	95	5	9	6.7	24920	PASS
173	174	0.00	2	1.7	4760	PASS
174	95	50	100	75.0	281088	PASS
175	174	5	9	7.6	21352	PASS
176	174	95	101	97.0	272576	PASS
177	176	5	9	7.2	19504	PASS