


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD122818\
Data File : VD060742.D
Acq On : 28 Dec 2018 10:12
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122018S.M
Title : SW846 8260
Last Update : Fri Dec 21 17:37:47 2018

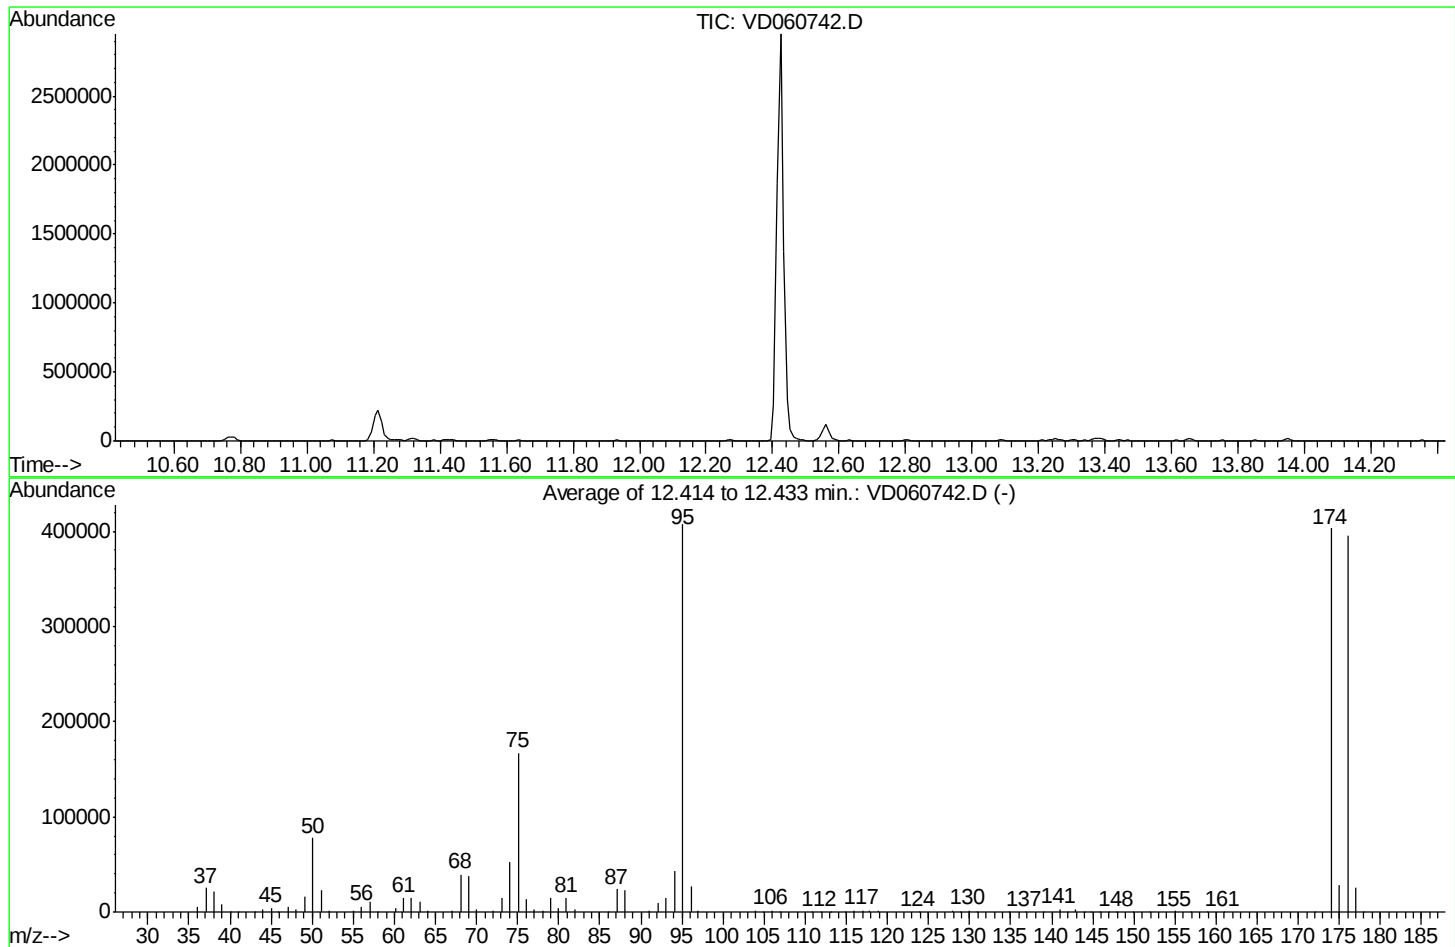

AutoFind: Scans 1137, 1138, 1139; Background Corrected with Scan 1132

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	77853	PASS
75	95	30	60	41.0	167114	PASS
95	95	100	100	100.0	407210	PASS
96	95	5	9	6.5	26620	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	99.2	403818	PASS
175	174	5	9	6.9	27842	PASS
176	174	95	101	98.0	395861	PASS
177	176	5	9	6.6	26234	PASS