
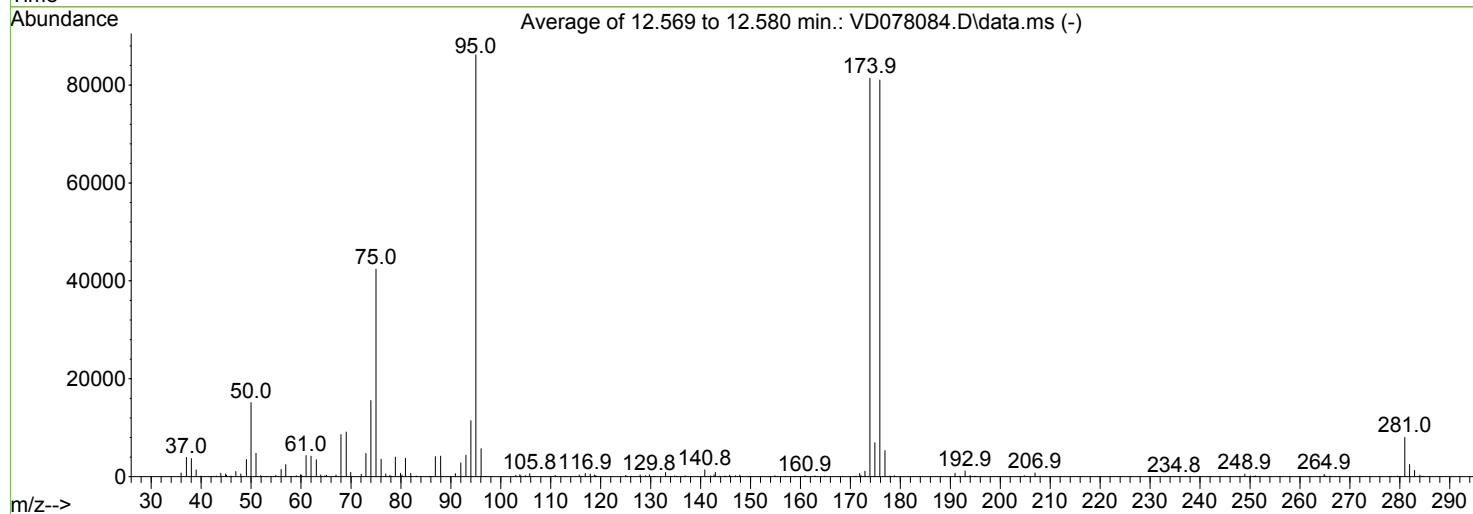


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD122823\
Data File : VD078084.D
Acq On : 28 Dec 2023 08:38
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122623S.M
Title : SW846 8260
Last Update : Wed Dec 27 03:40:16 2023

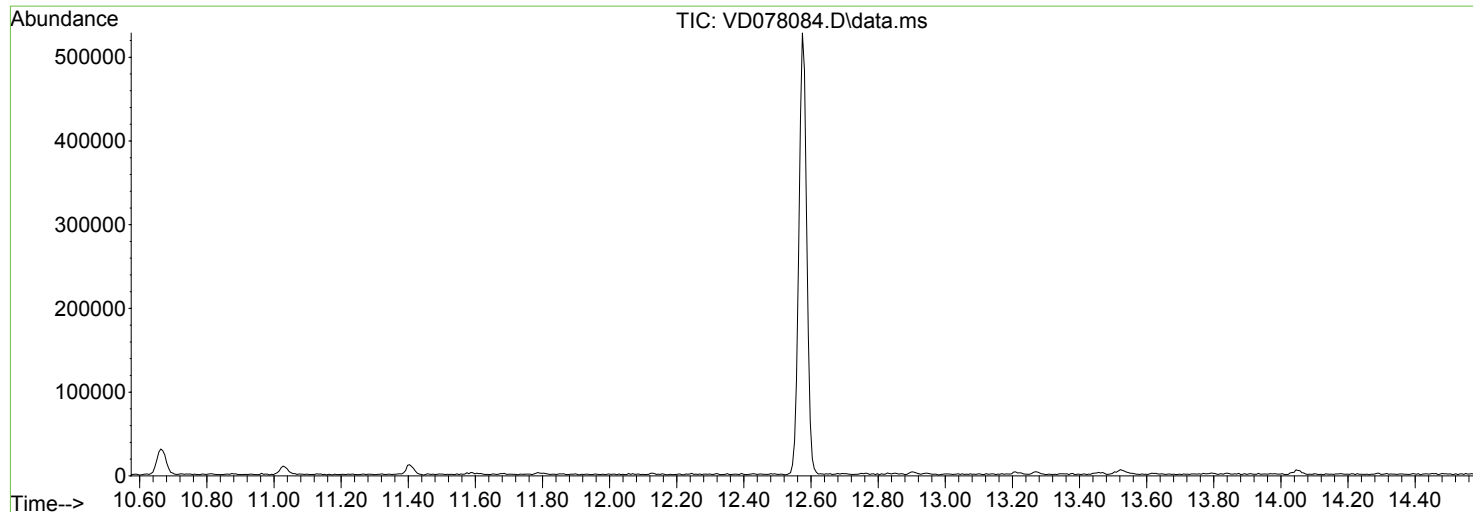

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	15155	PASS
75	95	30	60	49.2	42400	PASS
95	95	100	100	100.0	86181	PASS
96	95	5	9	6.7	5732	PASS
173	174	0.00	2	1.4	1110	PASS
174	95	50	100	94.5	81408	PASS
175	174	5	9	8.5	6945	PASS
176	174	95	101	99.6	81043	PASS
177	176	5	9	6.6	5346	PASS