


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD123019\
Data File : VD064670.D
Acq On : 30 Dec 2019 09:27
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D122419S.M
Title : SW846 8260
Last Update : Tue Dec 24 13:19:06 2019

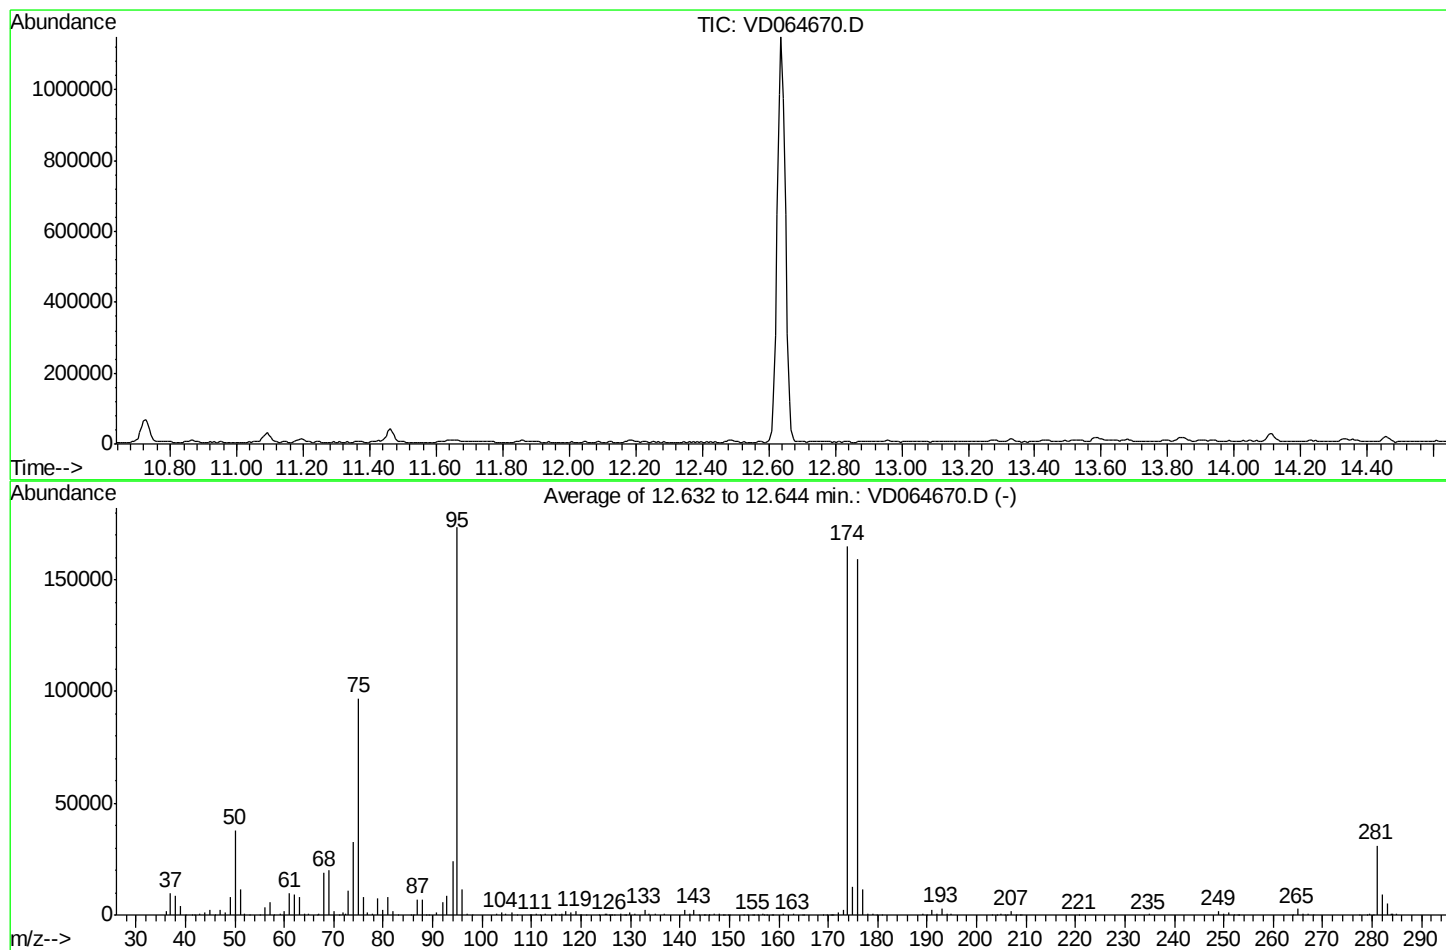

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	37978	PASS
75	95	30	60	55.9	96885	PASS
95	95	100	100	100.0	173461	PASS
96	95	5	9	6.6	11363	PASS
173	174	0.00	2	1.4	2256	PASS
174	95	50	100	95.1	165034	PASS
175	174	5	9	7.6	12598	PASS
176	174	95	101	96.4	159125	PASS
177	176	5	9	7.2	11391	PASS