


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD123021\
Data File : VD071536.D
Acq On : 30 Dec 2021 08:11
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D122221S.M
Title : SW846 8260
Last Update : Thu Dec 23 08:20:24 2021

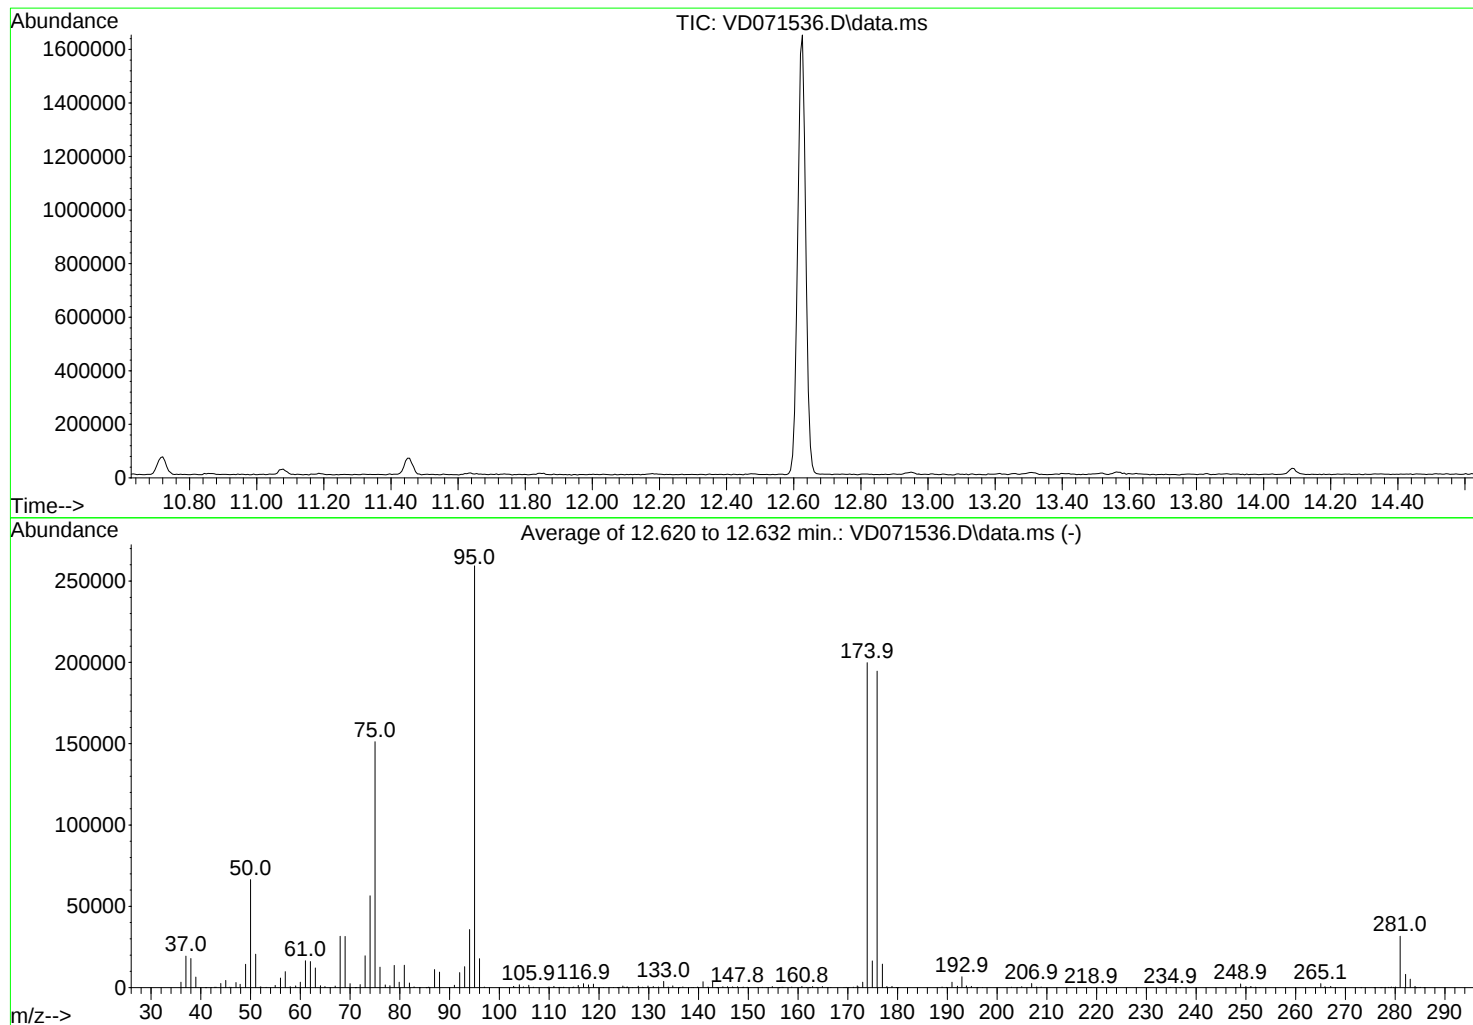

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.6	66408	PASS
75	95	30	60	58.3	151251	PASS
95	95	100	100	100.0	259371	PASS
96	95	5	9	6.9	17776	PASS
173	174	0.00	2	1.7	3330	PASS
174	95	50	100	77.0	199829	PASS
175	174	5	9	8.2	16484	PASS
176	174	95	101	97.4	194603	PASS
177	176	5	9	7.4	14449	PASS