


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD011221\
 Data File : VD068050.D
 Acq On : 12 Jan 2021 11:08
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011221S.M
 Title : SW846 8260
 Last Update : Wed Jan 13 03:57:57 2021

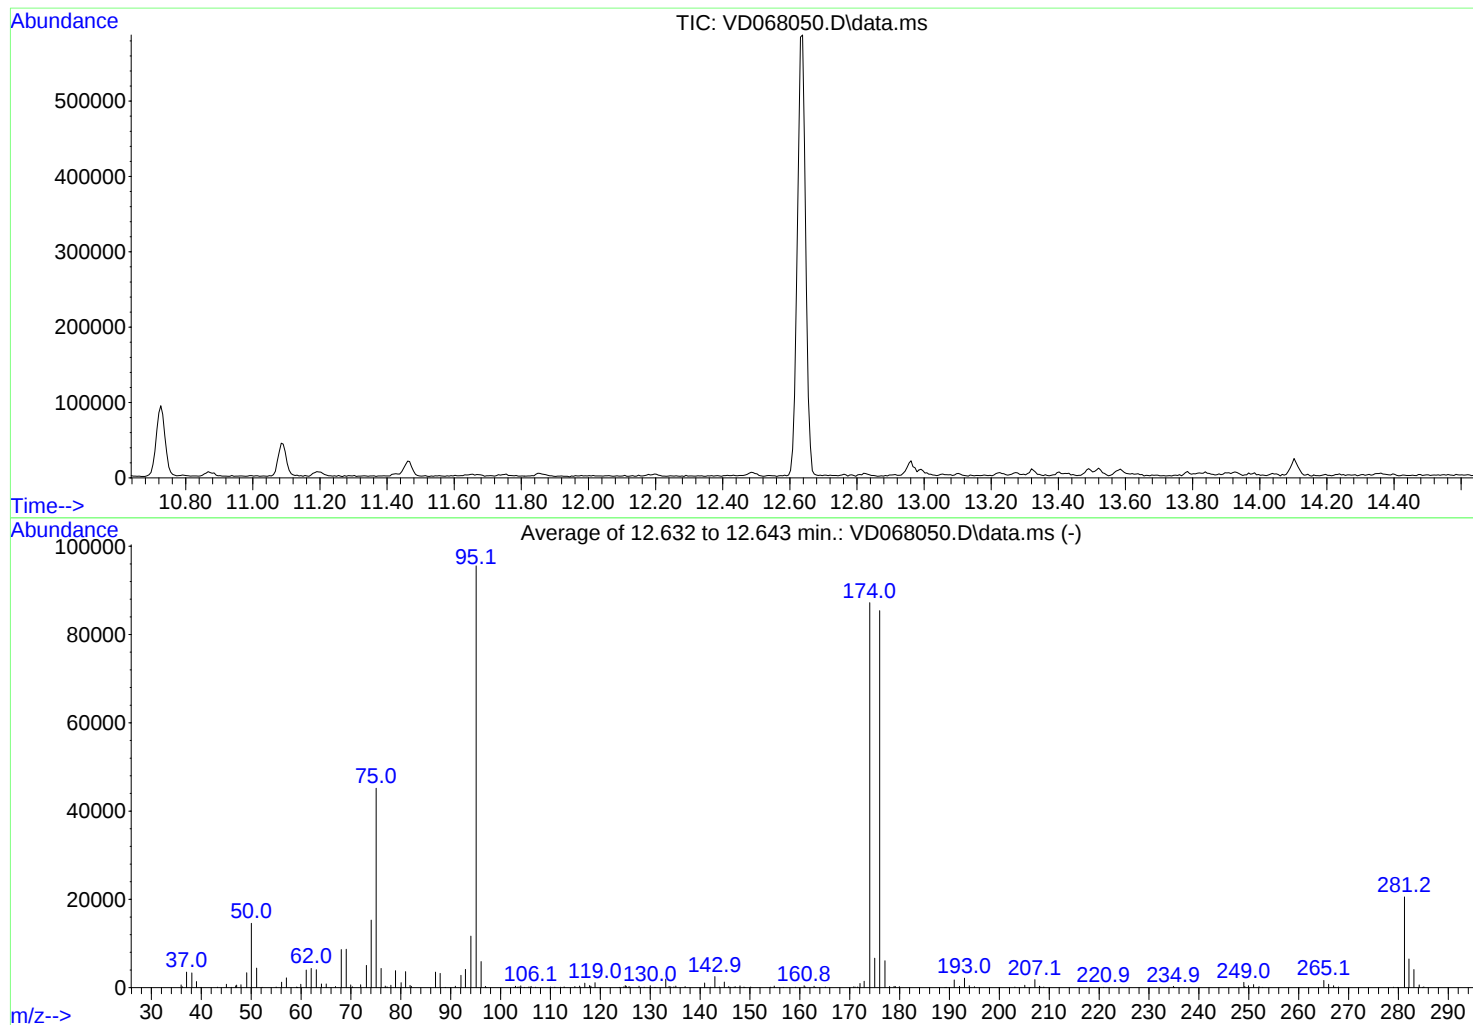

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	14589	PASS
75	95	30	60	47.3	45163	PASS
95	95	100	100	100.0	95563	PASS
96	95	5	9	6.2	5899	PASS
173	174	0.00	2	1.7	1449	PASS
174	95	50	100	91.3	87213	PASS
175	174	5	9	7.7	6684	PASS
176	174	95	101	97.9	85424	PASS
177	176	5	9	7.1	6101	PASS