

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012121\
 Data File : VD068131.D
 Acq On : 21 Jan 2021 14:31
 Operator : VA/SY
 Sample : M1152-02
 Misc : 7.71G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-EF-01-017-ABCD

Quant Time: Jan 22 00:09:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 19 13:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	575781	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	976232	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.650	117	968113	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	457494	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	261224	47.43	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	94.86%
35) Dibromofluoromethane	7.920	113	274412	50.84	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.68%
50) Toluene-d8	10.344	98	1228646	56.91	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	113.82%
62) 4-Bromofluorobenzene	12.632	95	465498	59.88	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	119.76%


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD012121\
Data File : VD068131.D
Acq On : 21 Jan 2021 14:31
Operator : VA/SY
Sample : M1152-02
Misc : 7.71G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FK-EF-01-017-ABCD

Quant Time: Jan 22 00:09:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D011921S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 19 13:19:08 2021
Response via : Initial Calibration




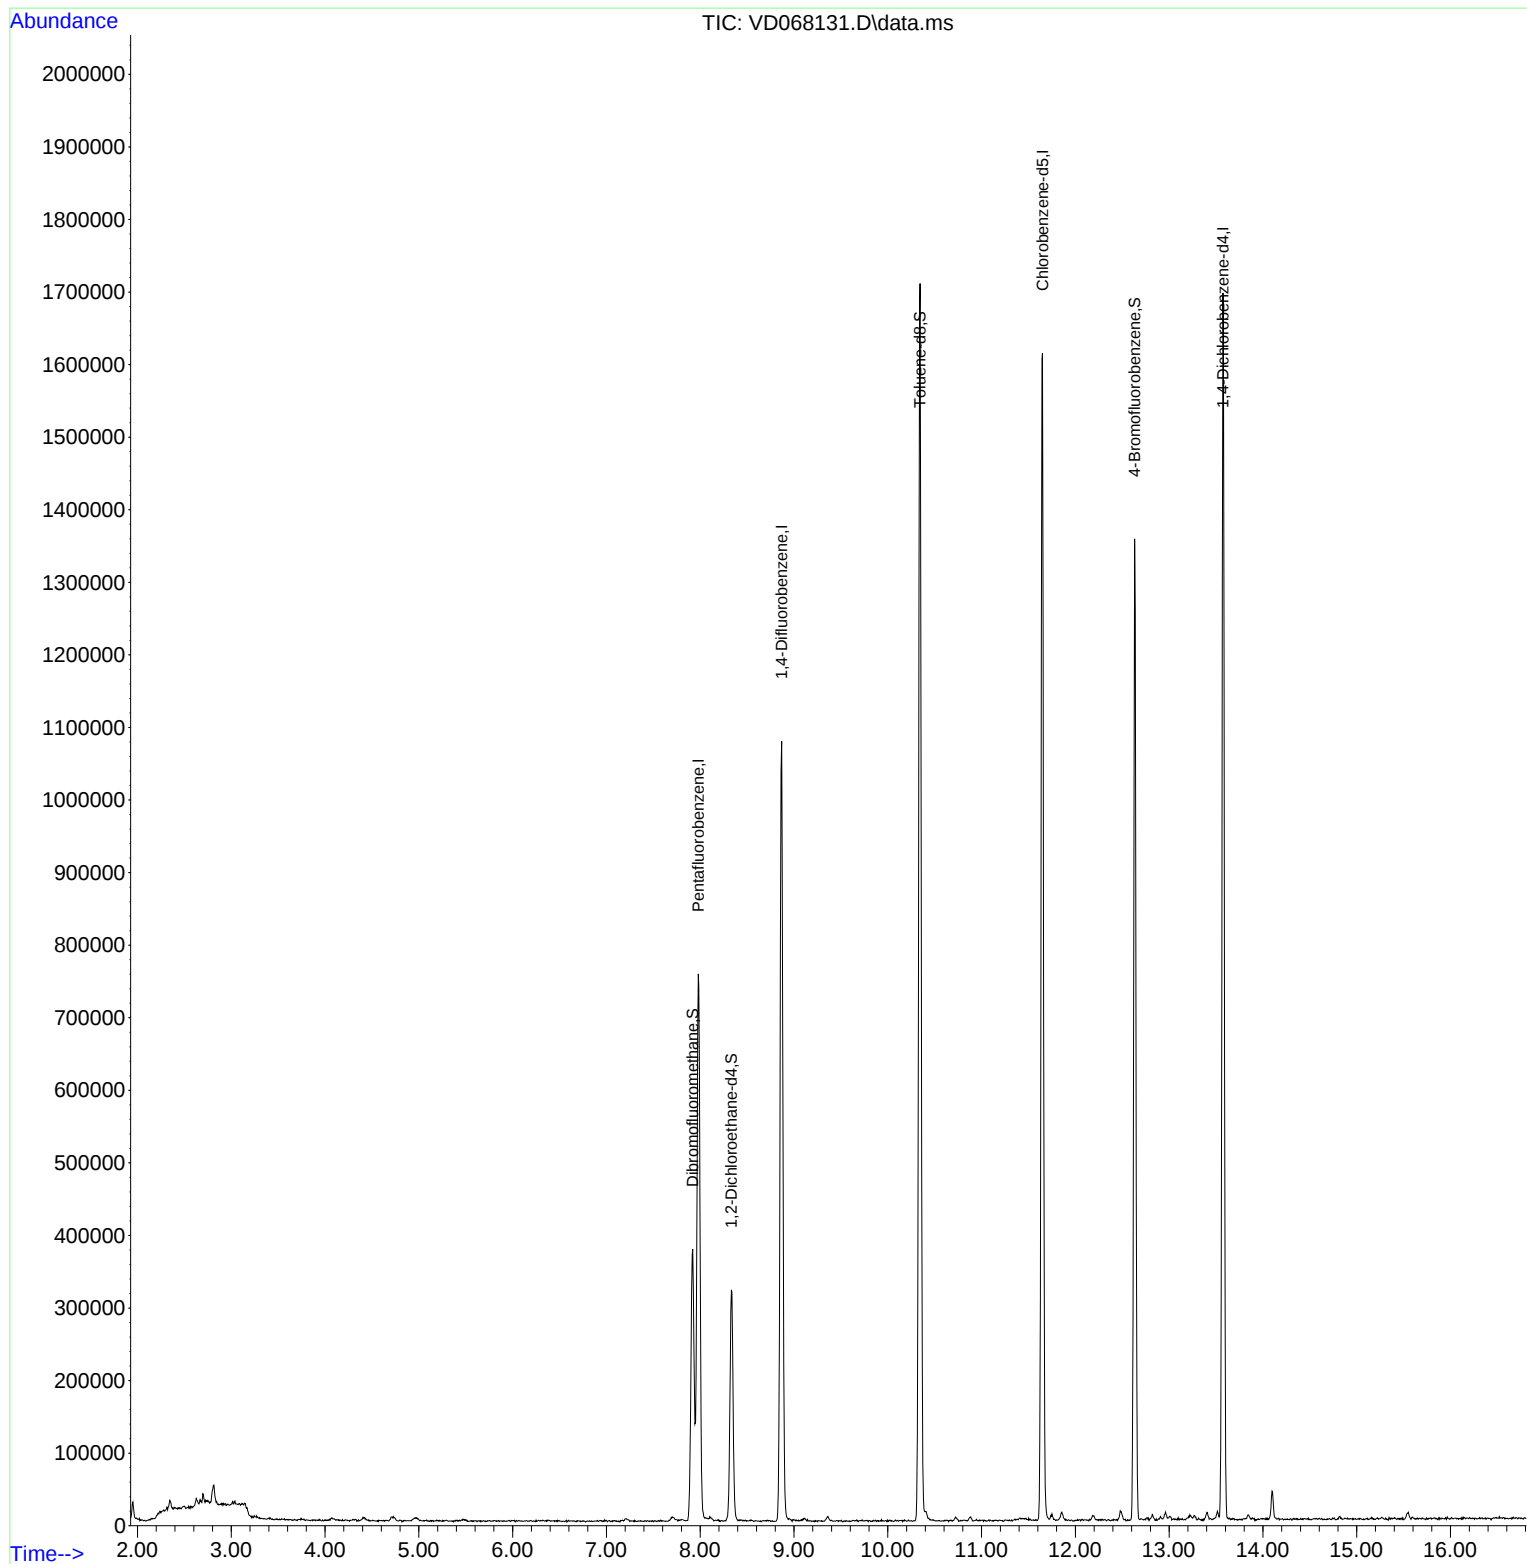


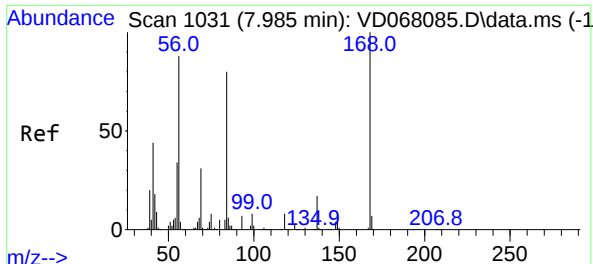

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.006 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31




Instrument :
MSVOA_D
ClientSampleId :
FK-EF-01-017-ABCD


Tgt Ion:168 Resp: 575781
Ion Ratio Lower Upper
168 100
99 59.2 43.5 65.3

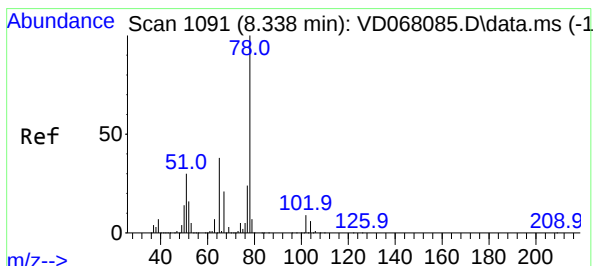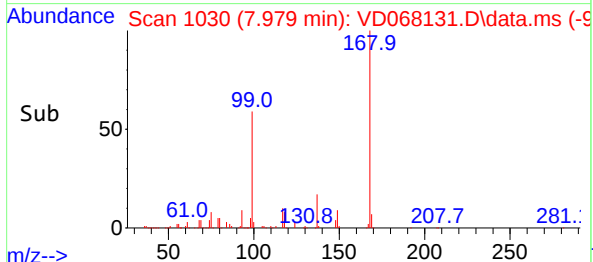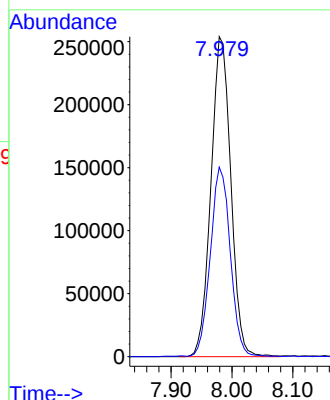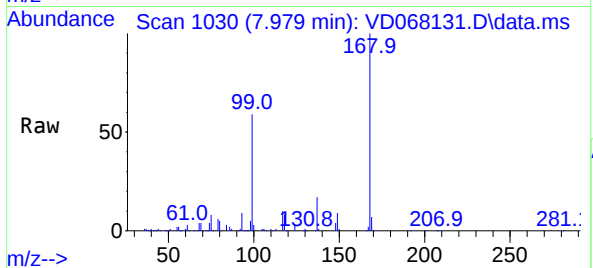

#33
1,2-Dichloroethane-d4
Concen: 47.43 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.005 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31

Tgt Ion: 65 Resp: 261224
Ion Ratio Lower Upper
65 100
67 52.7 0.0 105.0

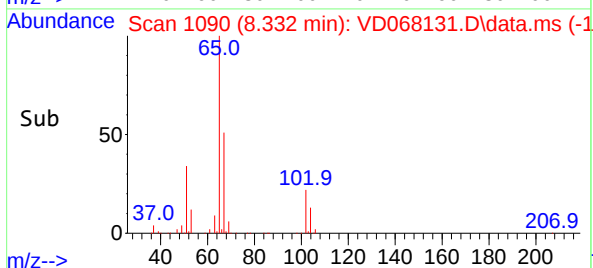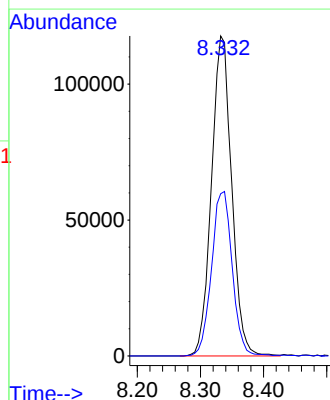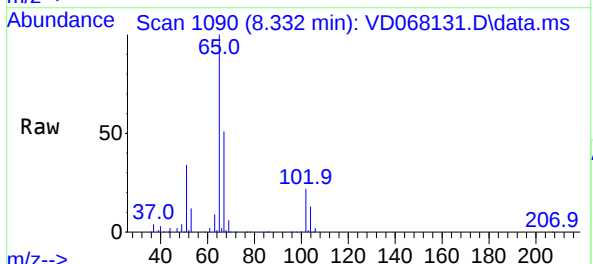




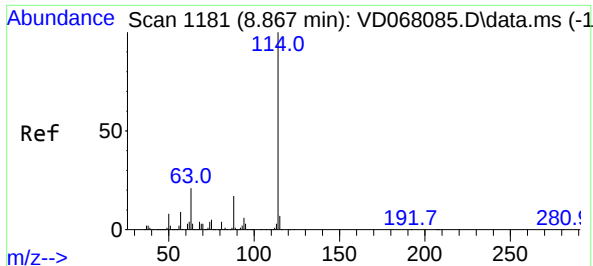


#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31

Instrument :
MSVOA_D
ClientSampleId :
FK-EF-01-017-ABCD

Tgt Ion:114 Resp: 976232




Ion	Ratio	Lower	Upper
114	100		
63	20.2	0.0	34.8
88	15.4	0.0	31.6

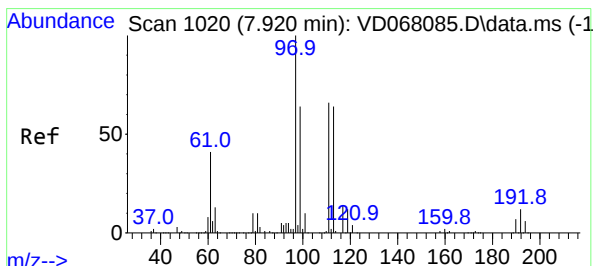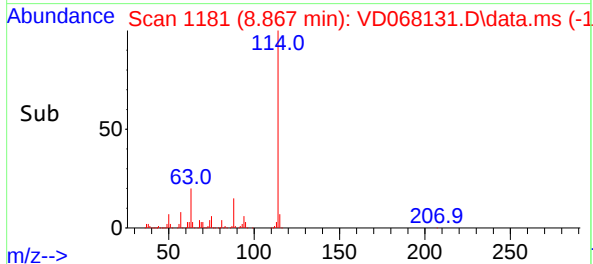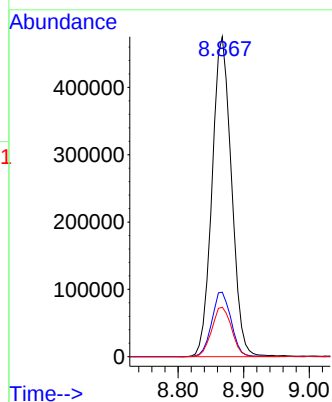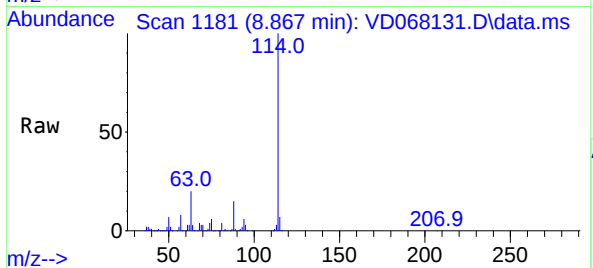


#35
Dibromofluoromethane
Concen: 50.84 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31

Tgt Ion:113 Resp: 274412

Ion	Ratio	Lower	Upper
113	100		
111	103.5	81.4	122.0
192	18.9	16.1	24.1


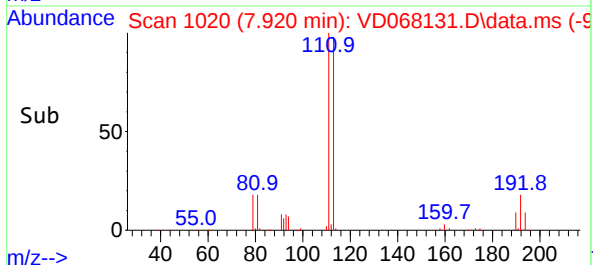
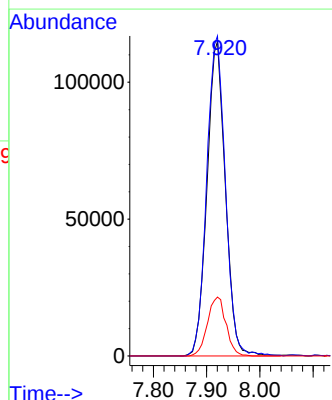
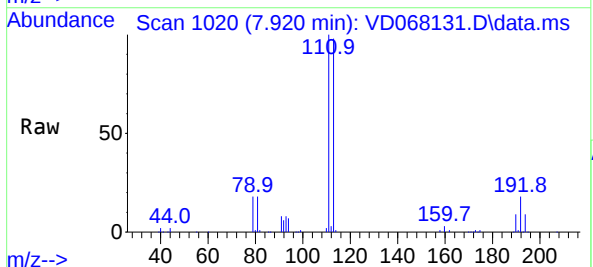


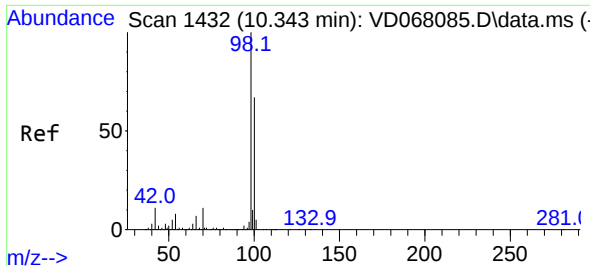

#50
Toluene-d8
Concen: 56.91 ug/l
RT: 10.344 min Scan# 1432
Delta R.T. 0.000 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31




Instrument :
MSVOA_D
ClientSampleId :
FK-EF-01-017-ABCD


Tgt Ion: 98 Resp: 1228646
Ion Ratio Lower Upper
98 100
100 65.3 53.0 79.4

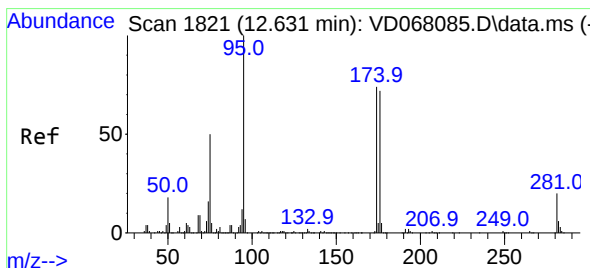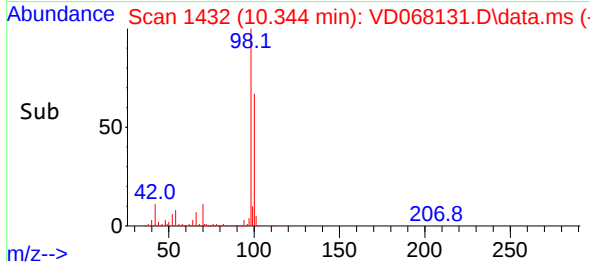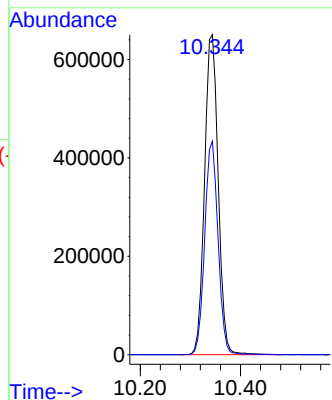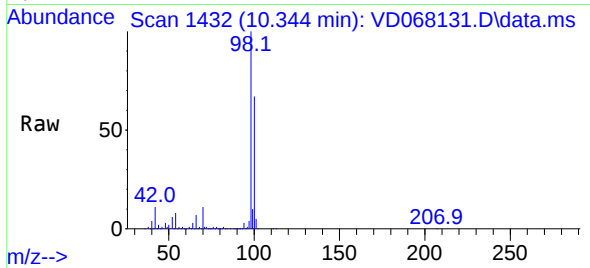

#62
4-Bromofluorobenzene
Concen: 59.88 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31


Tgt Ion: 95 Resp: 465498
Ion Ratio Lower Upper
95 100
174 76.3 0.0 172.4
176 73.8 0.0 168.4

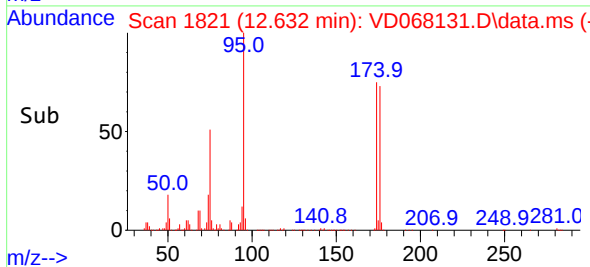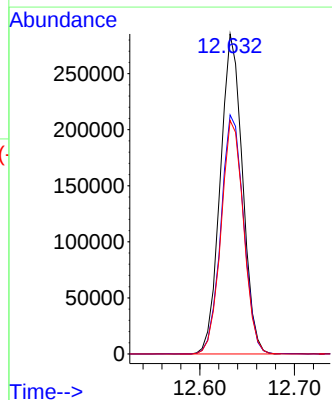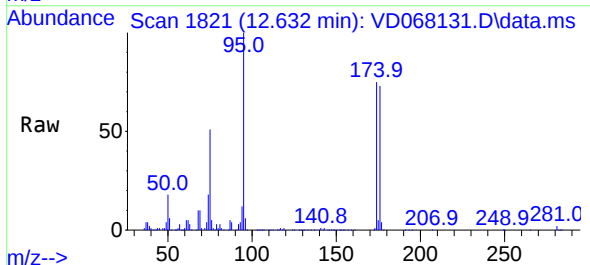



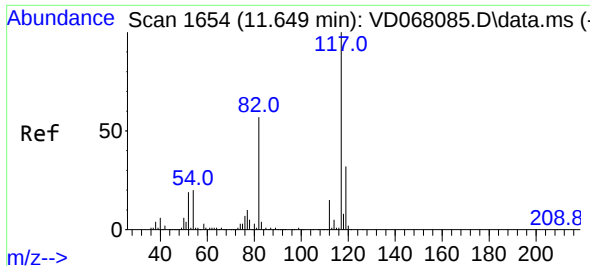


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.650 min Scan# 1654
Delta R.T. 0.001 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31


Instrument :
MSVOA_D
ClientSampleId :
FK-EF-01-017-ABCD

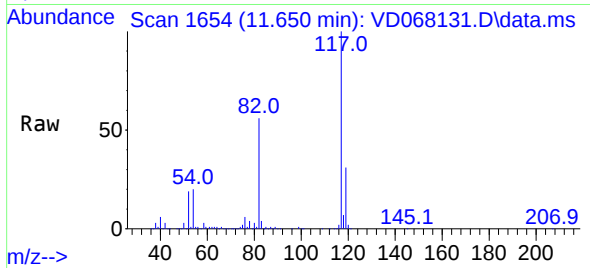

Tgt Ion:117 Resp: 968113
Ion Ratio Lower Upper
117 100
82 56.0 41.4 62.0
119 31.2 26.1 39.1

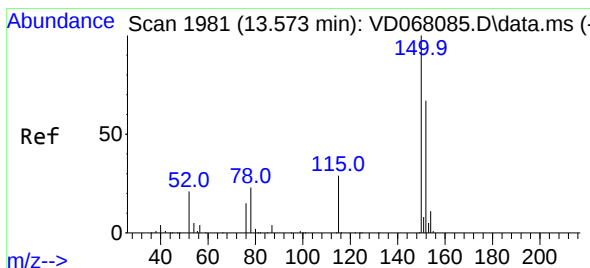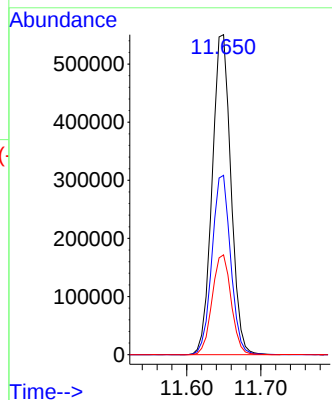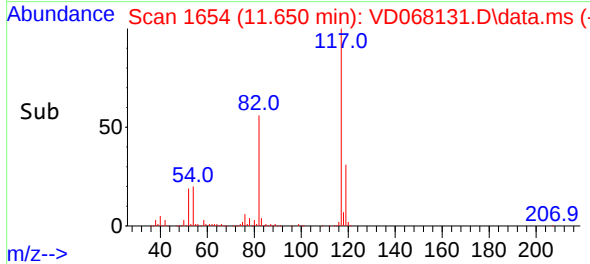

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.000 min
Lab File: VD068131.D
Acq: 21 Jan 2021 14:31

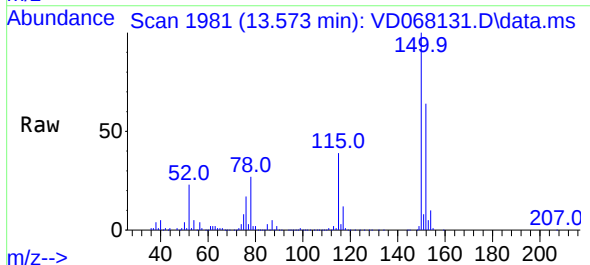

Tgt Ion:152 Resp: 457494
Ion Ratio Lower Upper
152 100
115 60.2 28.9 86.8
150 157.5 0.0 344.4

