
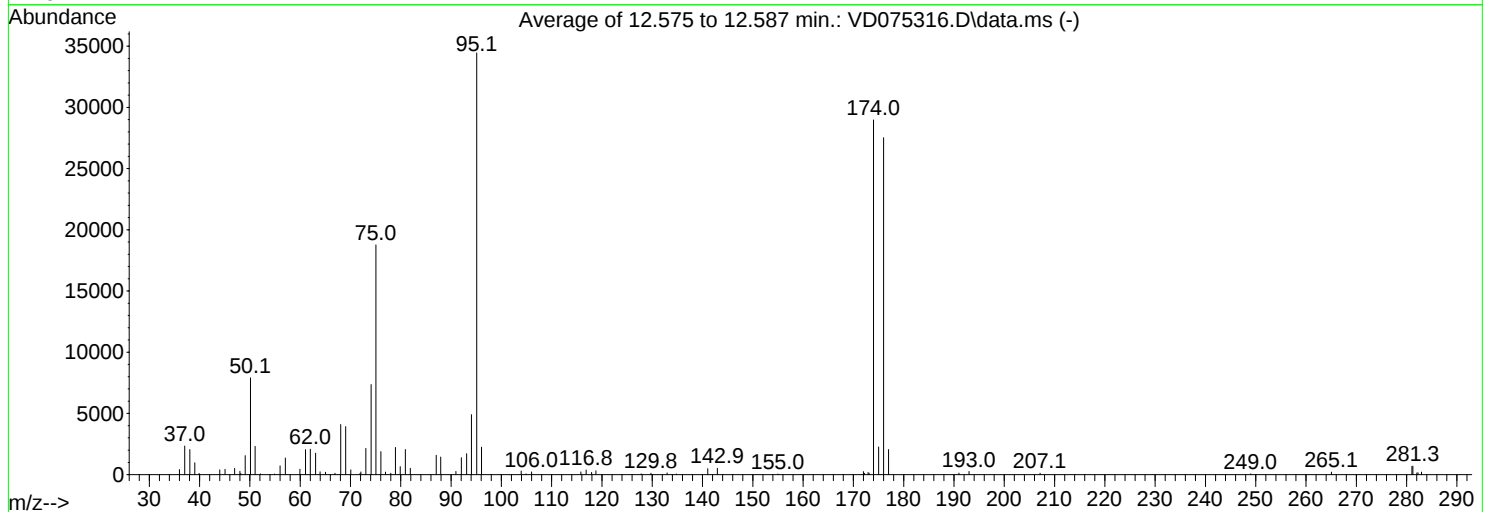


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021323\
Data File : VD075316.D
Acq On : 13 Feb 2023 08:50
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020723S.M
Title : SW846 8260
Last Update : Wed Feb 08 04:26:58 2023

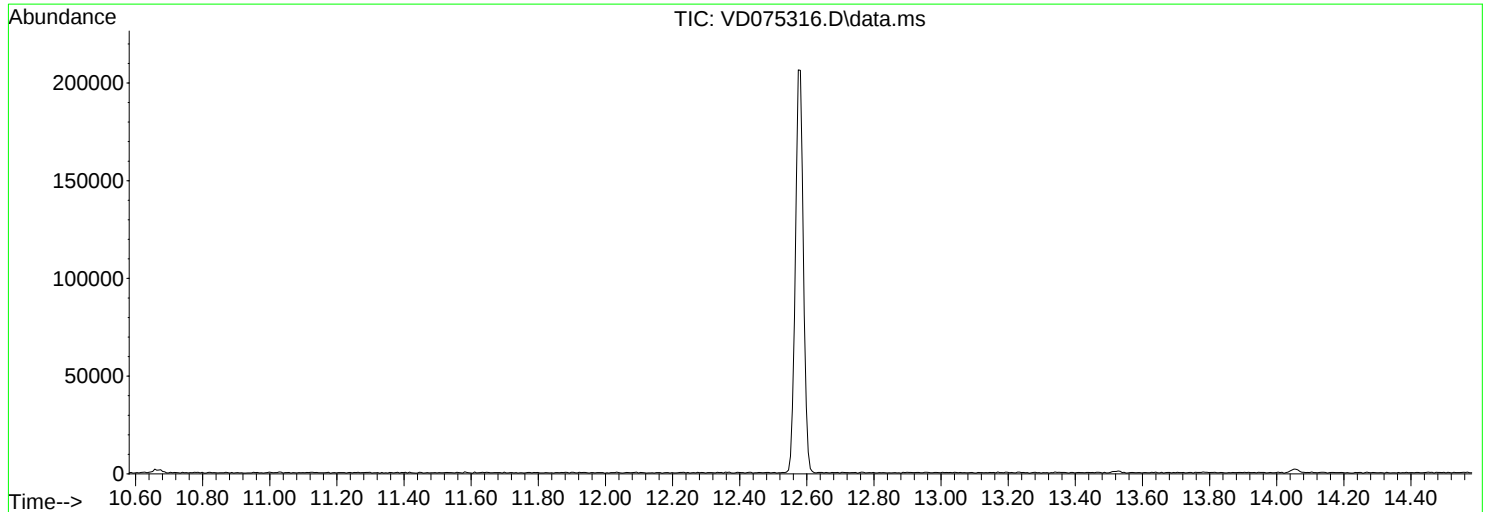

AutoFind: Scans 1868, 1869, 1870; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	7909	PASS
75	95	30	60	54.5	18771	PASS
95	95	100	100	100.0	34456	PASS
96	95	5	9	6.5	2253	PASS
173	174	0.00	2	0.6	172	PASS
174	95	50	100	84.1	28973	PASS
175	174	5	9	7.8	2269	PASS
176	174	95	101	95.0	27520	PASS
177	176	5	9	7.4	2046	PASS