
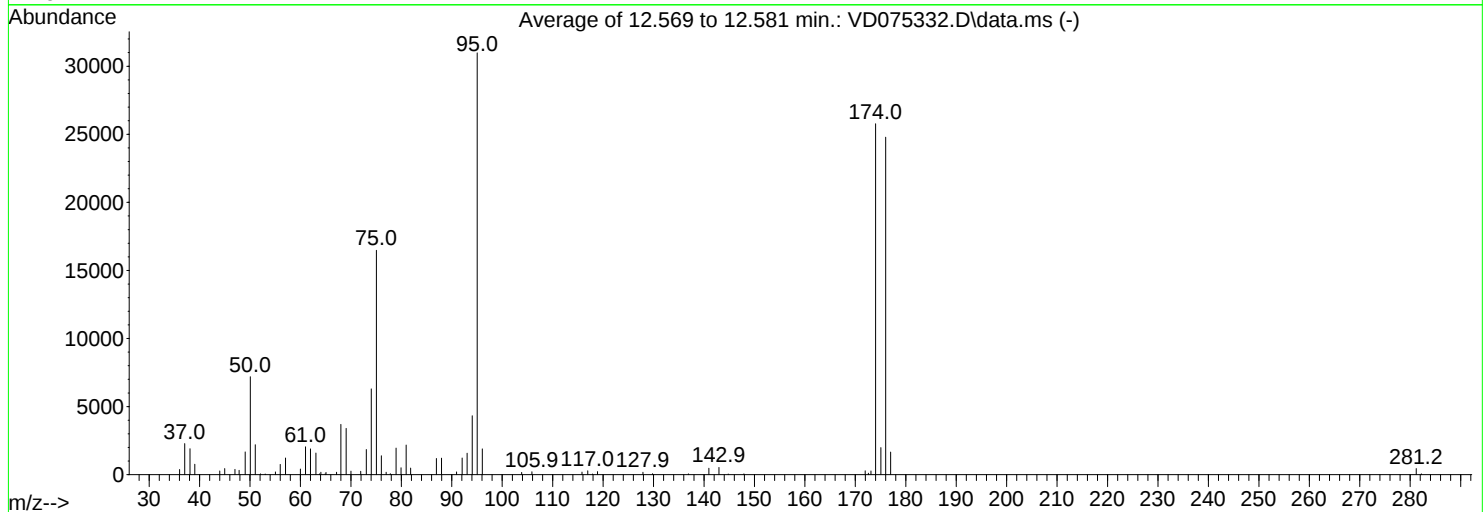


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD021423\
Data File : VD075332.D
Acq On : 14 Feb 2023 09:25
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D020723S.M
Title : SW846 8260
Last Update : Wed Feb 08 04:26:58 2023

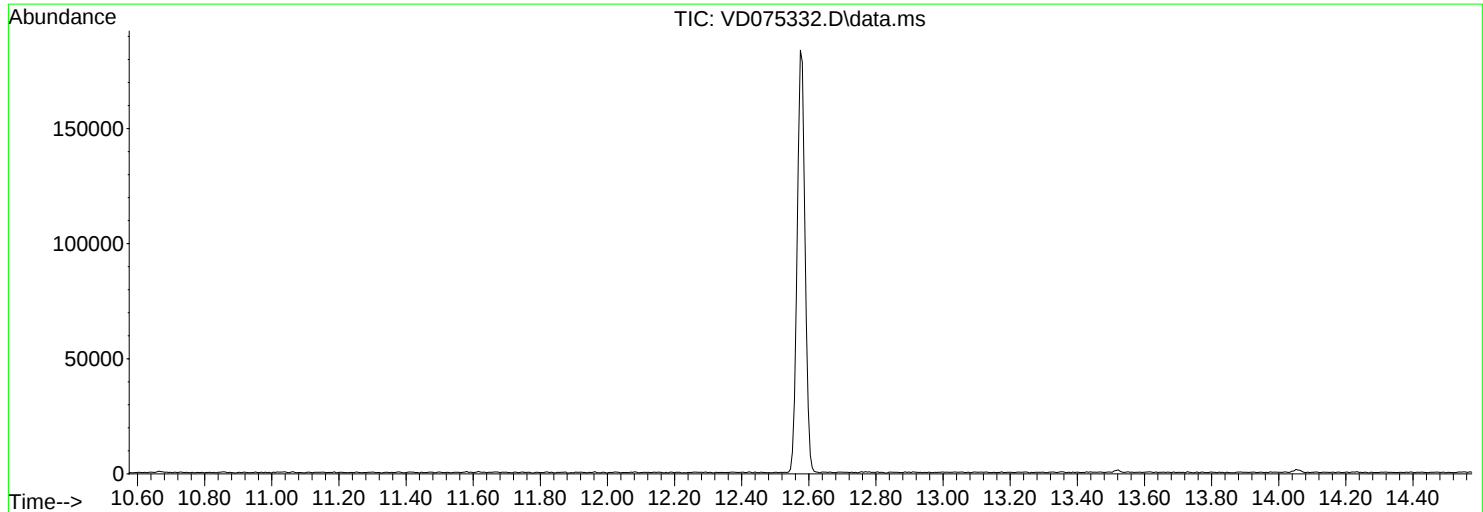

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	7195	PASS
75	95	30	60	53.2	16482	PASS
95	95	100	100	100.0	30984	PASS
96	95	5	9	6.1	1892	PASS
173	174	0.00	2	1.1	273	PASS
174	95	50	100	83.2	25776	PASS
175	174	5	9	7.7	1987	PASS
176	174	95	101	96.2	24787	PASS
177	176	5	9	6.7	1652	PASS