
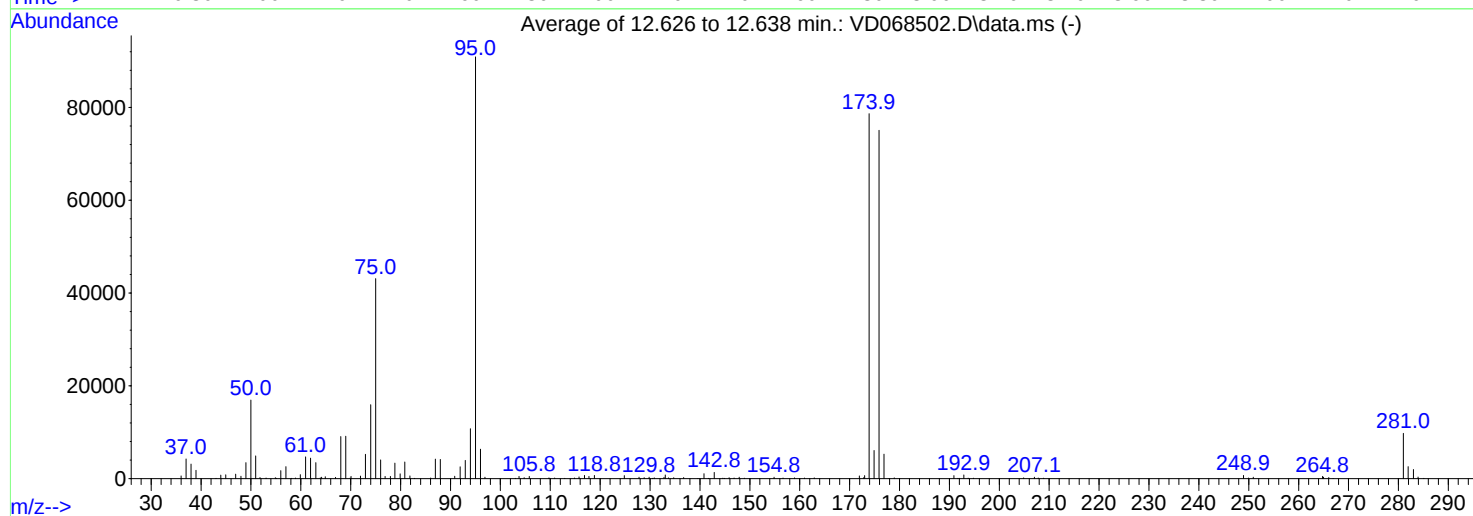


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030321\
 Data File : VD068502.D
 Acq On : 03 Mar 2021 08:36
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Title : SW846 8260
 Last Update : Fri Feb 26 14:04:14 2021

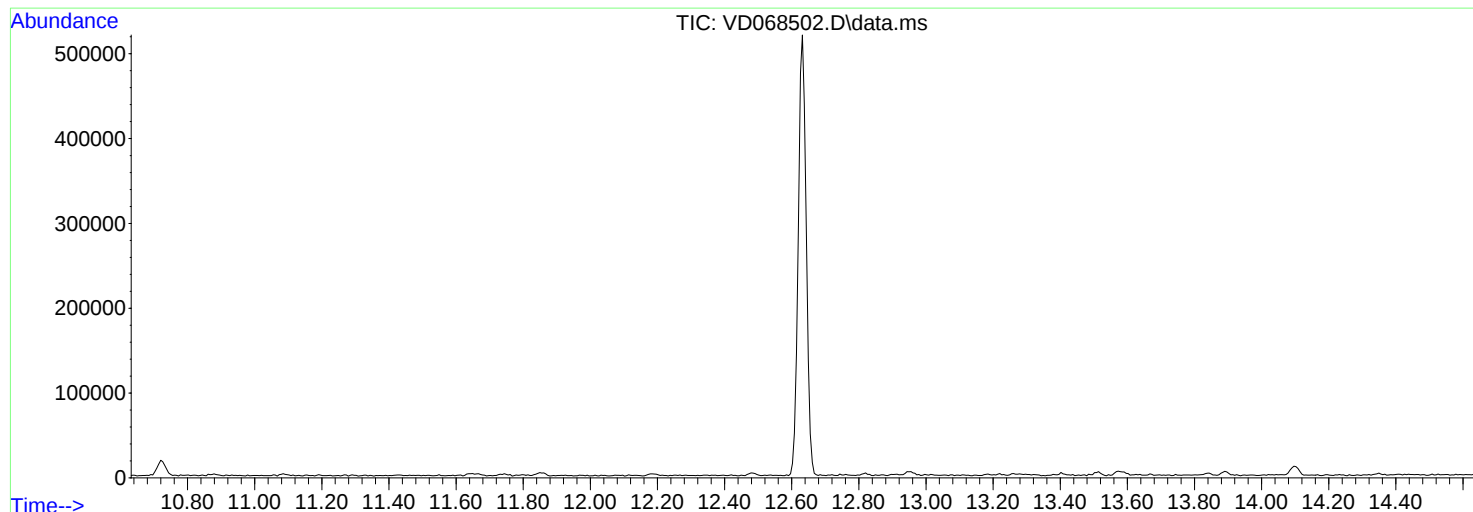

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	16930	PASS
75	95	30	60	47.4	43120	PASS
95	95	100	100	100.0	90907	PASS
96	95	5	9	7.0	6338	PASS
173	174	0.00	2	0.8	655	PASS
174	95	50	100	86.5	78648	PASS
175	174	5	9	7.7	6064	PASS
176	174	95	101	95.4	75064	PASS
177	176	5	9	7.1	5294	PASS