


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD030519\
Data File : VD060940.D
Acq On : 5 Mar 2019 9:57
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D030119S.M
Title : SW846 8260
Last Update : Sat Mar 02 01:28:28 2019

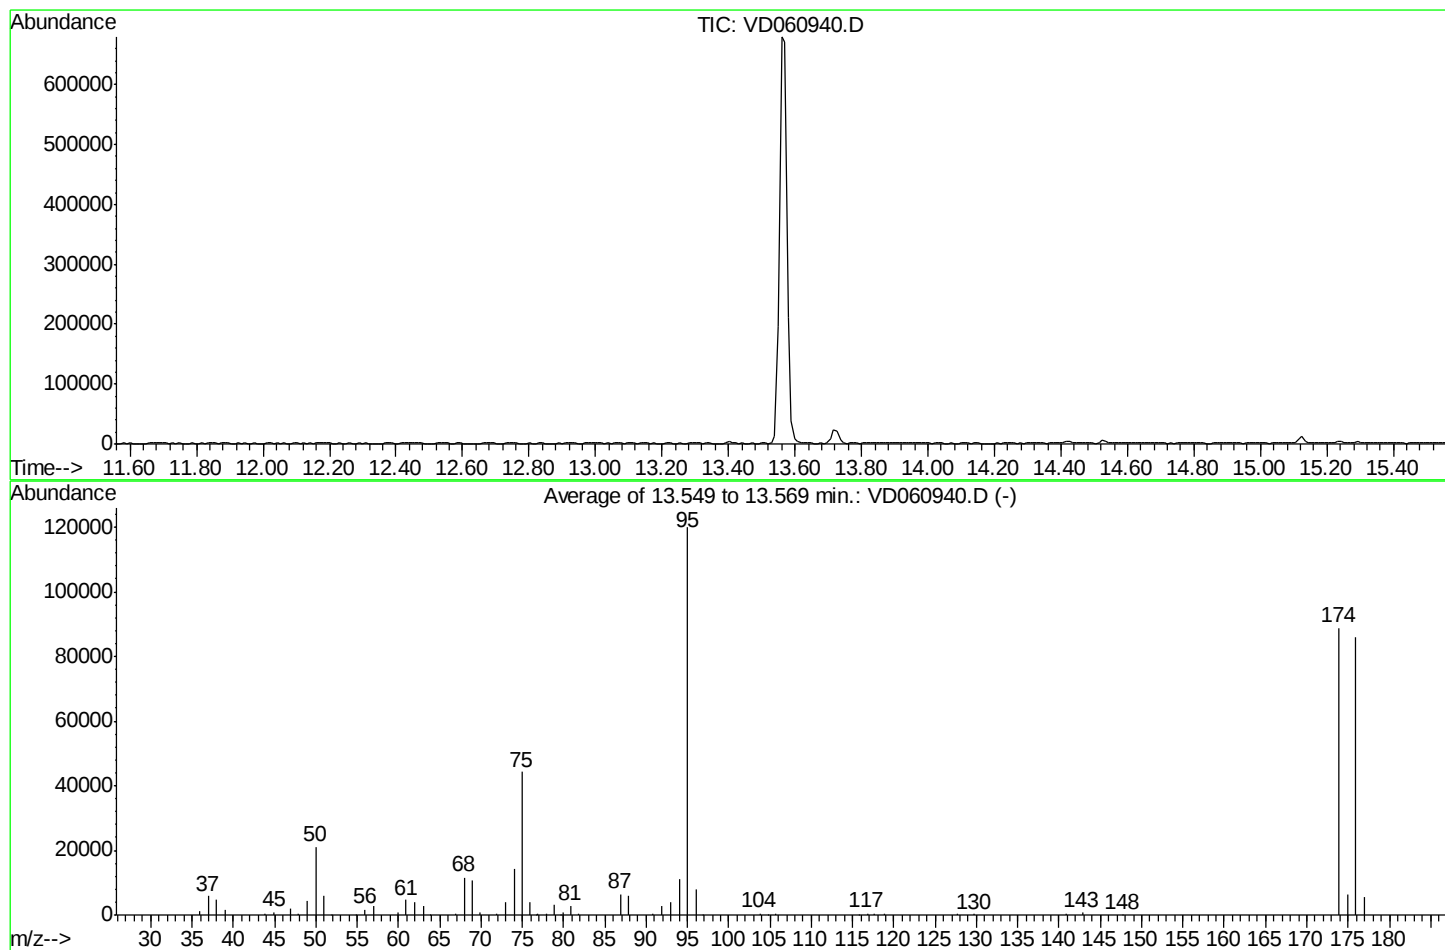

AutoFind: Scans 1232, 1233, 1234; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	21098	PASS
75	95	30	60	36.8	44178	PASS
95	95	100	100	100.0	119941	PASS
96	95	5	9	6.5	7765	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.0	88744	PASS
175	174	5	9	7.3	6493	PASS
176	174	95	101	96.8	85941	PASS
177	176	5	9	6.3	5408	PASS