

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030821\
 Data File : VD068553.D
 Acq On : 08 Mar 2021 11:32
 Operator : VA/SY
 Sample : VD0308SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0308SBL01

Quant Time: Mar 09 00:08:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 26 14:04:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.985	168	390588	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	662498	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	633625	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	291473	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	185088	47.43	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 94.86%			
35) Dibromofluoromethane	7.920	113	202016	50.62	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 101.24%			
50) Toluene-d8	10.338	98	832300	52.36	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 104.72%			
62) 4-Bromofluorobenzene	12.632	95	271132	52.92	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 105.84%			
Target Compounds						
					Qvalue	
10) Methyl Iodide	4.309	142	1265	2.87	ug/l #	68
16) Acetone	4.167	43	1434	2.31	ug/l #	57
20) Methylene Chloride	4.979	84	9462	Below Cal	#	81
31) Cyclohexane	7.979	56	9827	1.38	ug/l #	14
76) 1,2,3-Trichloropropane	12.632	75	134412	51.95	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.632	75	134412	121.22	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030821\
Data File : VD068553.D
Acq On : 08 Mar 2021 11:32
Operator : VA/SY
Sample : VD0308SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01

Quant Time: Mar 09 00:08:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Quant Title : SW846 8260
QLast Update : Fri Feb 26 14:04:14 2021
Response via : Initial Calibration




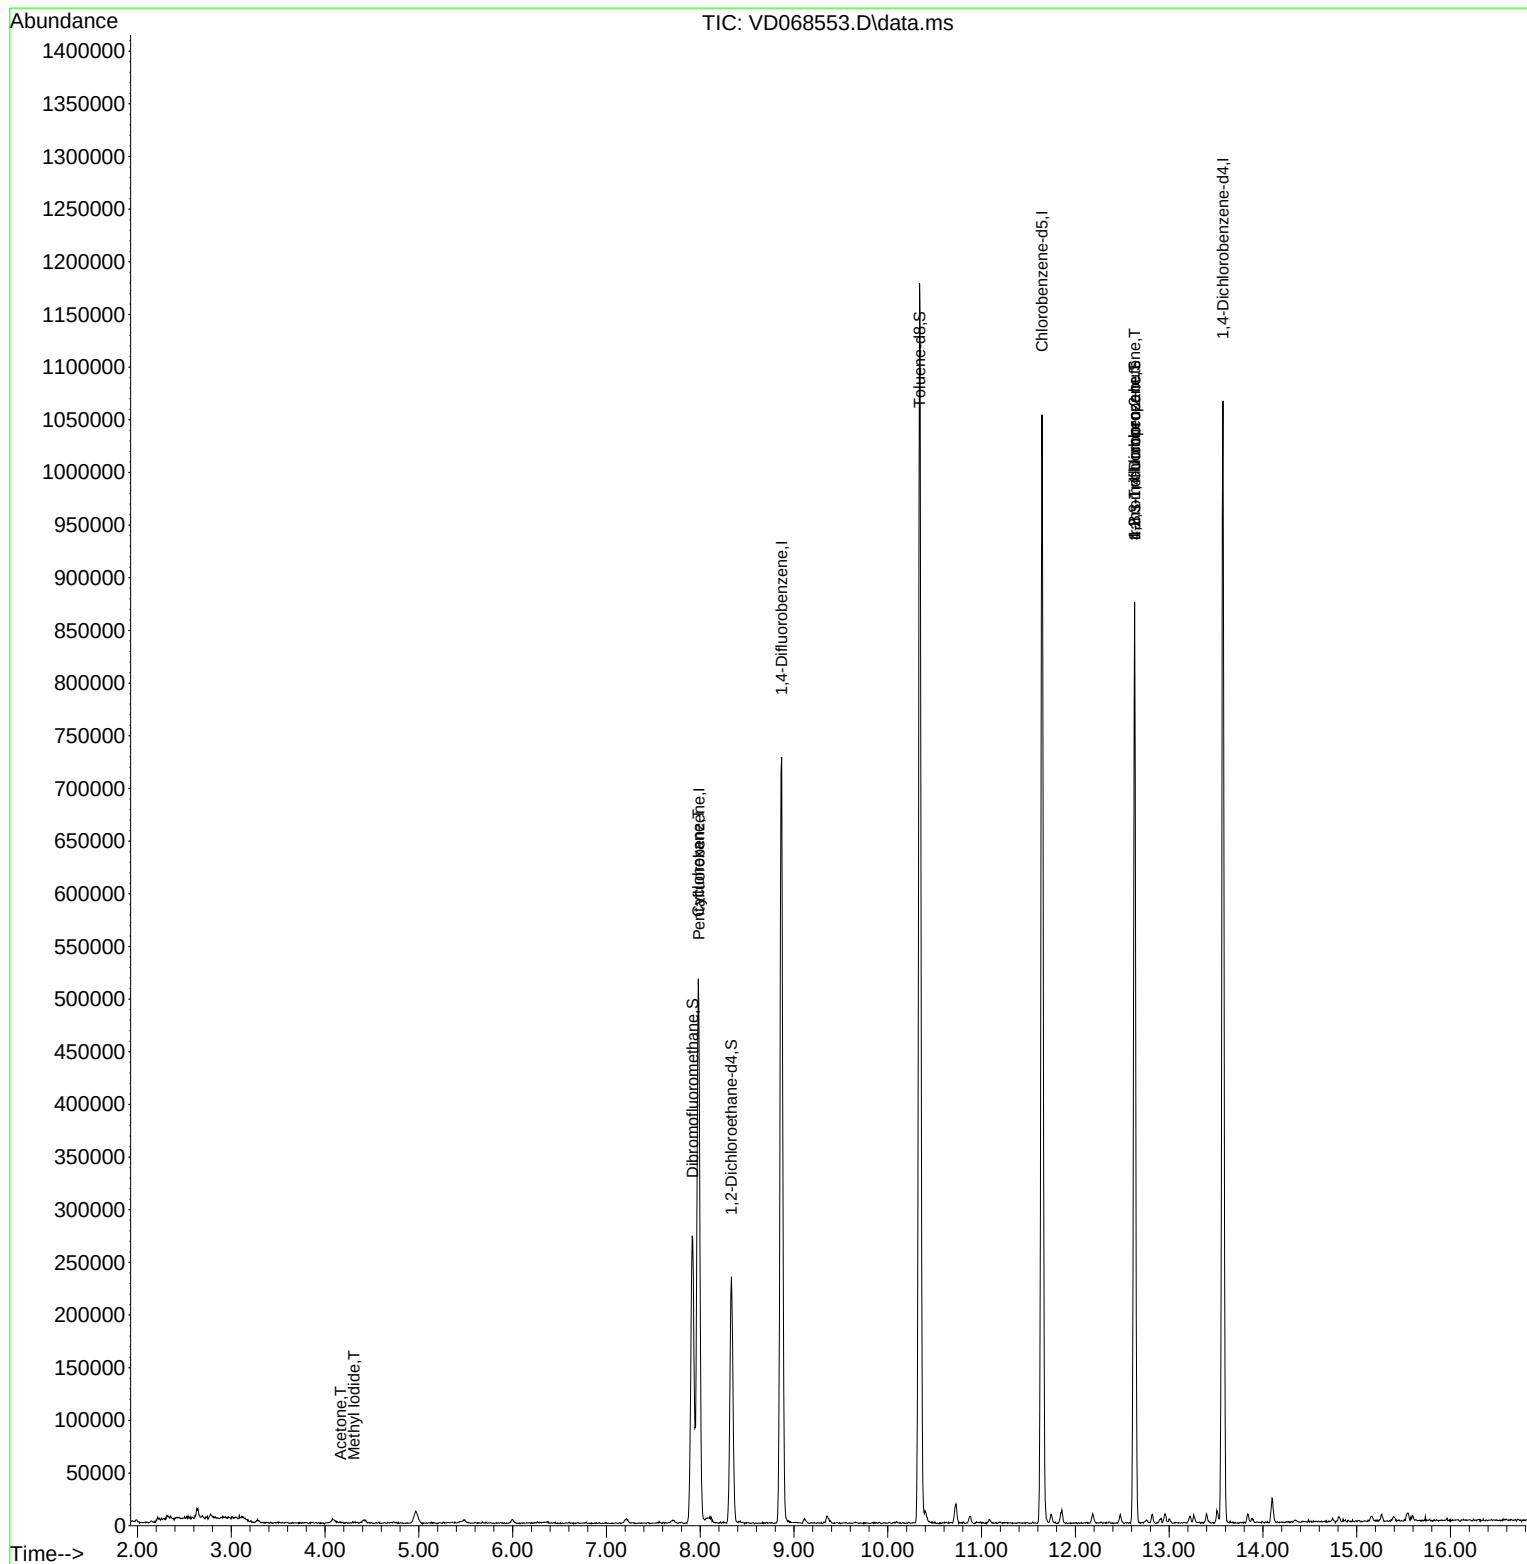


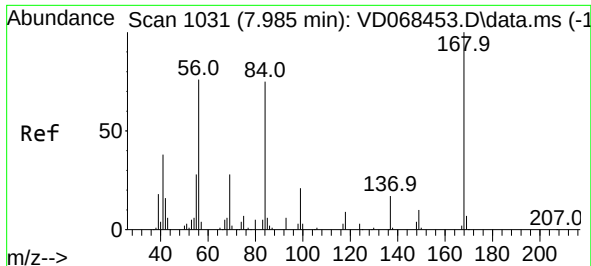

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.985 min Scan# 1031
Delta R.T. -0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion:168 Resp: 390588
Ion Ratio Lower Upper
168 100
99 52.4 43.5 65.3

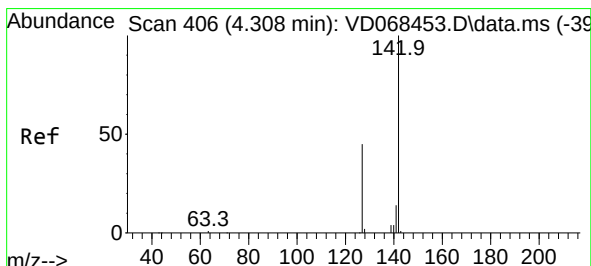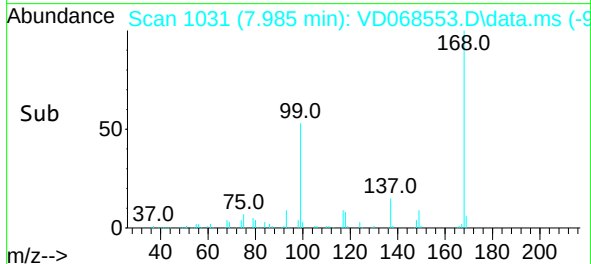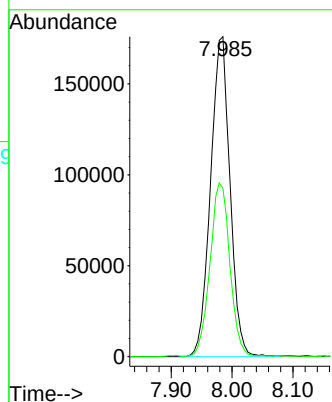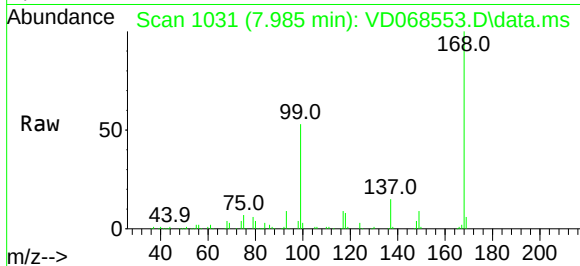

#10
Methyl Iodide
Concen: 2.87 ug/l
RT: 4.309 min Scan# 406
Delta R.T. 0.001 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion:142 Resp: 1265
Ion Ratio Lower Upper
142 100
127 26.5 37.9 56.9#
141 0.0 11.5 17.3#


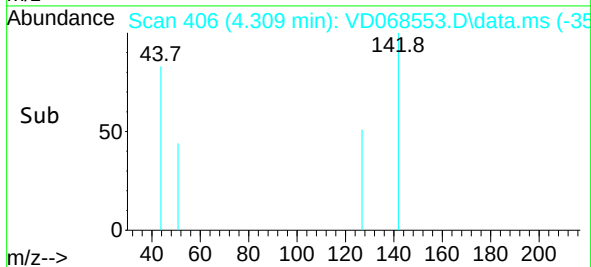
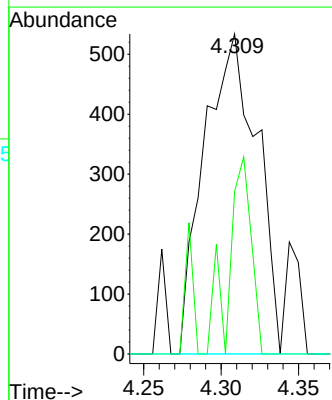
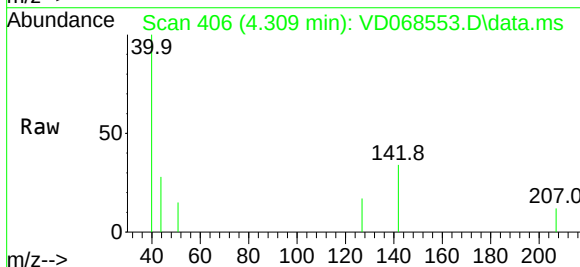


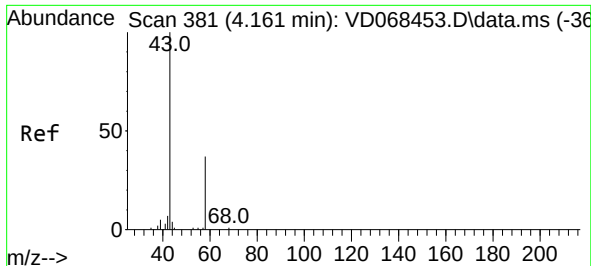

#16
Acetone
Concen: 2.31 ug/l
RT: 4.167 min Scan# 382
Delta R.T. 0.006 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion: 43 Resp: 1434
Ion Ratio Lower Upper
43 100
58 53.8 24.2 36.4#

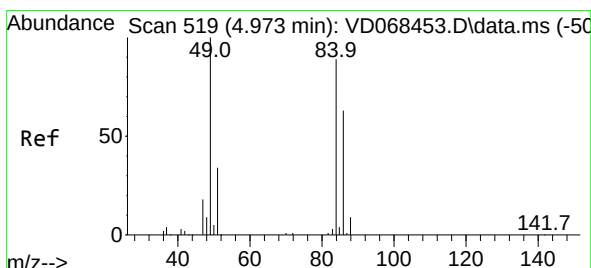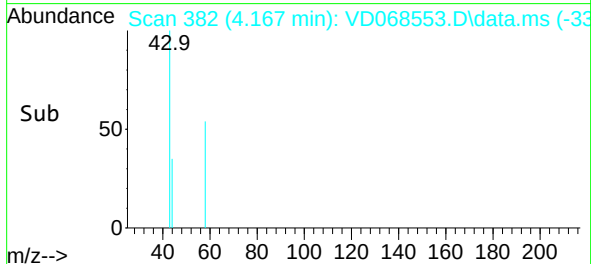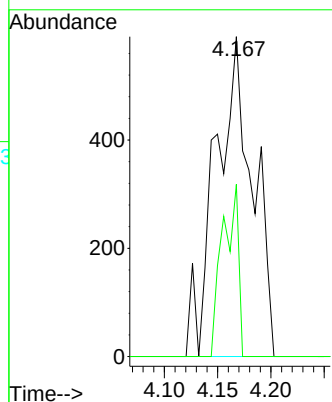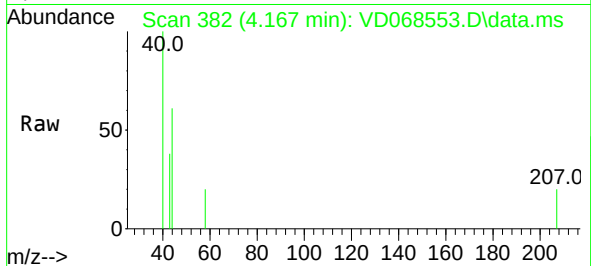

#20
Methylene Chloride
Concen: Below Cal
RT: 4.979 min Scan# 520
Delta R.T. 0.006 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion: 84 Resp: 9462
Ion Ratio Lower Upper
84 100
49 71.9 77.4 116.2#
51 23.0 26.1 39.1#
86 55.4 51.8 77.8


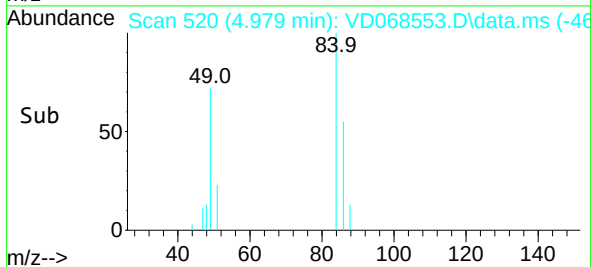
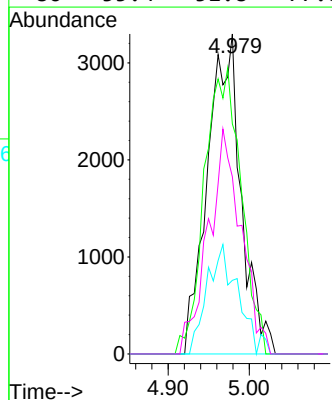
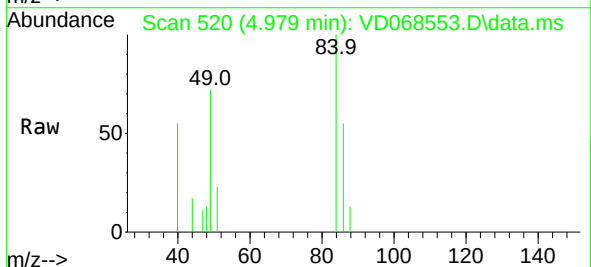


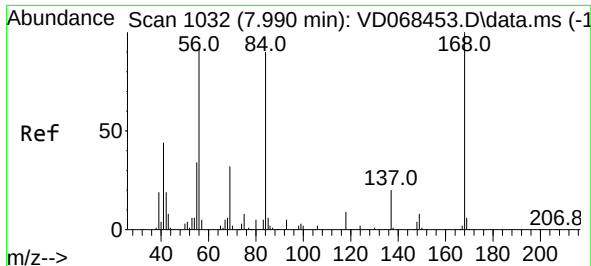

#31
Cyclohexane
Concen: 1.38 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.011 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion: 56 Resp: 9827
Ion Ratio Lower Upper
56 100
69 125.4 30.1 45.1#
84 166.8 82.1 123.1#

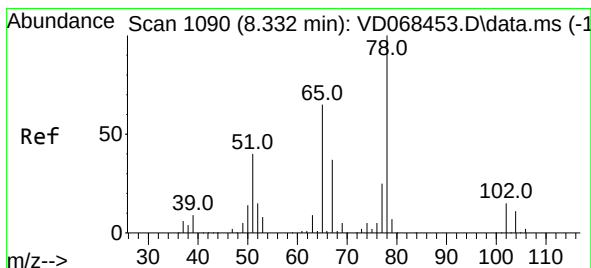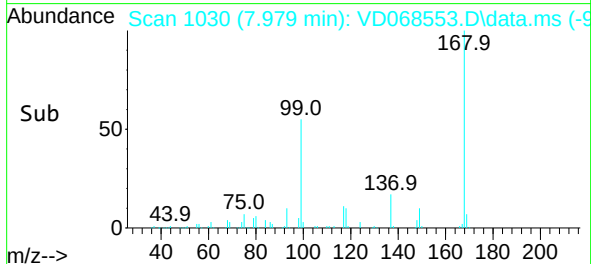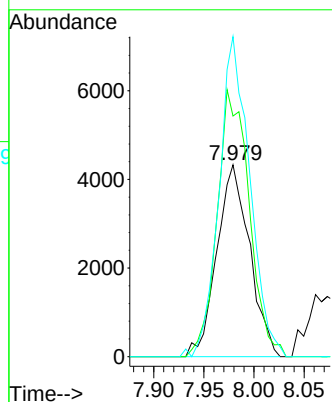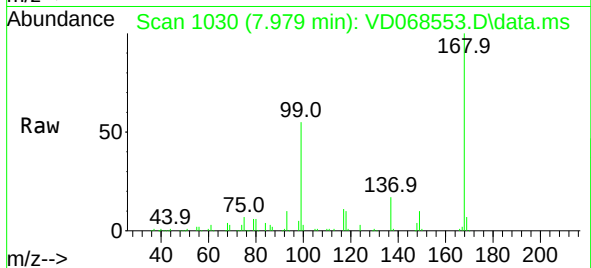

#33
1,2-Dichloroethane-d4
Concen: 47.43 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. 0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion: 65 Resp: 185088
Ion Ratio Lower Upper
65 100
67 55.0 0.0 105.0


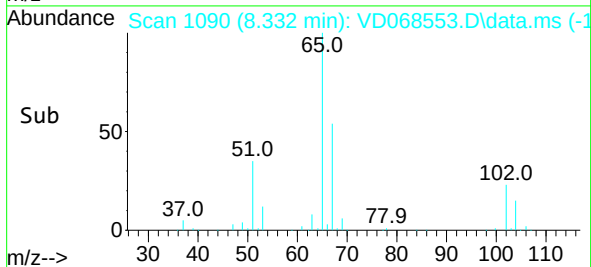
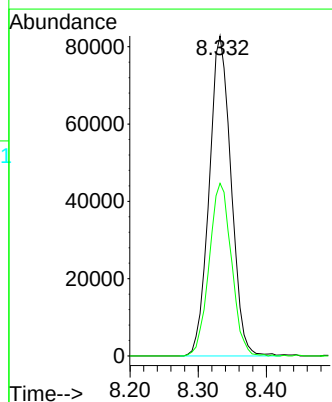
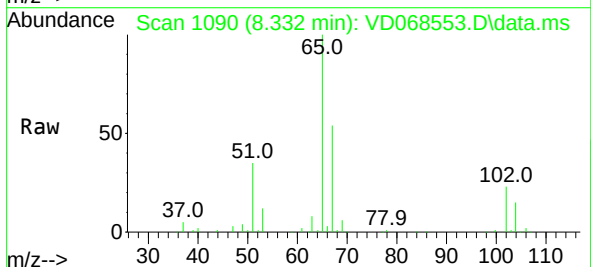


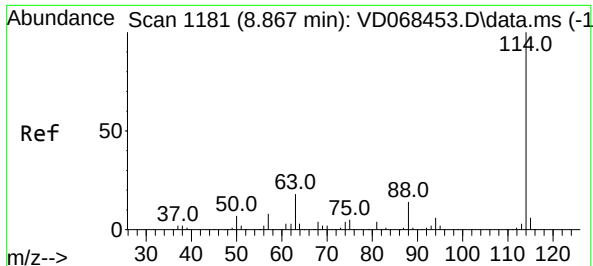

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion:114 Resp: 662498
Ion Ratio Lower Upper
114 100
63 17.7 0.0 34.8
88 15.5 0.0 31.6

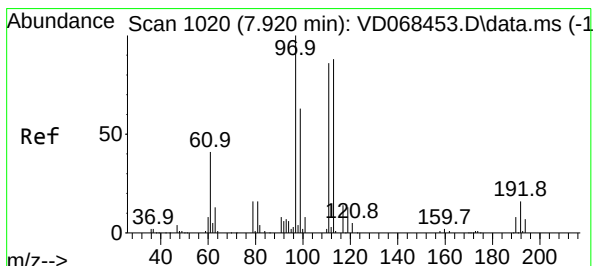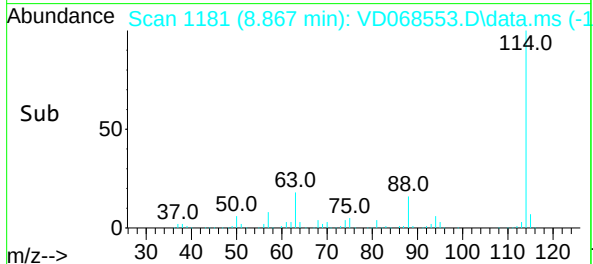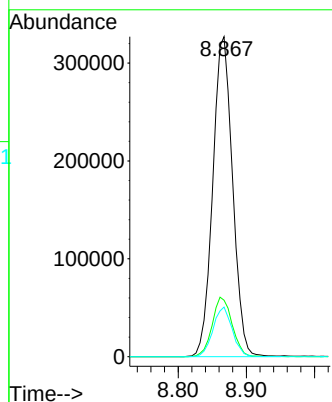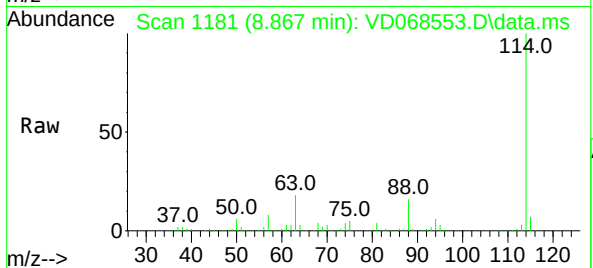

#35
Dibromofluoromethane
Concen: 50.62 ug/l
RT: 7.920 min Scan# 1020
Delta R.T. 0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion:113 Resp: 202016
Ion Ratio Lower Upper
113 100
111 101.4 81.4 122.0
192 19.3 16.1 24.1


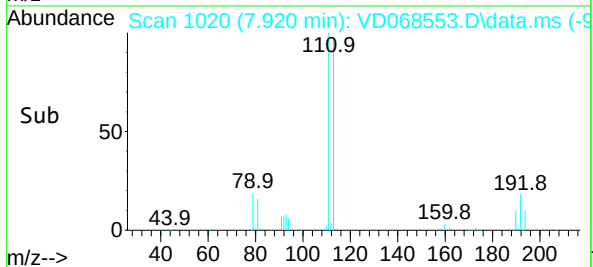
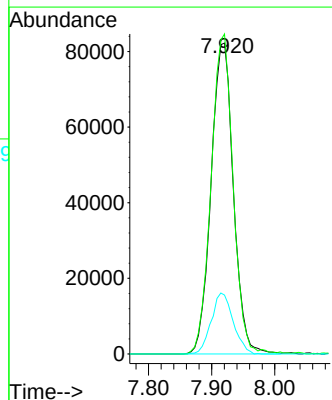
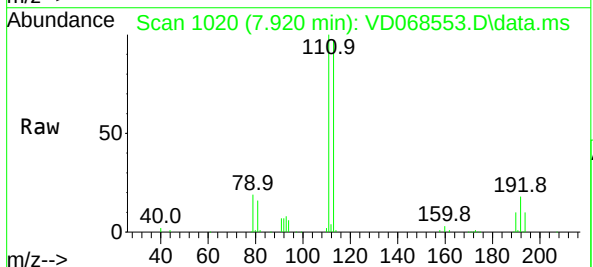


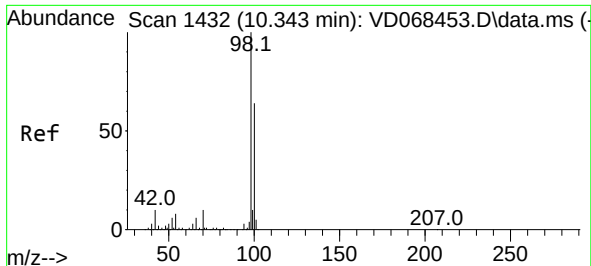

#50
Toluene-d8
Concen: 52.36 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.005 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion: 98 Resp: 832300
Ion Ratio Lower Upper
98 100
100 64.6 53.0 79.4

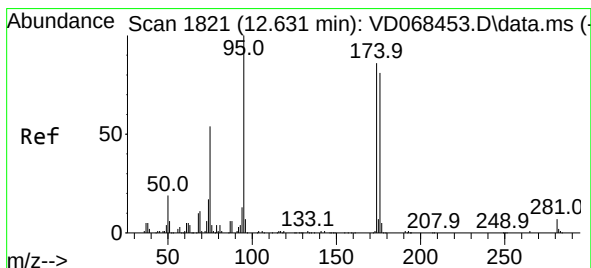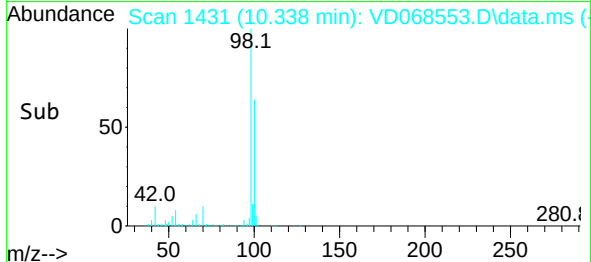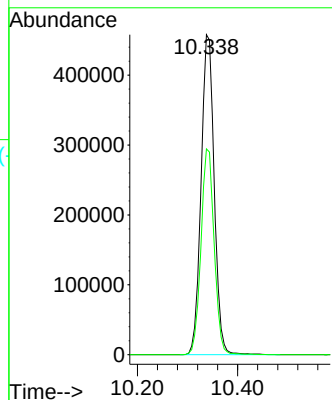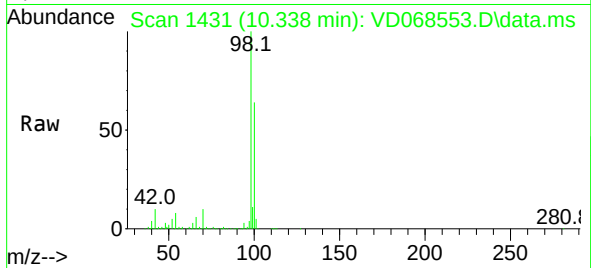

#62
4-Bromofluorobenzene
Concen: 52.92 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion: 95 Resp: 271132
Ion Ratio Lower Upper
95 100
174 84.9 0.0 172.4
176 81.3 0.0 168.4


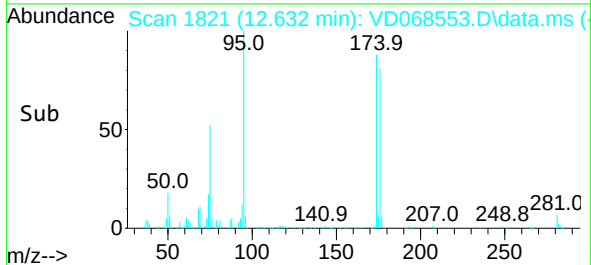
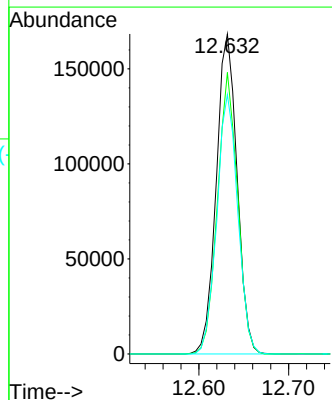
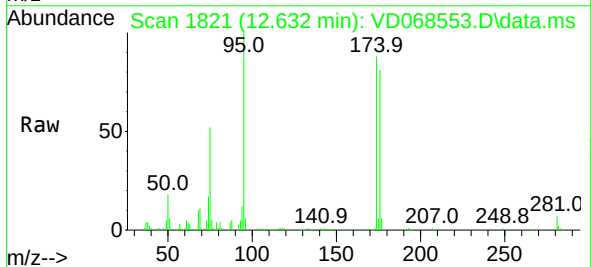


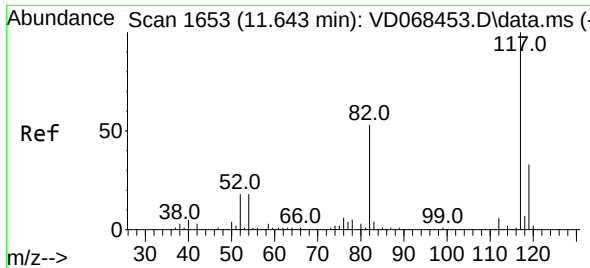

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.000 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32




Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01


Tgt Ion:117 Resp: 633625
Ion Ratio Lower Upper
117 100
82 52.5 41.4 62.0
119 31.9 26.1 39.1

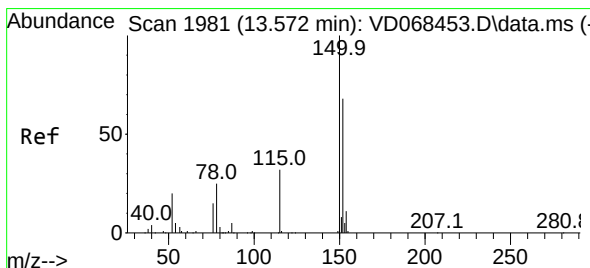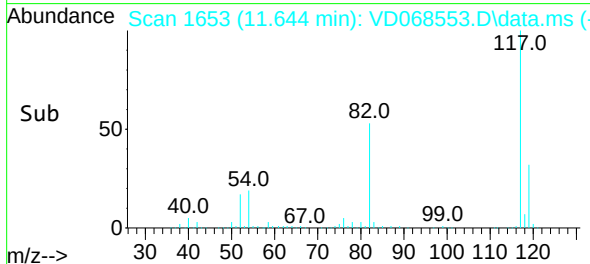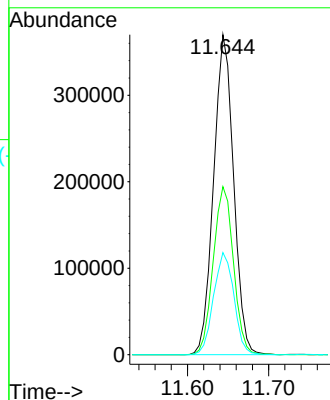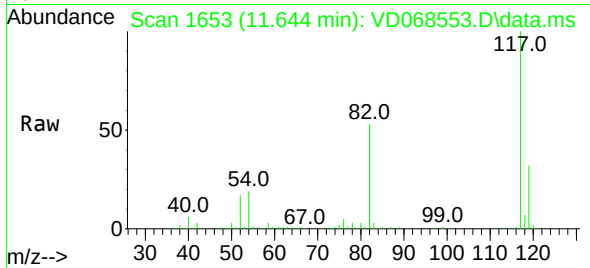

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. 0.001 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion:152 Resp: 291473
Ion Ratio Lower Upper
152 100
115 57.9 28.9 86.8
150 157.7 0.0 344.4


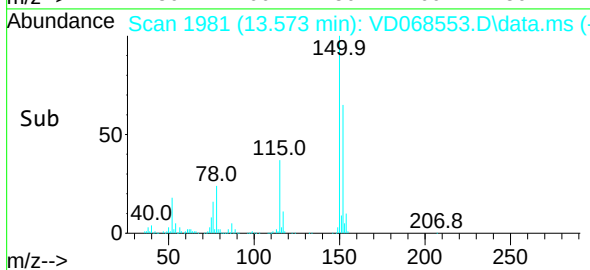
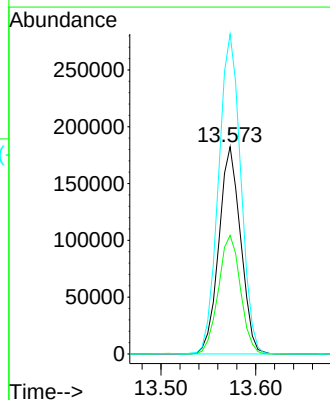
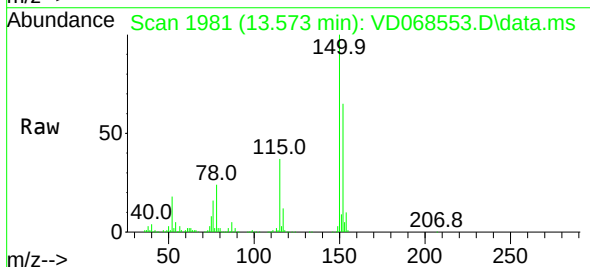


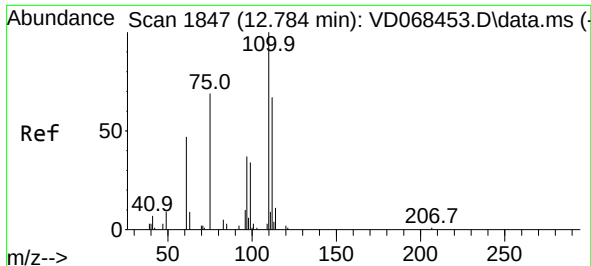

#76
1,2,3-Trichloropropane
Concen: 51.95 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.152 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Instrument :
MSVOA_D
ClientSampleId :
VD0308SBL01

Tgt Ion: 75 Resp: 134412
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

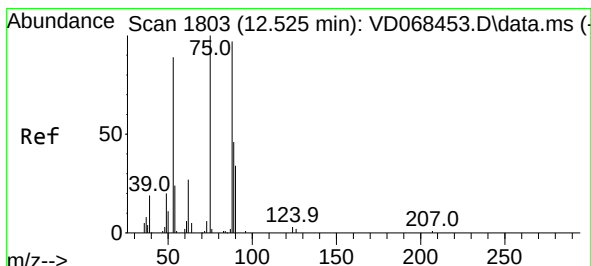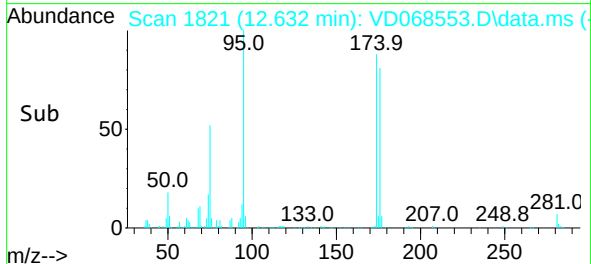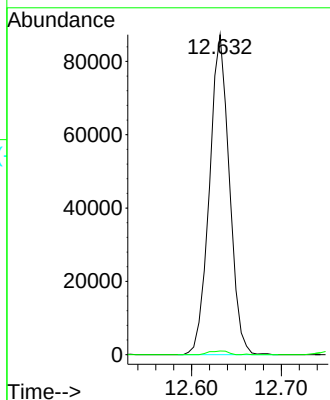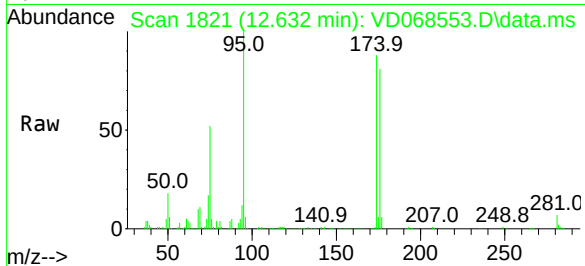

#81
trans-1,4-Dichloro-2-butene
Concen: 121.22 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. 0.106 min
Lab File: VD068553.D
Acq: 08 Mar 2021 11:32

Tgt Ion: 75 Resp: 134412
Ion Ratio Lower Upper
75 100
53 0.1 70.2 105.2#
89 0.0 40.3 60.5#

