


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD030821\
Data File : VD068551.D
Acq On : 08 Mar 2021 10:21
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D022621S.M
Title : SW846 8260
Last Update : Fri Feb 26 14:04:14 2021

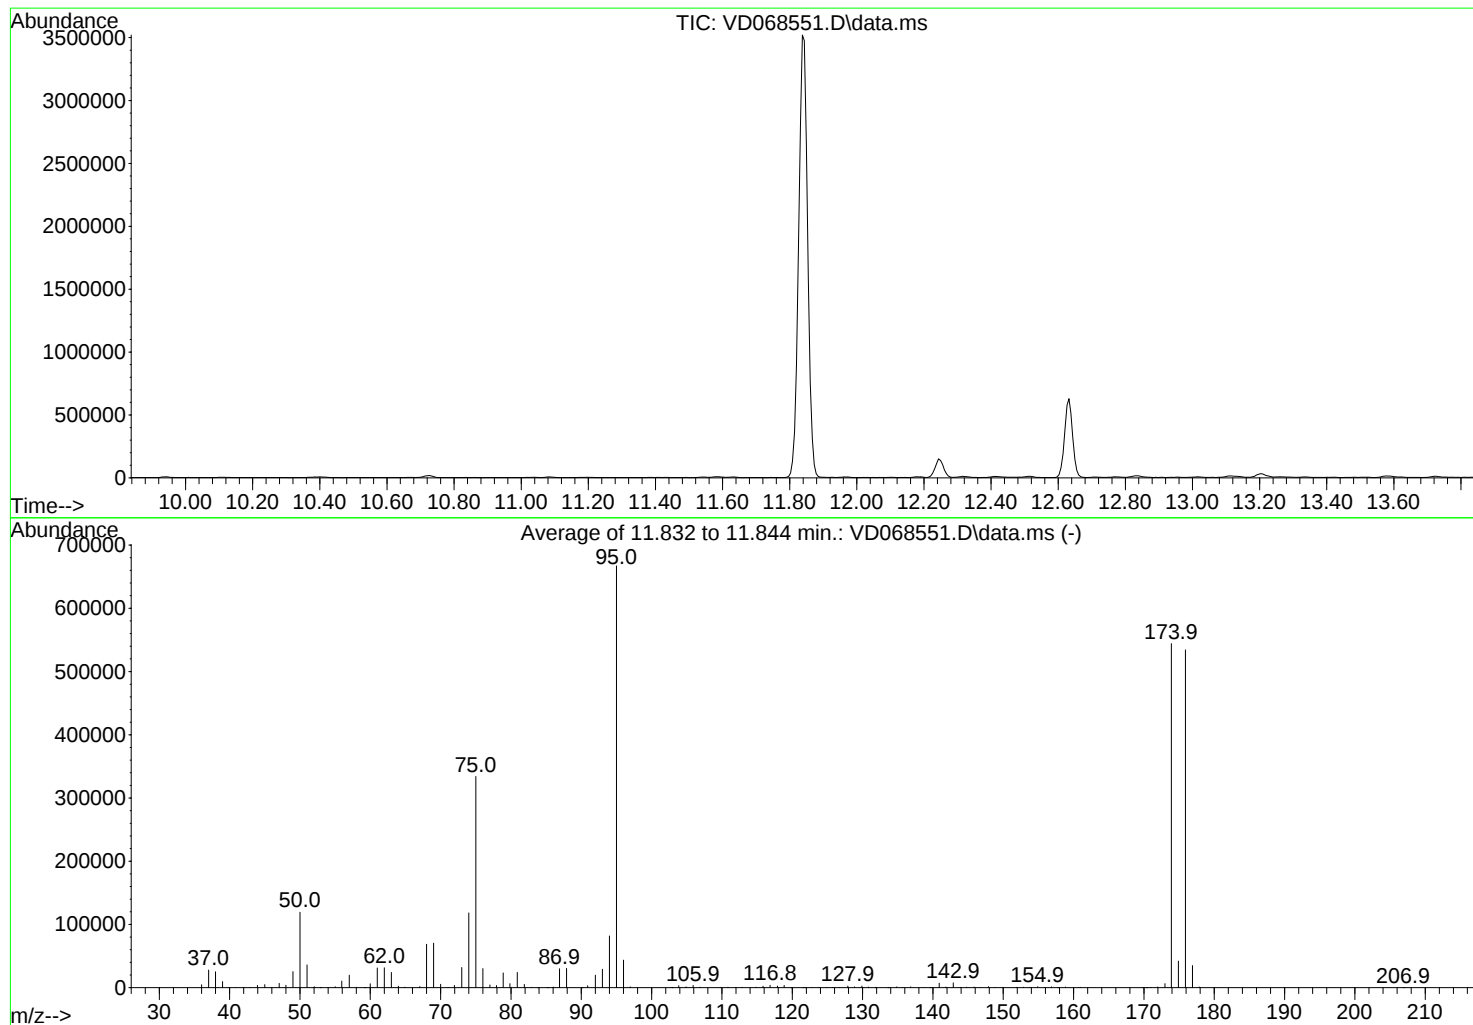

AutoFind: Scans 1685, 1686, 1687; Background Corrected with Scan 1675

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	119123	PASS
75	95	30	60	50.1	334016	PASS
95	95	100	100	100.0	667243	PASS
96	95	5	9	6.5	43504	PASS
173	174	0.00	2	1.2	6267	PASS
174	95	50	100	81.5	544128	PASS
175	174	5	9	7.7	41976	PASS
176	174	95	101	98.2	534400	PASS
177	176	5	9	6.5	34821	PASS