

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032921\
 Data File : VD068702.D
 Acq On : 29 Mar 2021 17:02
 Operator : VA/SY
 Sample : M1852-01
 Misc : 6.77G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 OR-03-032921

Quant Time: Mar 30 01:06:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 20 02:00:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	297188	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	594300	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.643	117	545457	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.573	152	281098	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	183804	61.34	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.68%
35) Dibromofluoromethane	7.914	113	195895	52.98	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.96%
50) Toluene-d8	10.338	98	717236	50.31	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	100.62%
62) 4-Bromofluorobenzene	12.632	95	280589	60.71	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	121.42%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD032921\
Data File : VD068702.D
Acq On : 29 Mar 2021 17:02
Operator : VA/SY
Sample : M1852-01
Misc : 6.77G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
OR-03-032921

Quant Time: Mar 30 01:06:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D031921S.M
Quant Title : SW846 8260
QLast Update : Sat Mar 20 02:00:55 2021
Response via : Initial Calibration




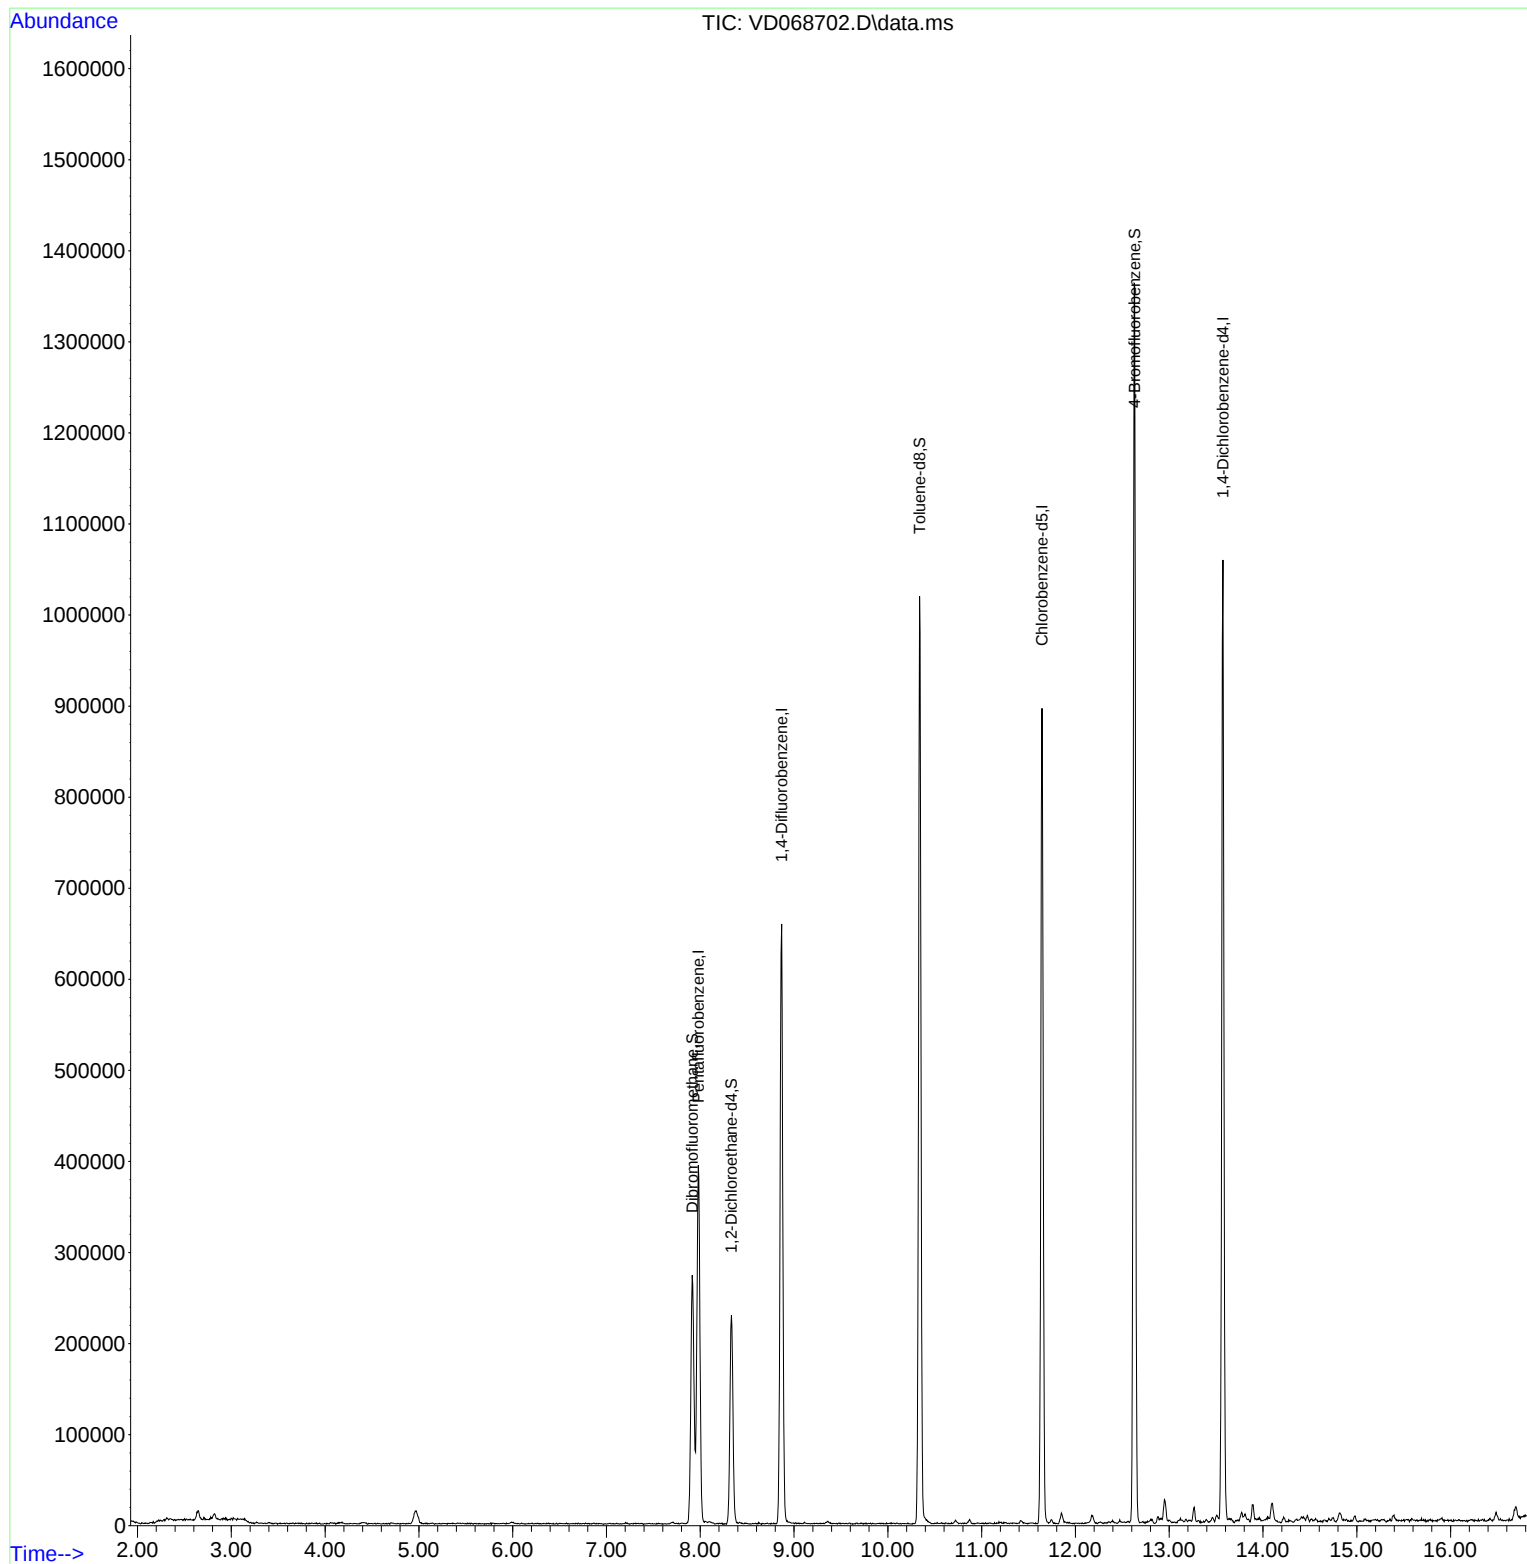


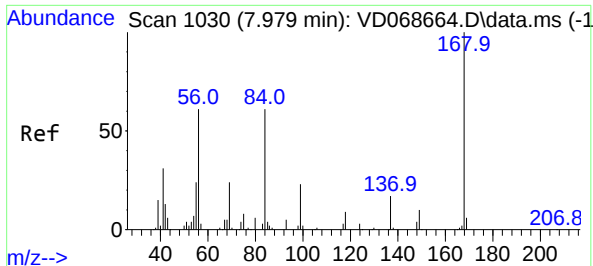

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02




Instrument :
MSVOA_D
ClientSampleId :
OR-03-032921


Tgt Ion:168 Resp: 297188
Ion Ratio Lower Upper
168 100
99 55.6 46.2 69.2

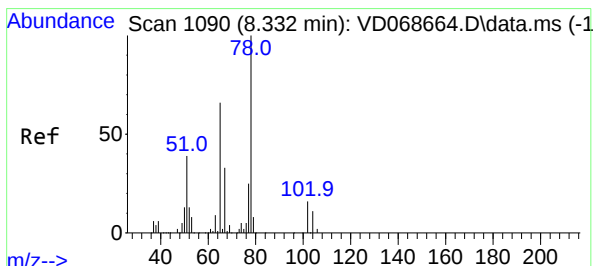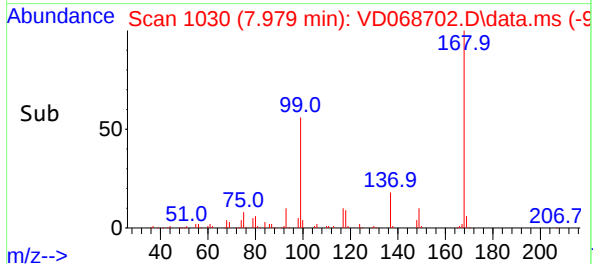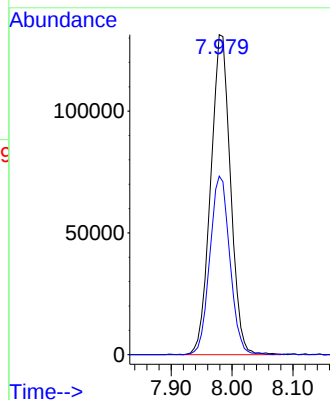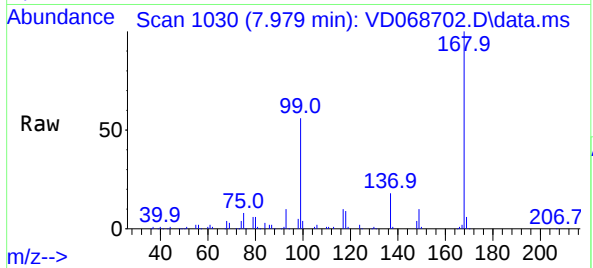

#33
1,2-Dichloroethane-d4
Concen: 61.34 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Tgt Ion: 65 Resp: 183804
Ion Ratio Lower Upper
65 100
67 53.1 0.0 106.0

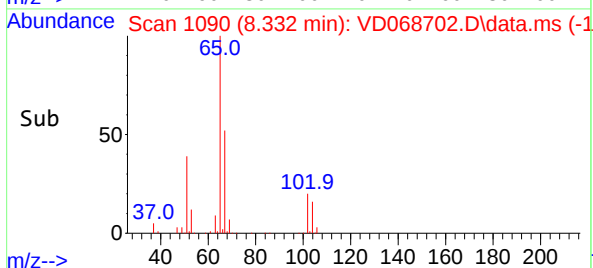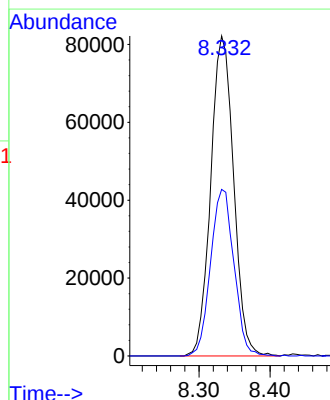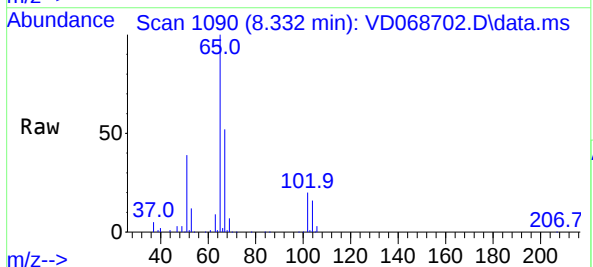




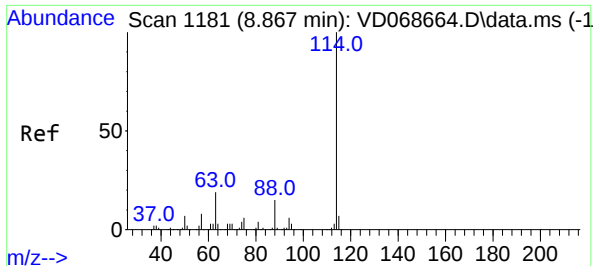


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Instrument :
MSVOA_D
ClientSampleId :
OR-03-032921




Tgt Ion:	114	Resp:	594300
Ion Ratio	Lower	Upper	
114	100		
63	18.0	0.0	38.2
88	15.5	0.0	29.4

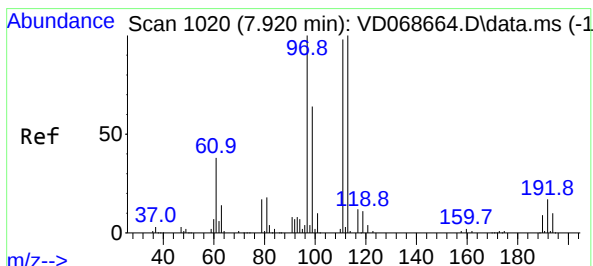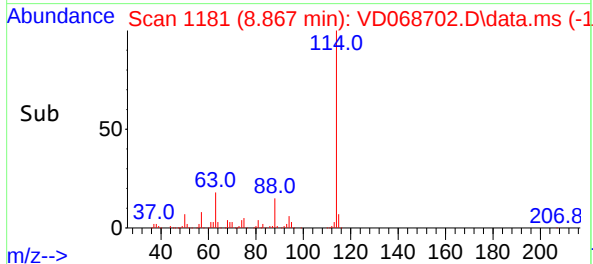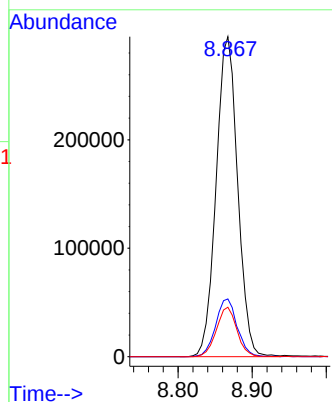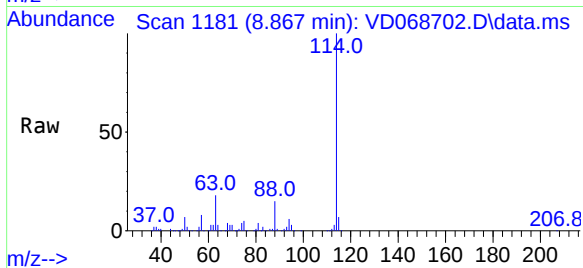


#35

Dibromofluoromethane
Concen: 52.98 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.006 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Tgt Ion:	113	Resp:	195895
Ion Ratio	Lower	Upper	
113	100		
111	103.6	82.5	123.7
192	19.1	15.1	22.7


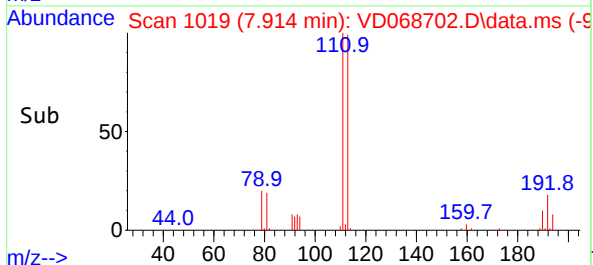
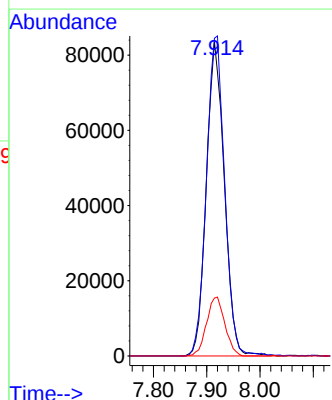
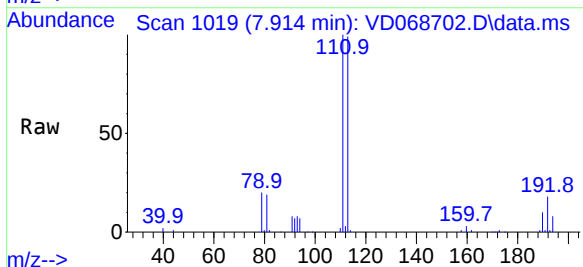


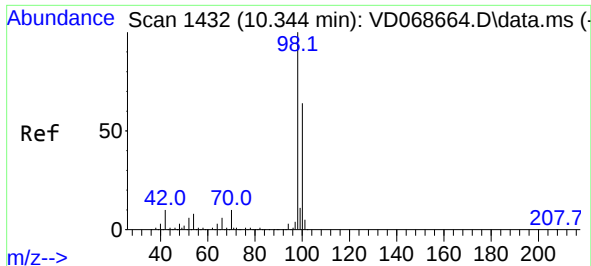

#50
Toluene-d8
Concen: 50.31 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.006 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02




Instrument :
MSVOA_D
ClientSampleId :
OR-03-032921


Tgt Ion: 98 Resp: 717236
Ion Ratio Lower Upper
98 100
100 63.3 51.8 77.6

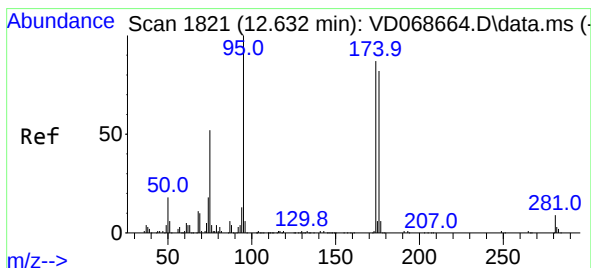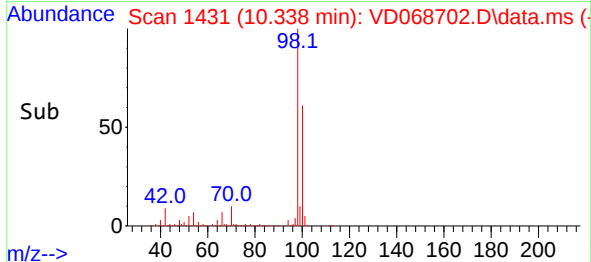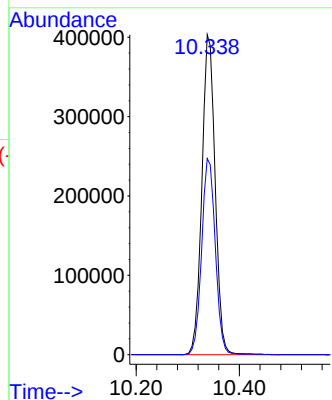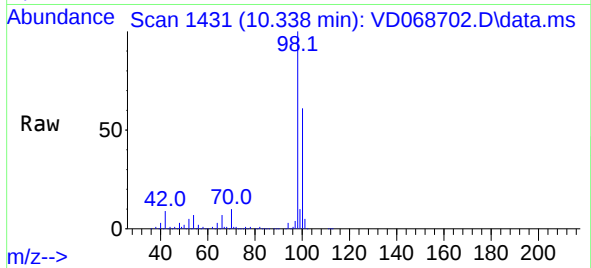

#62
4-Bromofluorobenzene
Concen: 60.71 ug/l
RT: 12.632 min Scan# 1821
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Tgt Ion: 95 Resp: 280589
Ion Ratio Lower Upper
95 100
174 82.9 0.0 168.0
176 79.7 0.0 160.2


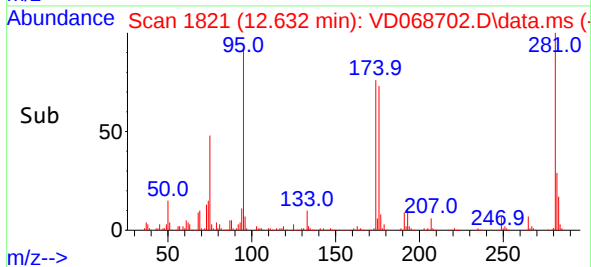
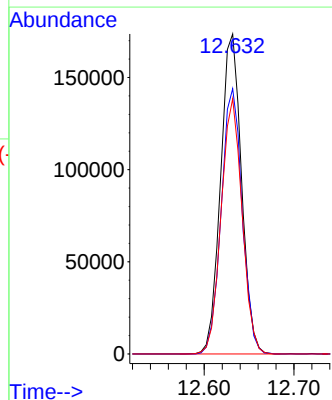
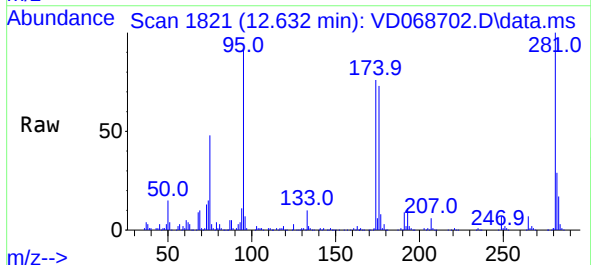


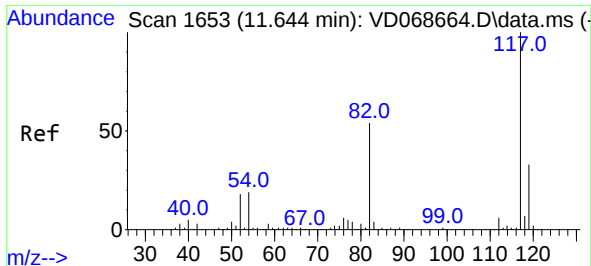

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.643 min Scan# 1653
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Instrument :
MSVOA_D
ClientSampleId :
OR-03-032921

Tgt Ion:117 Resp: 545457
Ion Ratio Lower Upper
117 100
82 51.4 43.5 65.3
119 32.4 26.7 40.1

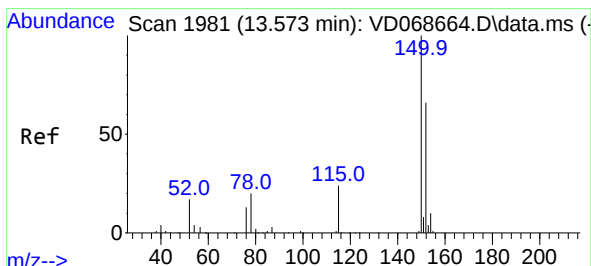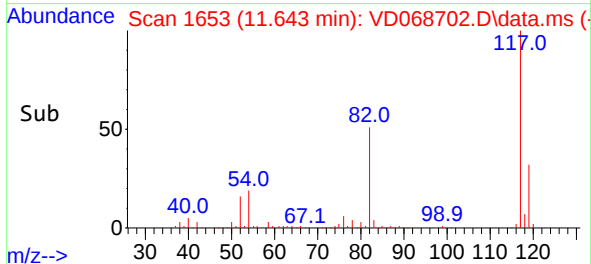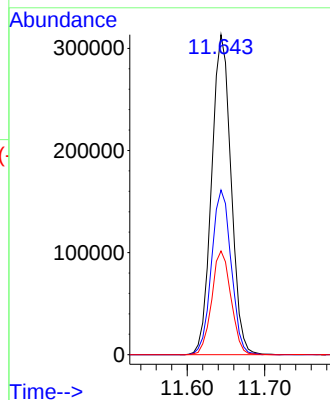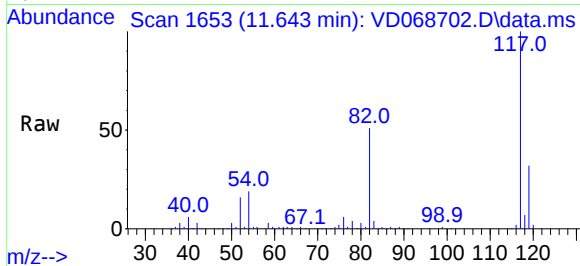

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.573 min Scan# 1981
Delta R.T. -0.000 min
Lab File: VD068702.D
Acq: 29 Mar 2021 17:02

Tgt Ion:152 Resp: 281098
Ion Ratio Lower Upper
152 100
115 59.8 29.3 87.8
150 157.3 0.0 347.6

