
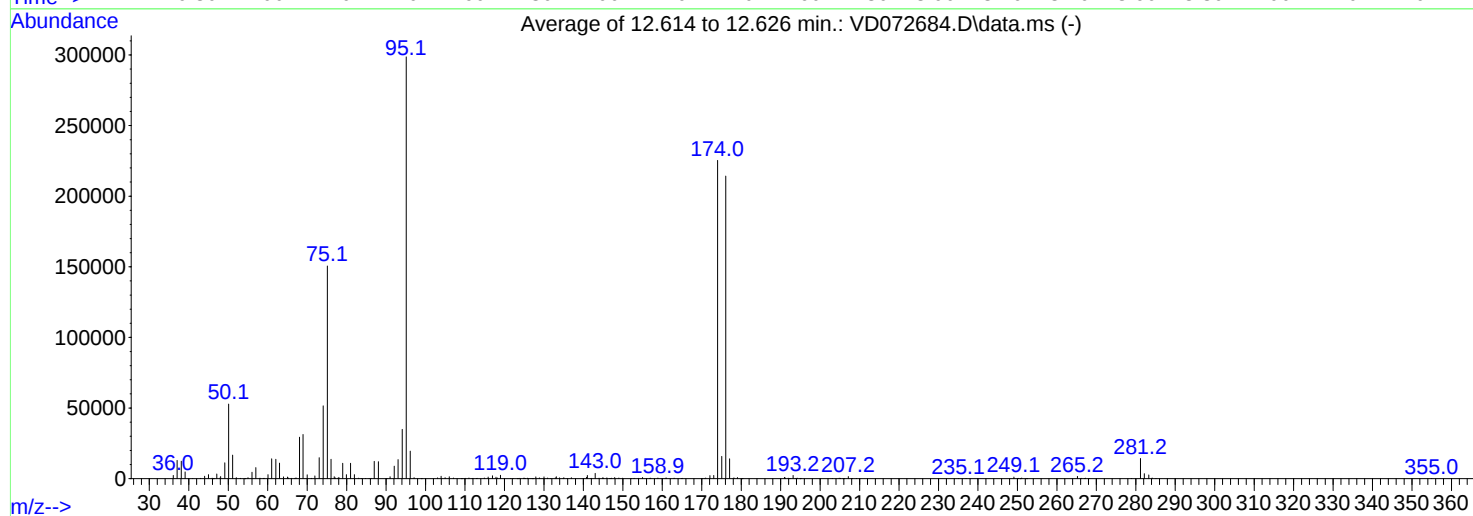


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042222\
 Data File : VD072684.D
 Acq On : 22 Apr 2022 08:53
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D032922S.M
 Title : SW846 8260
 Last Update : Wed Mar 30 02:44:36 2022

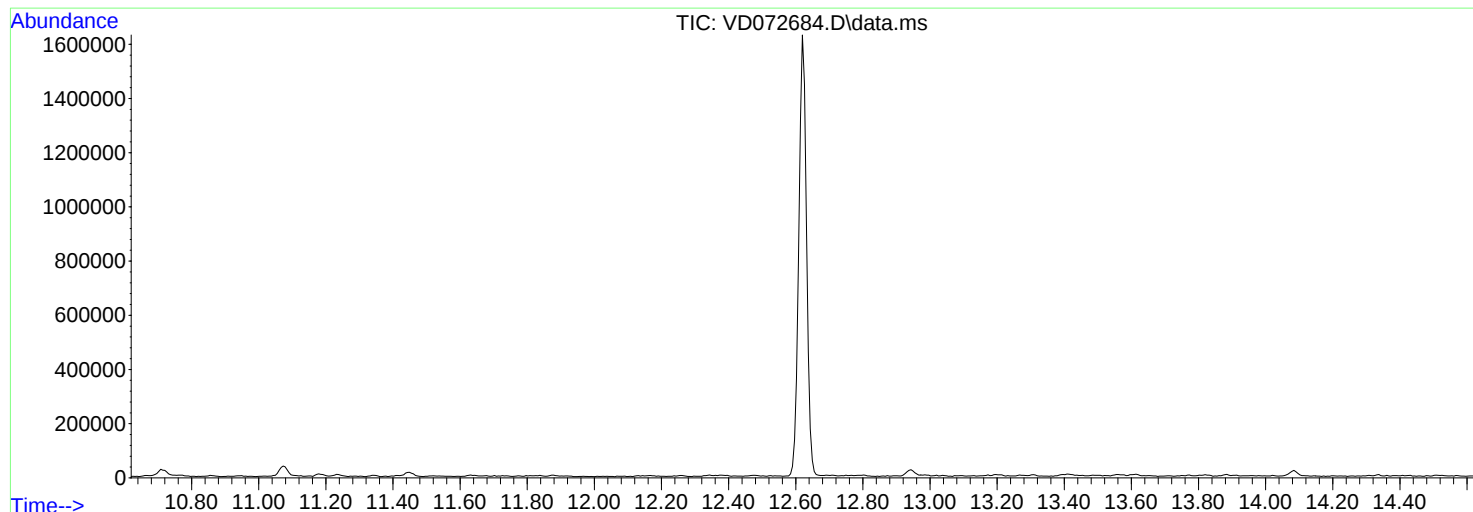

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1807

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	52829	PASS
75	95	30	60	50.4	150592	PASS
95	95	100	100	100.0	298667	PASS
96	95	5	9	6.5	19451	PASS
173	174	0.00	2	1.0	2272	PASS
174	95	50	100	75.4	225323	PASS
175	174	5	9	7.0	15815	PASS
176	174	95	101	95.1	214272	PASS
177	176	5	9	6.6	14083	PASS