




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075870.D
Acq On : 27 Apr 2023 19:35
Operator : KP/SY
Sample : 02525-03
Misc : 5.67G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

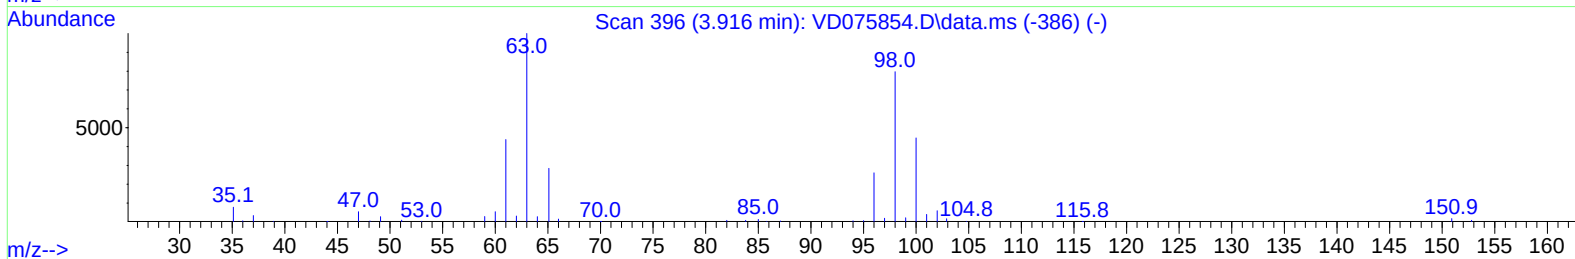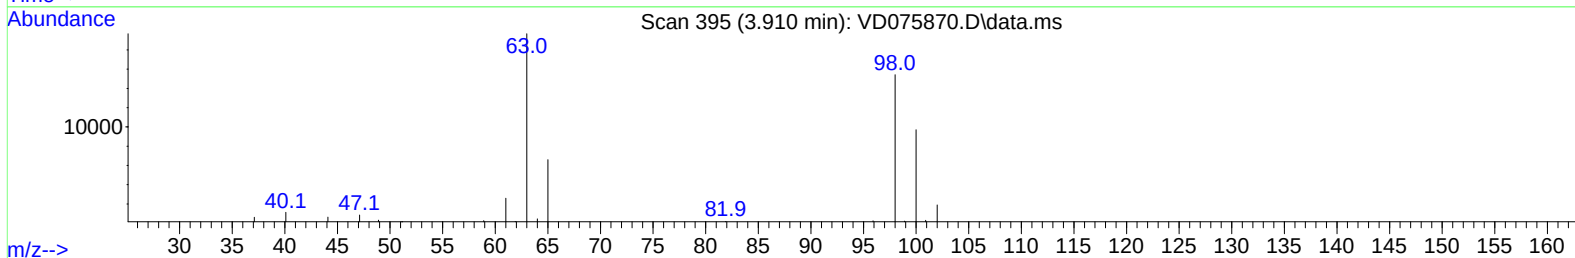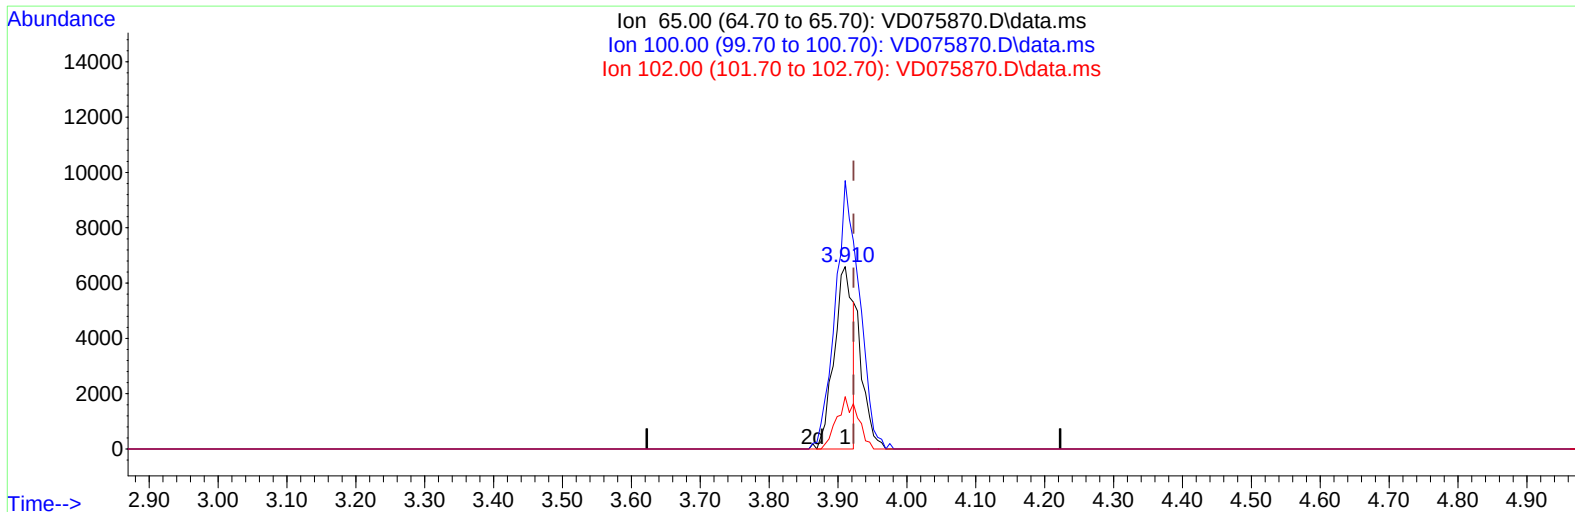

TIC: VD075870.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.910min (-0.012) 12.43 ug/L

response 12271

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	177.20	192.09
102.00	27.10	32.34
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075870.D
Acq On : 27 Apr 2023 19:35
Operator : KP/SY
Sample : 02525-03
Misc : 5.67G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

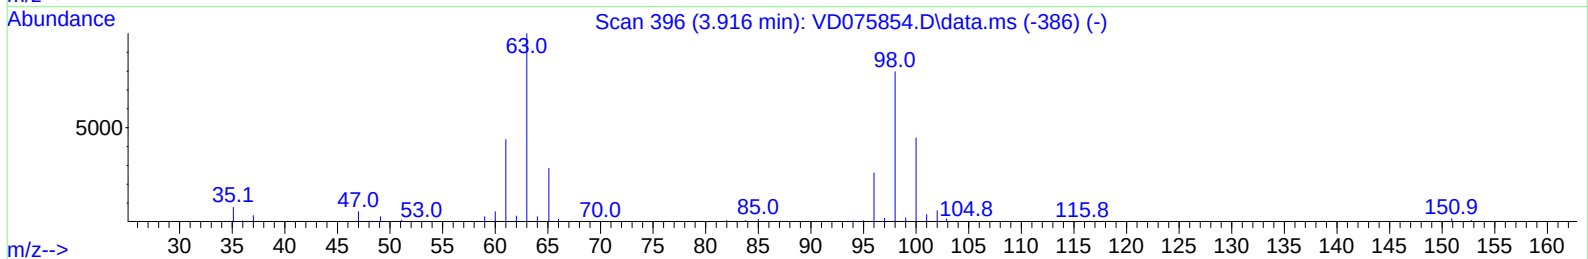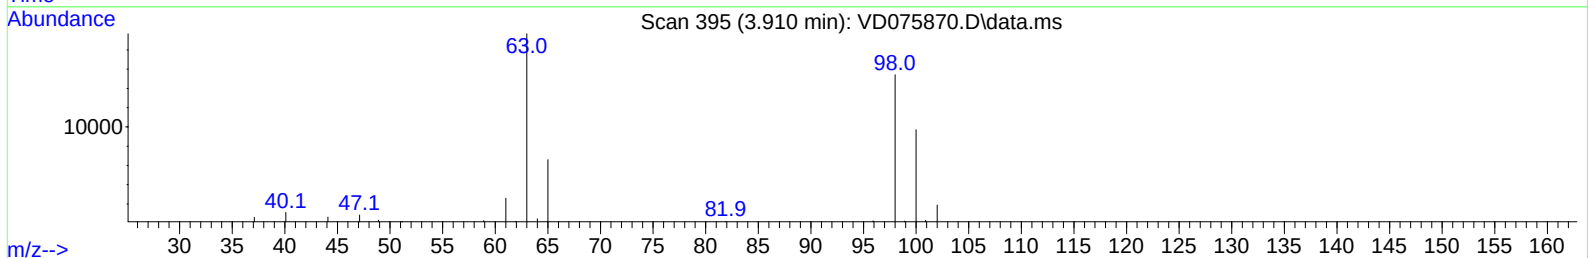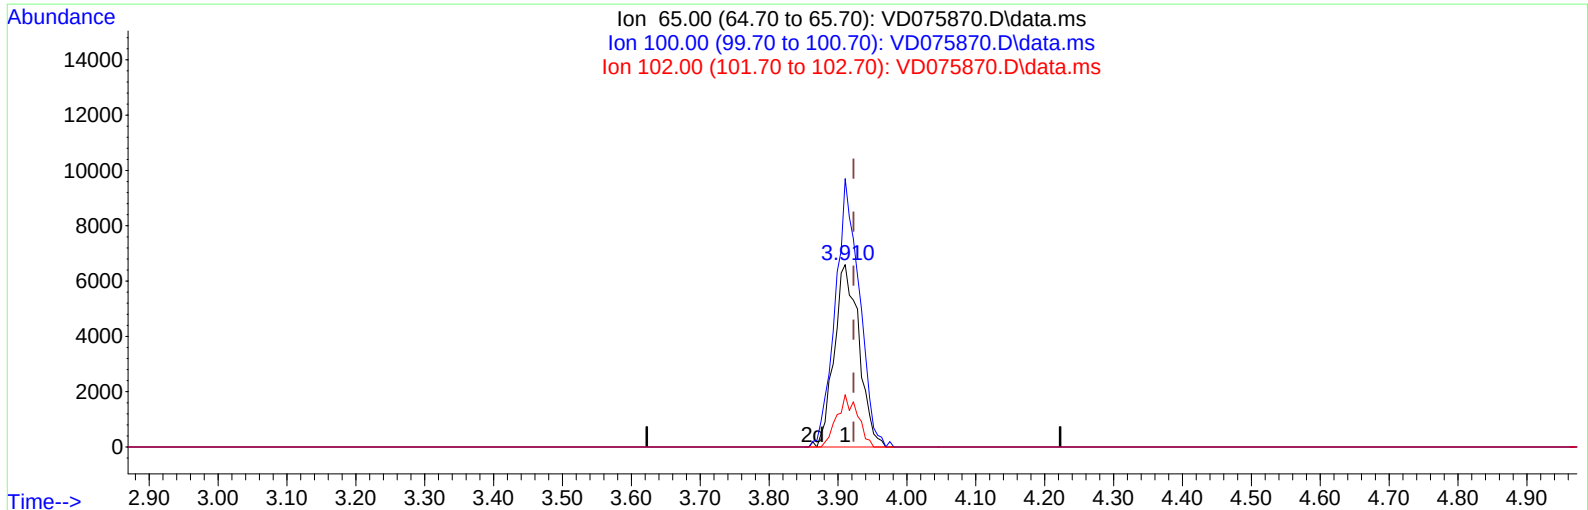

TIC: VD075870.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.910min (-0.012) 16.69 ug/L m

response 16472

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	177.20	143.10
102.00	27.10	24.09
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075870.D
Acq On : 27 Apr 2023 19:35
Operator : KP/SY
Sample : 02525-03
Misc : 5.67G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

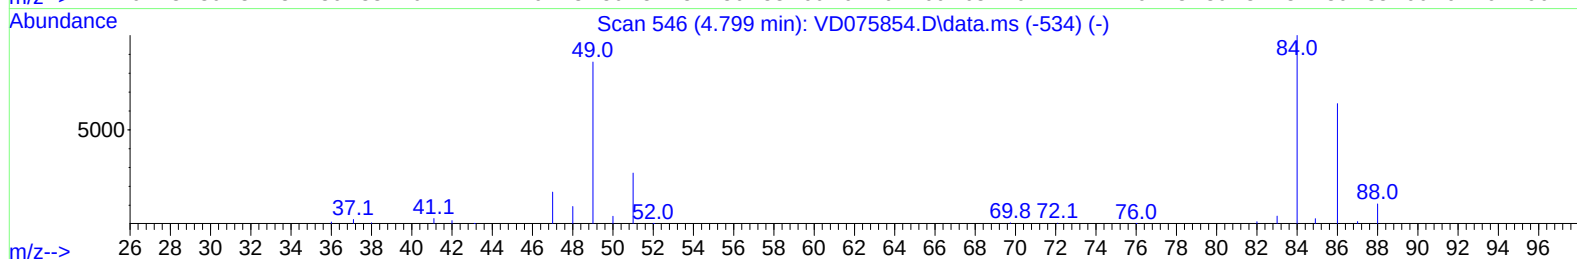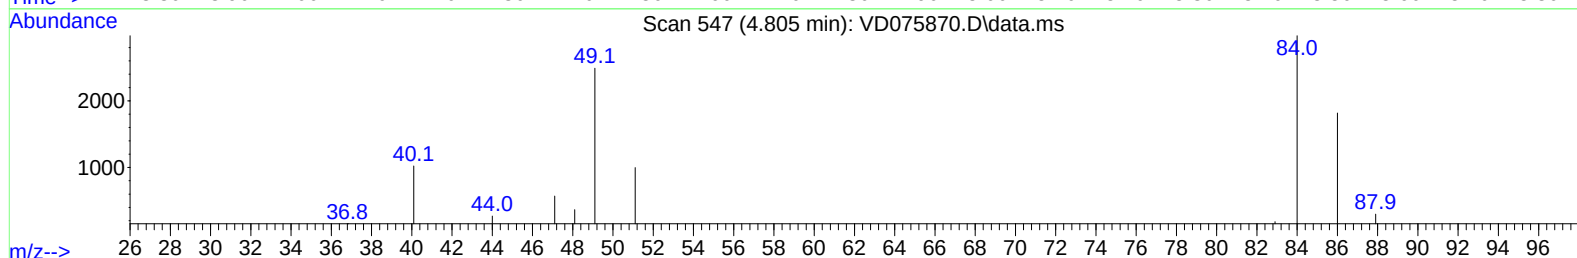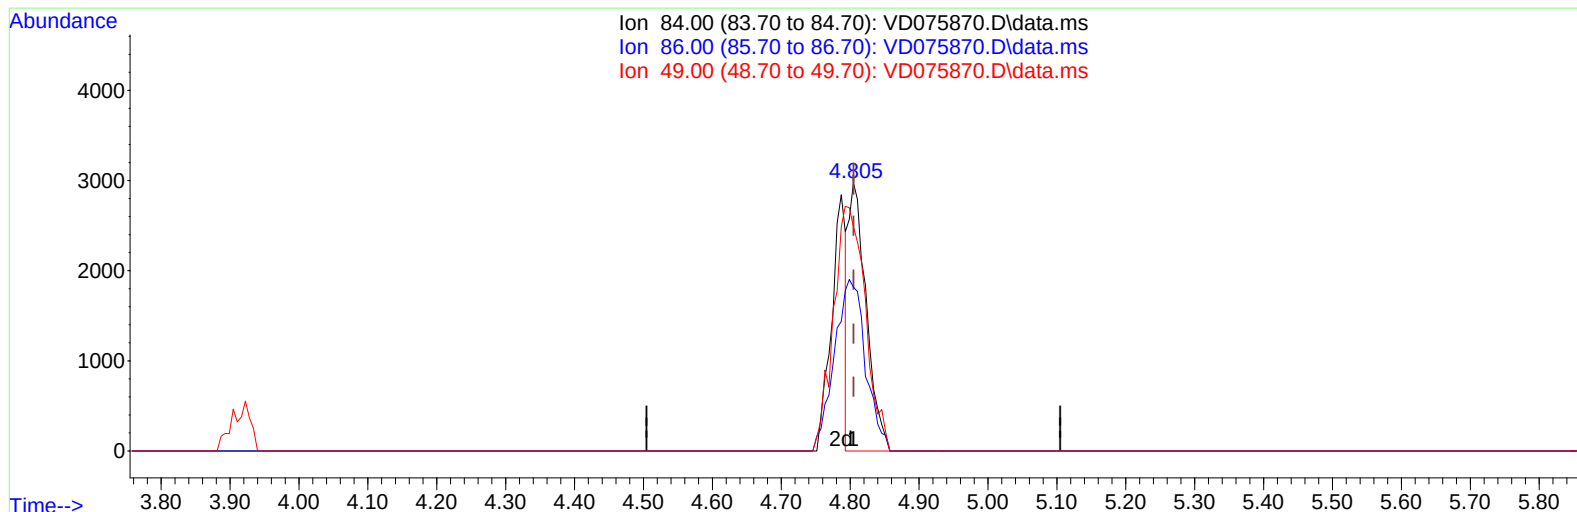

TIC: VD075870.D\data.ms

(16) Methylene chloride (T)

4.805min (-0.000) 1.34 ug/L

response 5316

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	61.07
49.00	86.80	83.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075870.D
 Acq On : 27 Apr 2023 19:35
 Operator : KP/SY
 Sample : 02525-03
 Misc : 5.67G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Manual IntegrationsAPPROVED

Quant Time: Apr 28 02:59:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

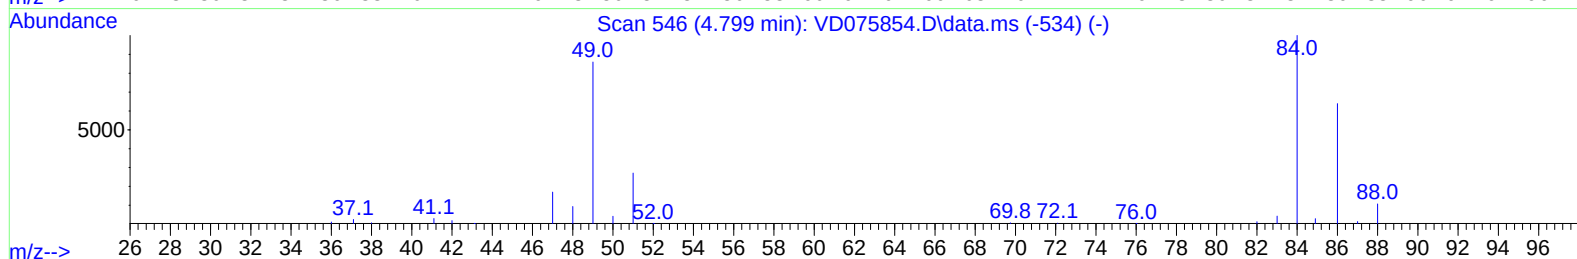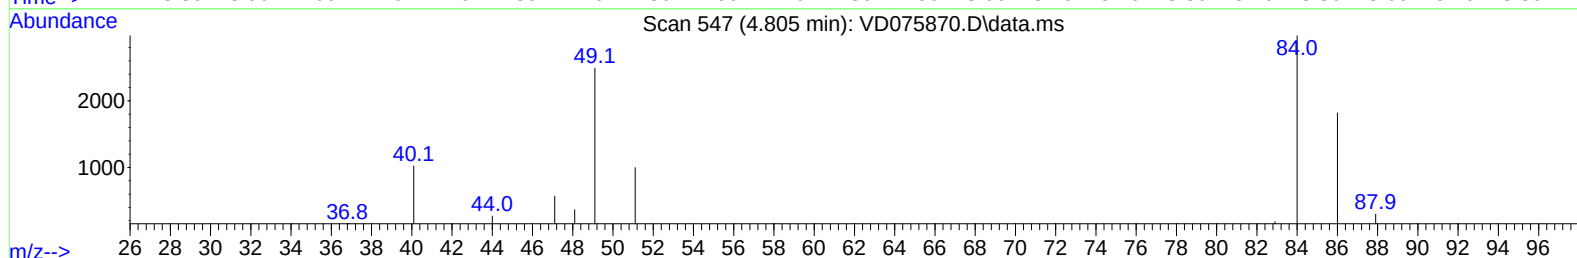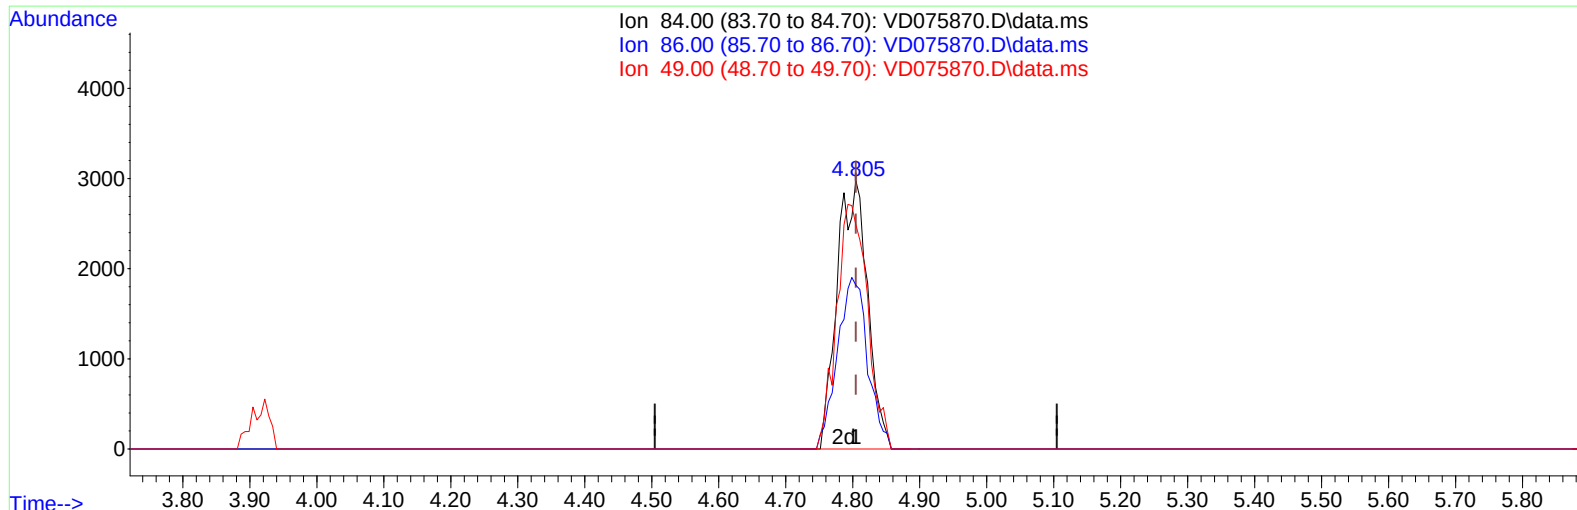

TIC: VD075870.D\data.ms

(16) Methylene chloride (T)

4.805min (-0.000) 2.38 ug/L m

response 9416

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	61.07
49.00	86.80	83.61
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075870.D
 Acq On : 27 Apr 2023 19:35
 Operator : KP/SY
 Sample : 02525-03
 Misc : 5.67G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Manual IntegrationsAPPROVED

Quant Time: Apr 28 02:59:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

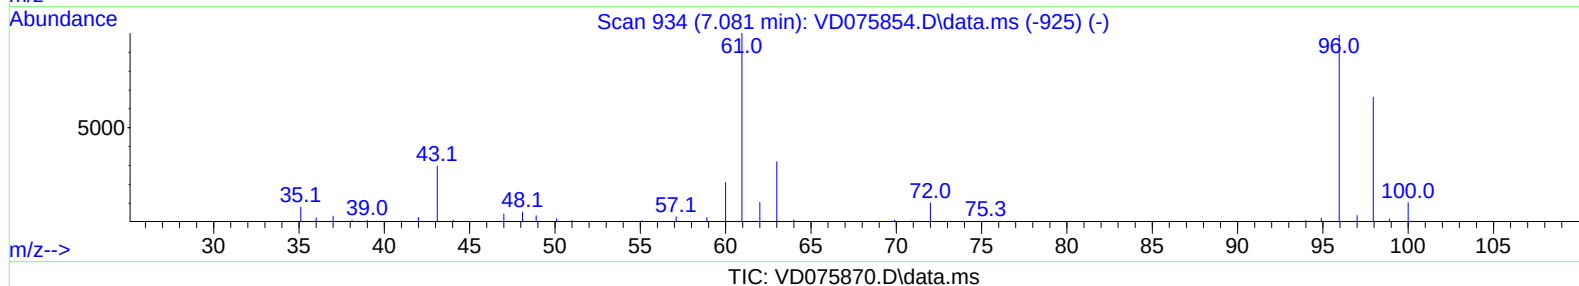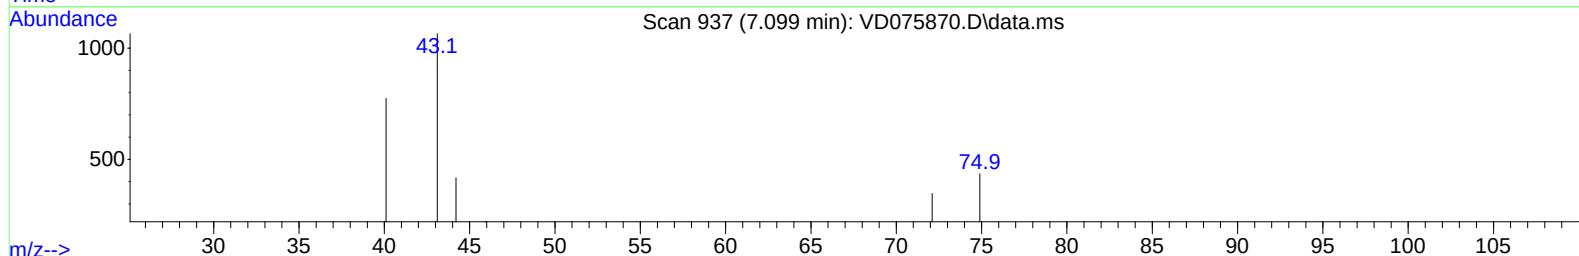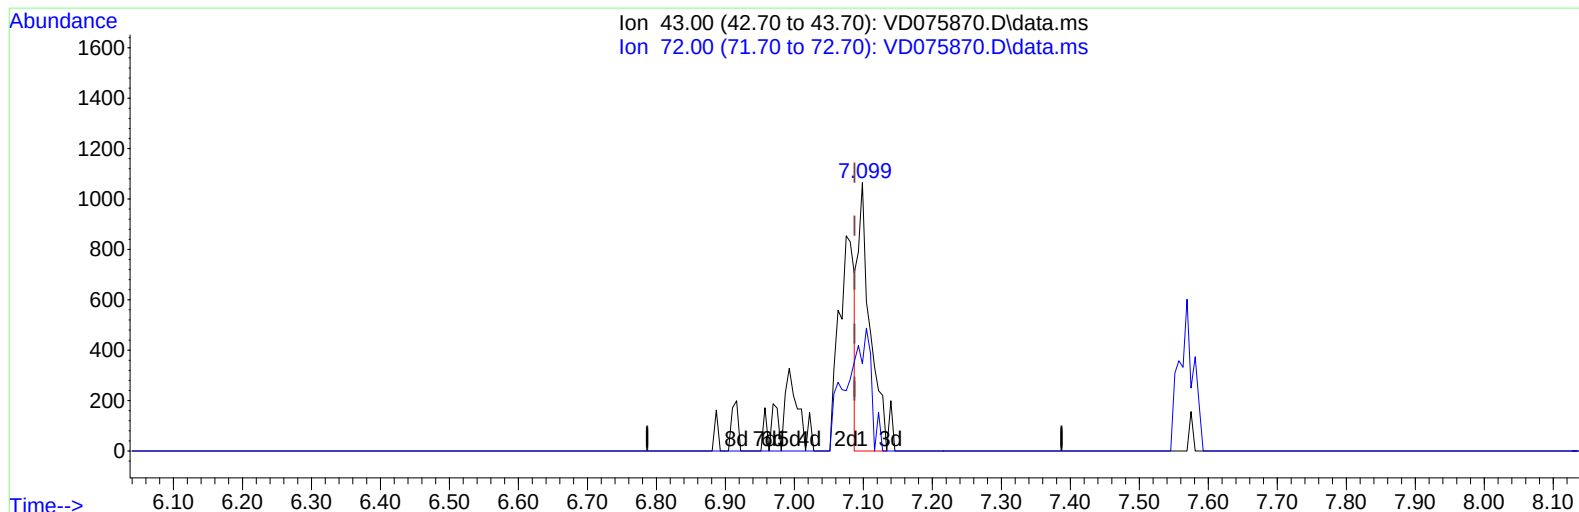

(22) 2-Butanone (T)

7.099min (+ 0.011) 3.16 ug/L

response 1309

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	41.00	23.53
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075870.D
 Acq On : 27 Apr 2023 19:35
 Operator : KP/SY
 Sample : 02525-03
 Misc : 5.67G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

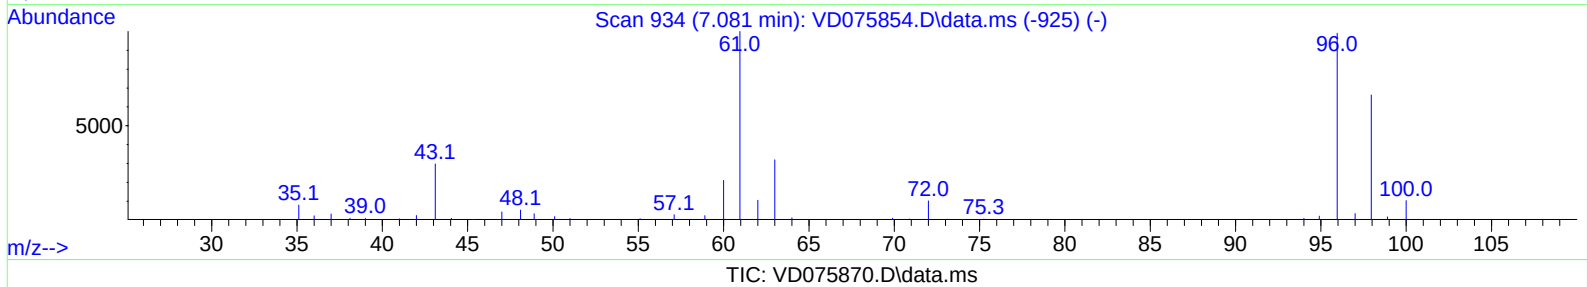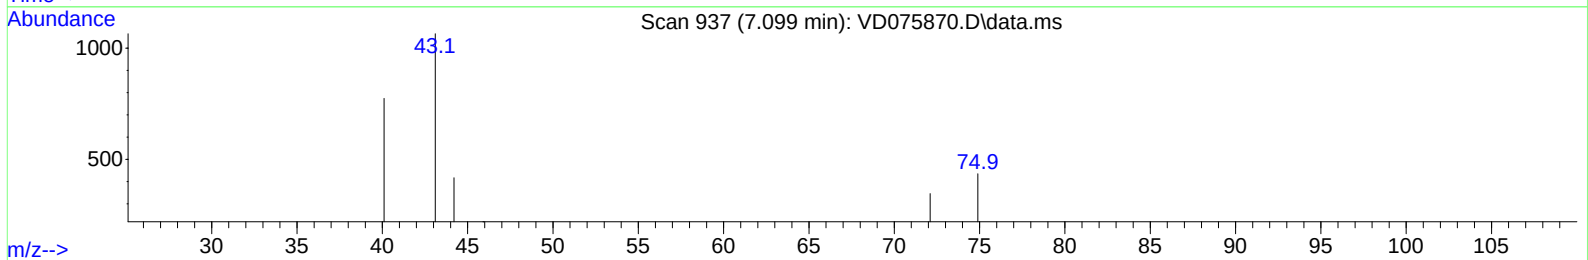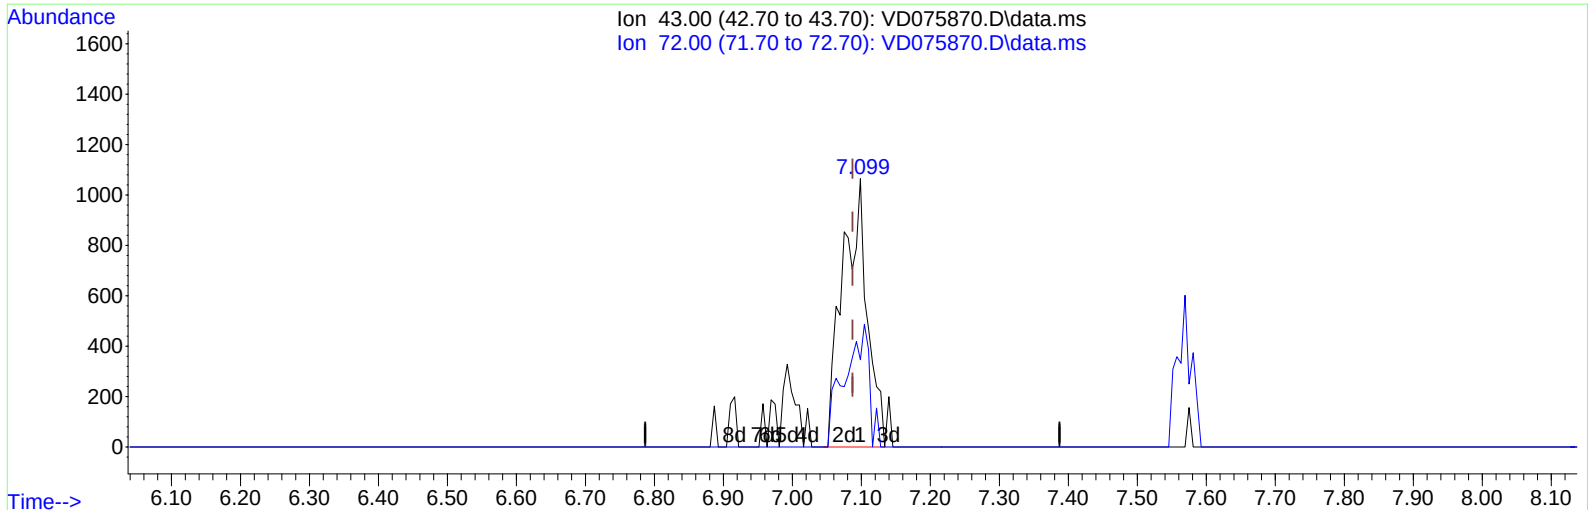

(22) 2-Butanone (T)

7.099min (+ 0.011) 6.39 ug/L m

response 2648

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	41.00	11.63#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075870.D
 Acq On : 27 Apr 2023 19:35
 Operator : KP/SY
 Sample : 02525-03
 Misc : 5.67G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC3

Manual IntegrationsAPPROVED

Quant Time: Apr 28 02:59:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	195148	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	229723	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	107343	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	67593	15.789	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.160%		
7) Chloroethane-d5	2.793	69	71332	19.285	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.120%		
11) 1,1-Dichloroethene-d2	3.910	65	16472m	16.689	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.760%		
21) 2-Butanone-d5	6.987	46	60283	162.205	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	324.400%#		
24) Chloroform-d	7.569	84	119680	24.525	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	98.080%		
26) 1,2-Dichloroethane-d4	8.234	65	73336	35.191	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	140.760%#		
32) Benzene-d6	8.198	84	212368	15.861	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	63.440%		
36) 1,2-Dichloropropane-d6	9.210	67	77707	20.968	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.880%		
41) Toluene-d8	10.269	98	183265	14.620	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	58.480%		
43) trans-1,3-Dichloroprop...	10.528	79	38783	25.318	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	101.280%		
47) 2-Hexanone-d5	10.881	63	46181	103.492	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	206.980%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	128280	45.234	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	180.920%#		
66) 1,2-Dichlorobenzene-d4	13.816	152	91242	24.031	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.120%		
Target Compounds					Qvalue	
13) Acetone	4.028	43	49804	156.594	ug/L	94
16) Methylene chloride	4.805	84	9416m	2.378	ug/L	
22) 2-Butanone	7.099	43	2648m	6.386	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075870.D
Acq On : 27 Apr 2023 19:35
Operator : KP/SY
Sample : 02525-03
Misc : 5.67G/10.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

