




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075871.D
Acq On : 27 Apr 2023 20:05
Operator : KP/SY
Sample : 02525-05
Misc : 6.16G/10.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

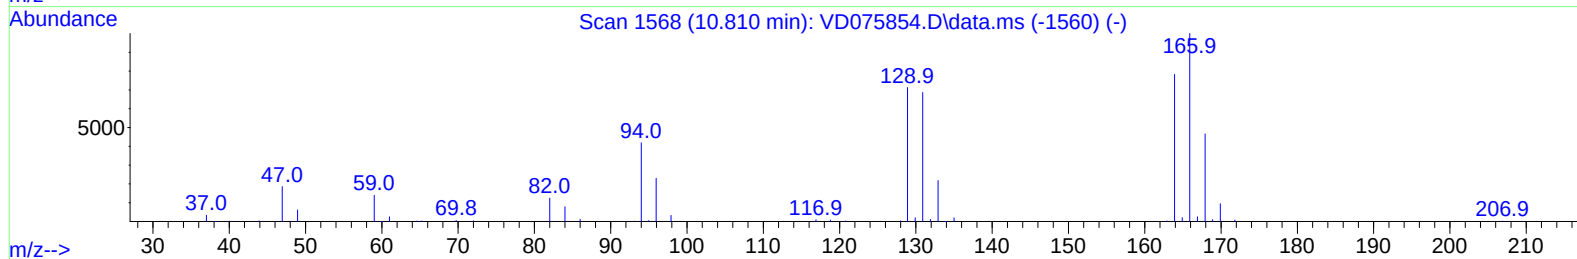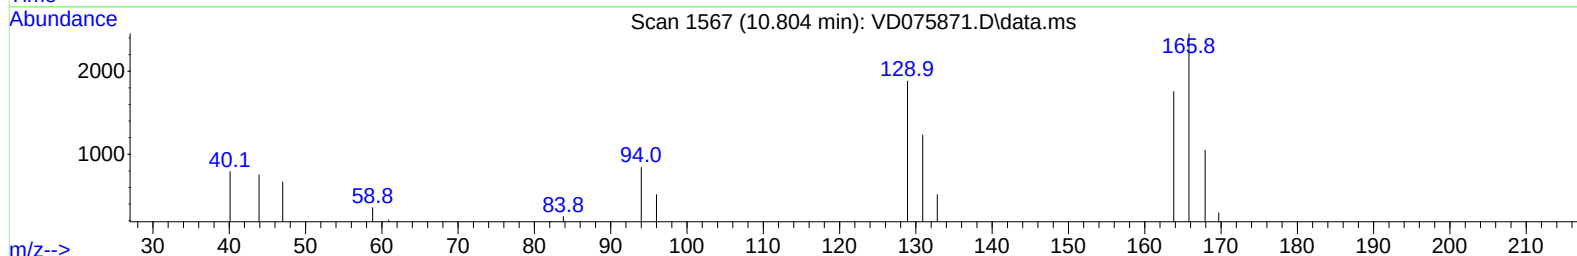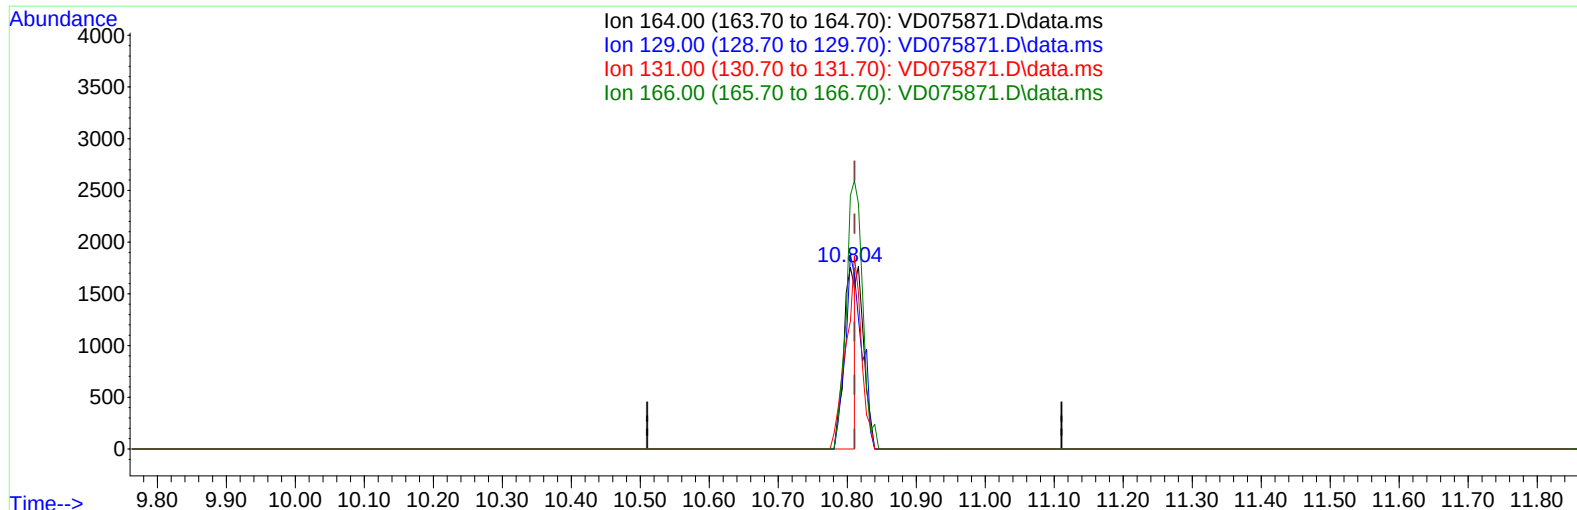

TIC: VD075871.D\data.ms

(46) Tetrachloroethene (T)

10.804min (-0.006) 0.32 ug/L

response 2037

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	86.20	107.06
131.00	84.10	70.27
166.00	118.50	139.58




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075871.D
Acq On : 27 Apr 2023 20:05
Operator : KP/SY
Sample : 02525-05
Misc : 6.16G/10.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

Quant Time: Apr 28 02:59:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

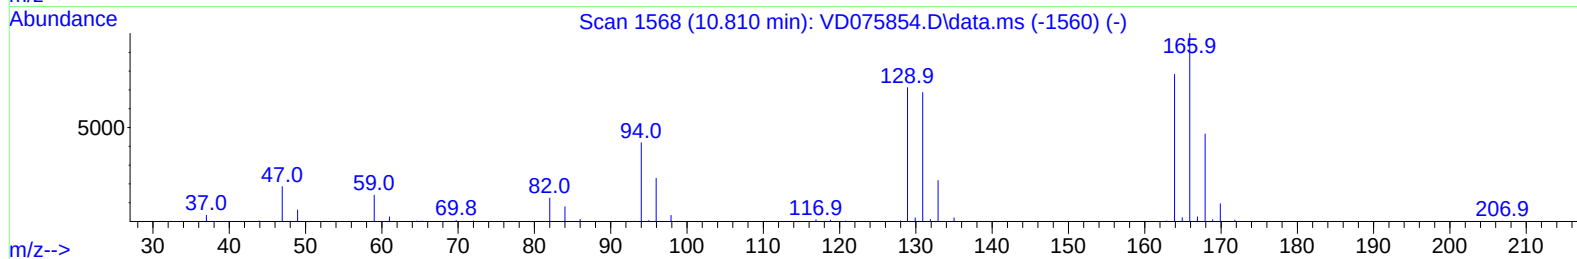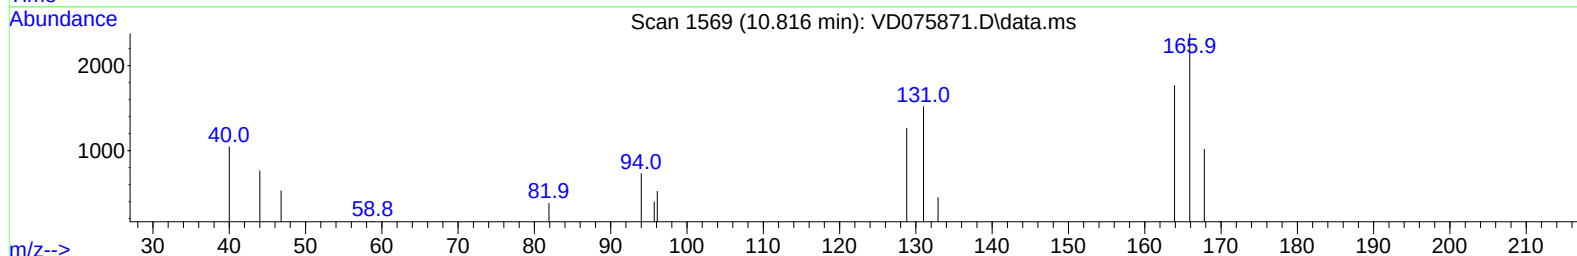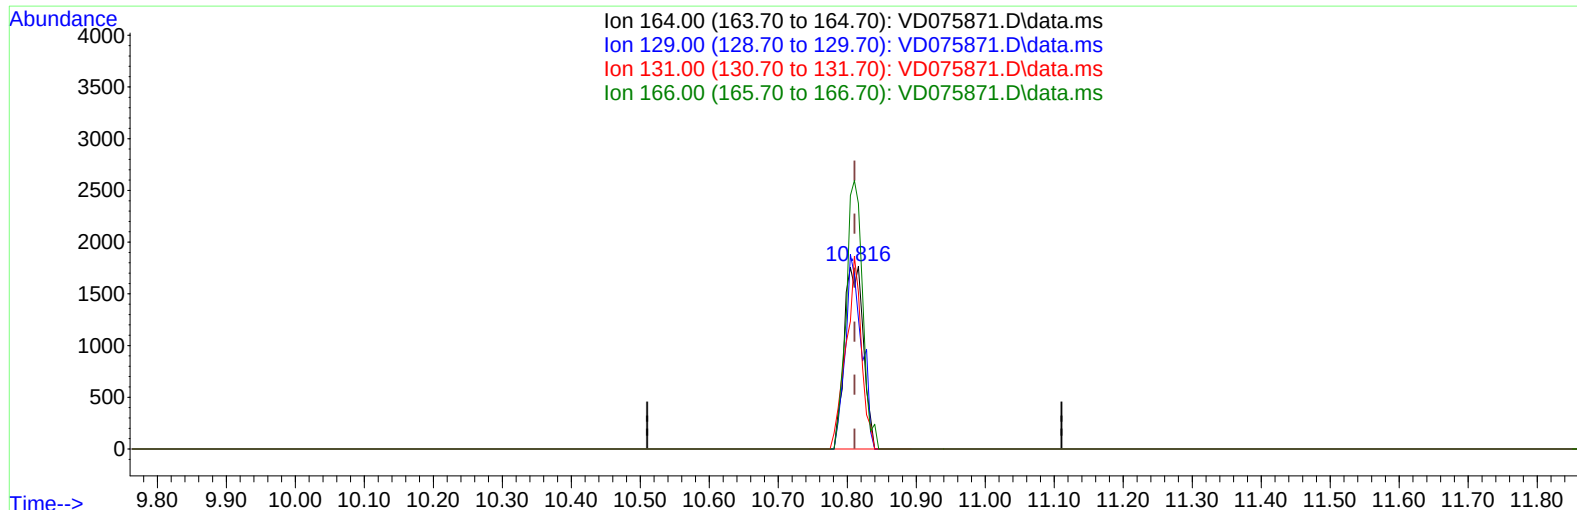

TIC: VD075871.D\data.ms

(46) Tetrachloroethene (T)

10.816min (+ 0.006) 0.54 ug/L m

response 3388

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	86.20	71.67
131.00	84.10	86.01
166.00	118.50	134.56

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075871.D
 Acq On : 27 Apr 2023 20:05
 Operator : KP/SY
 Sample : 02525-05
 Misc : 6.16G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCC5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 02:59:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2023
 Supervised By :Semsettin Yesilyurt 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	484000	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	492436	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	215036	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.270	65	183054	17.240	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	68.960%		
7) Chloroethane-d5	2.799	69	172082	18.758	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.040%		
11) 1,1-Dichloroethene-d2	3.911	65	42151	17.219	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	68.880%		
21) 2-Butanone-d5	6.987	46	58788	63.779	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	127.560%		
24) Chloroform-d	7.563	84	255969	21.149	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.600%		
26) 1,2-Dichloroethane-d4	8.228	65	119961	23.210	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.840%		
32) Benzene-d6	8.199	84	496866	17.312	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	69.240%		
36) 1,2-Dichloropropane-d6	9.210	67	160286	20.176	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.720%		
41) Toluene-d8	10.269	98	453696	16.885	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	67.520%		
43) trans-1,3-Dichloroprop...	10.522	79	63855	19.446	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.800%		
47) 2-Hexanone-d5	10.875	63	51251	53.580	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.160%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	154653	25.440	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.760%		
66) 1,2-Dichlorobenzene-d4	13.816	152	165676	21.782	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.120%		
Target Compounds						Qvalue
13) Acetone	4.017	43	102562	130.022	ug/L	98
16) Methylene chloride	4.799	84	19330	1.969	ug/L	90
25) Chloroform	7.587	83	3860	0.329	ug/L	90
46) Tetrachloroethene	10.816	164	3388m	0.536	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075871.D
Acq On : 27 Apr 2023 20:05
Operator : KP/SY
Sample : 02525-05
Misc : 6.16G/10.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCC5

Manual IntegrationsAPPROVED

Quant Time: Apr 28 02:59:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2023
Supervised By :Semsettin Yesilyurt 05/01/2023

