

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
 Data File : VD075872.D
 Acq On : 27 Apr 2023 20:35
 Operator : KP/SY
 Sample : 02525-11
 Misc : 6.49G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCK8

Quant Time: Apr 28 03:00:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Apr 27 02:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	506695	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	515208	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152	240107	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	197419	17.761	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.040%
7) Chloroethane-d5	2.793	69	182895	19.043	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.160%
11) 1,1-Dichloroethene-d2	3.916	65	45970	17.938	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.760%
21) 2-Butanone-d5	6.987	46	65013	67.373	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.740%
24) Chloroform-d	7.569	84	277718	21.918	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.680%
26) 1,2-Dichloroethane-d4	8.228	65	130112	24.046	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.200%
32) Benzene-d6	8.198	84	532722	17.740	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.960%
36) 1,2-Dichloropropane-d6	9.210	67	173608	20.887	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.560%
41) Toluene-d8	10.269	98	481836	17.139	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.560%
43) trans-1,3-Dichloroprop...	10.522	79	69742	20.300	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.200%
47) 2-Hexanone-d5	10.881	63	56076	56.033	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.060%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	171849	27.019	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.080%
66) 1,2-Dichlorobenzene-d4	13.816	152	188655	22.213	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.840%
Target Compounds						Qvalue
13) Acetone	4.022	43	37406	45.297	ug/L	95
16) Methylene chloride	4.799	84	20796	2.023	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042723\
Data File : VD075872.D
Acq On : 27 Apr 2023 20:35
Operator : KP/SY
Sample : 02525-11
Misc : 6.49G/10.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCK8

Quant Time: Apr 28 03:00:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Apr 27 02:02:18 2023
Response via : Initial Calibration

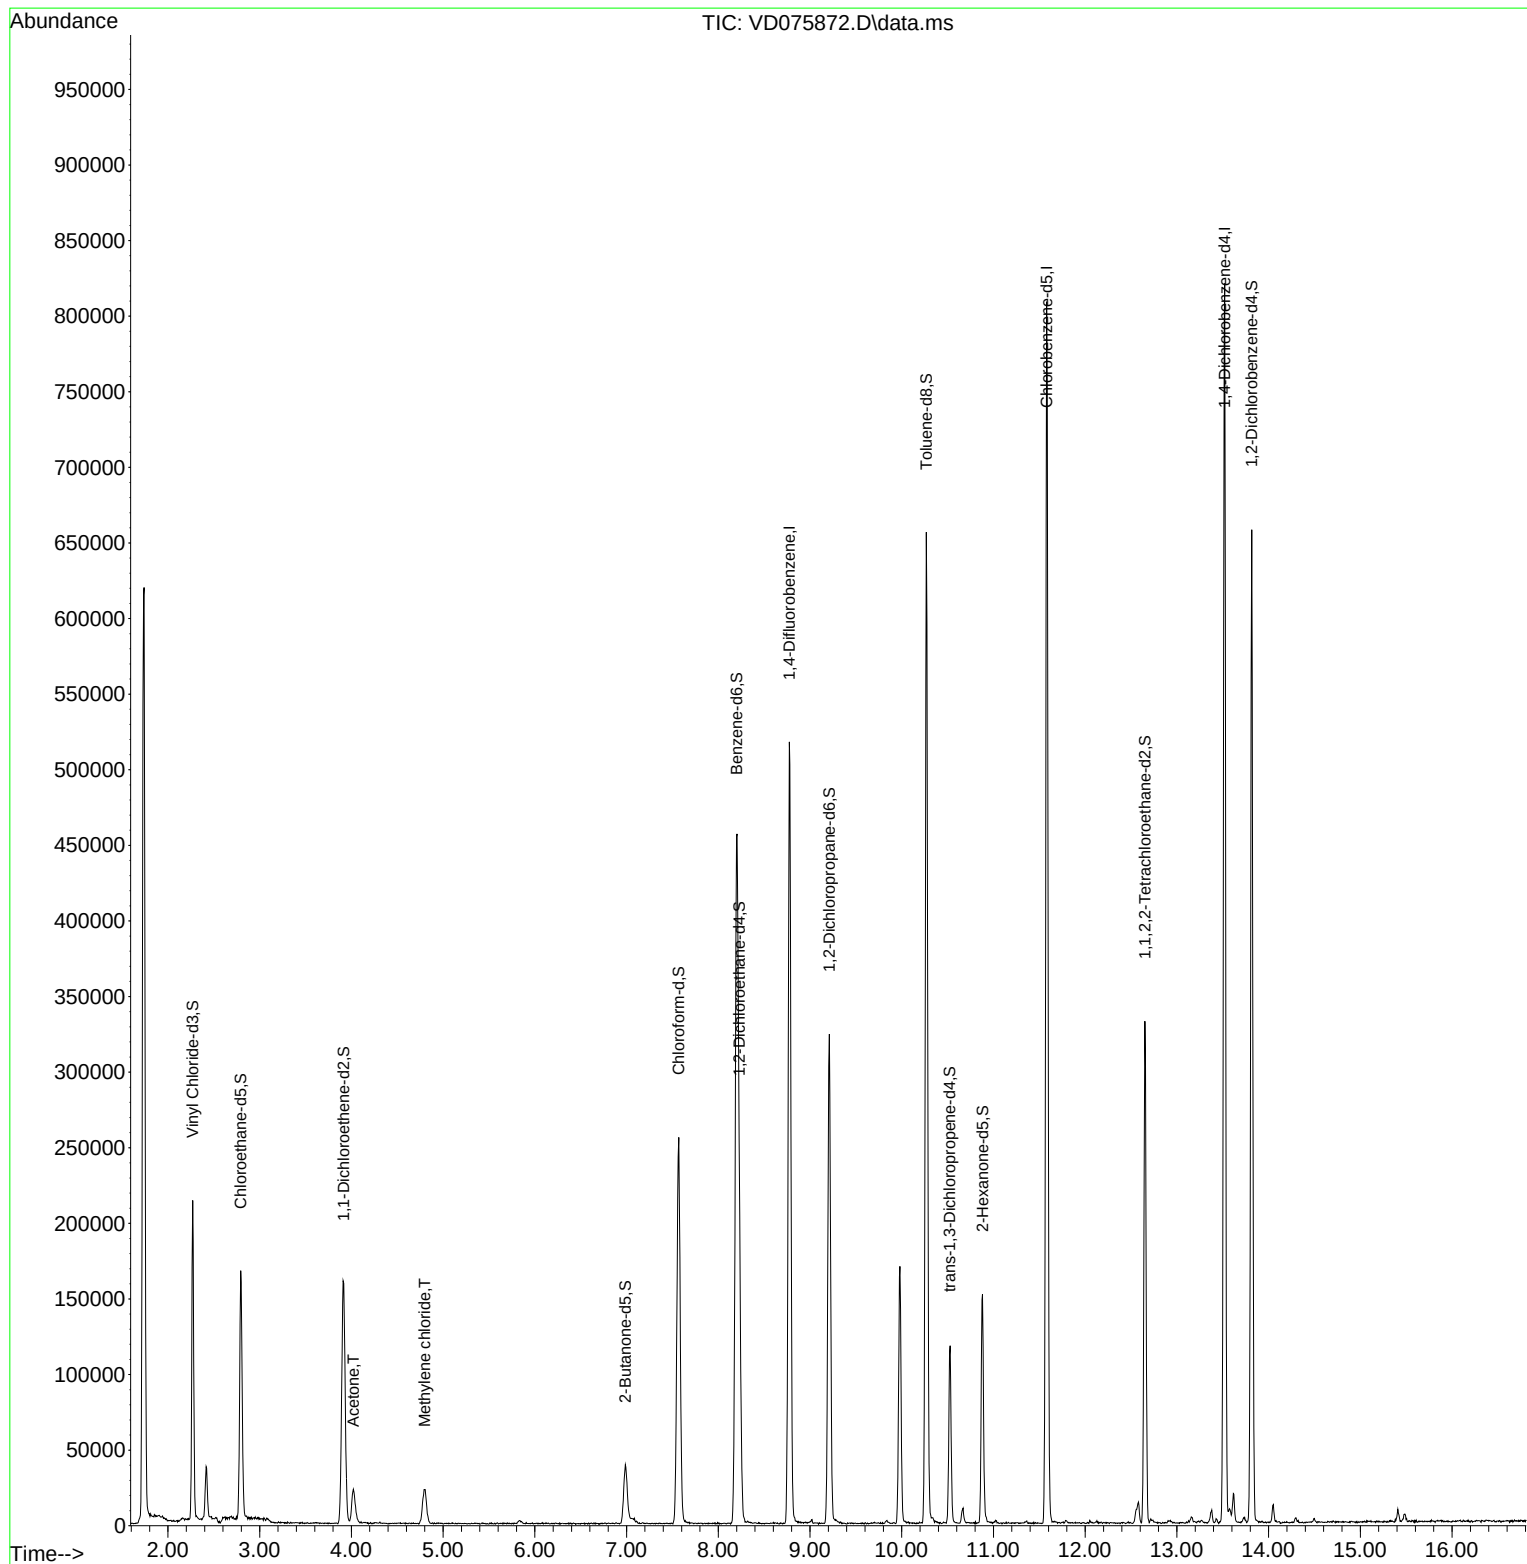

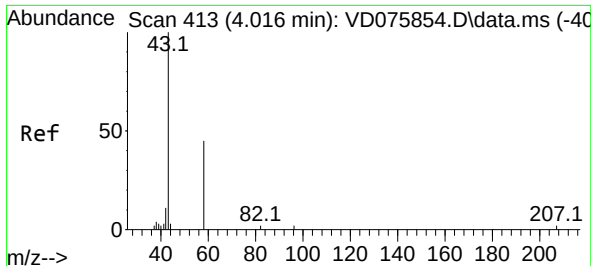

#13

Acetone

Concen: 45.297 ug/L

RT: 4.022 min Scan# 413

Delta R.T. -0.000 min

Lab File: VD075872.D

Acq: 27 Apr 2023 20:35

Instrument :

MSVOA_D

ClientSampleId :





DCCK8

Tgt Ion: 43 Resp: 37406

Ion Ratio Lower Upper

43 100

58 40.7 0.0 87.4

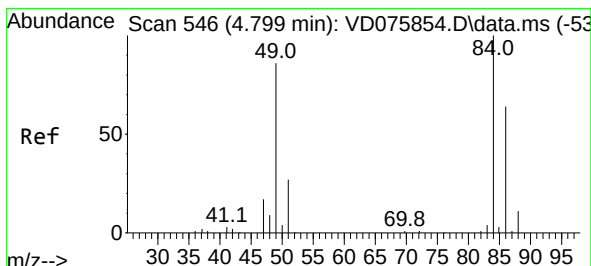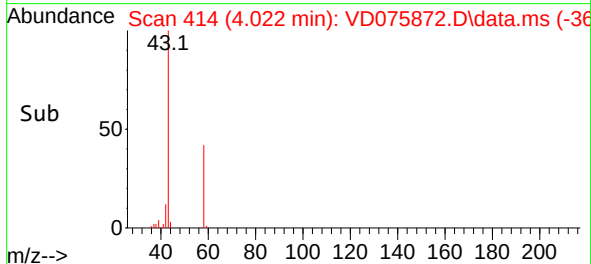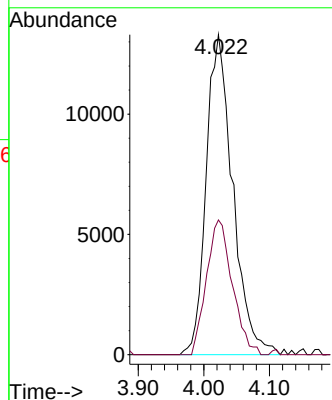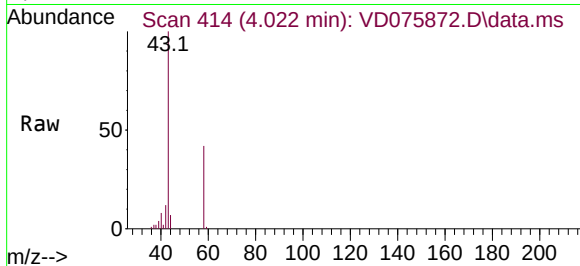

#16

Methylene chloride

Concen: 2.023 ug/L

RT: 4.799 min Scan# 546

Delta R.T. -0.006 min

Lab File: VD075872.D

Acq: 27 Apr 2023 20:35

Tgt Ion: 84 Resp: 20796

Ion Ratio Lower Upper

84 100

86 61.5 45.8 85.2

49 81.9 60.8 112.8

