




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075937.D
 Acq On : 01 May 2023 14:01
 Operator : KP/SY
 Sample : 02548-29RE
 Misc : 6.22G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCQ9RE

Manual IntegrationsAPPROVED

Quant Time: May 02 02:33:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 02:31:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Semsettin Yesilyurt 05/02/2023

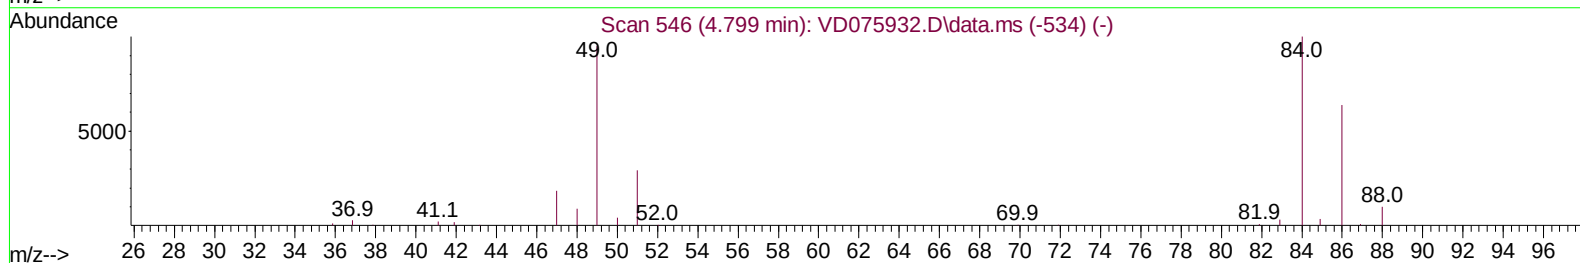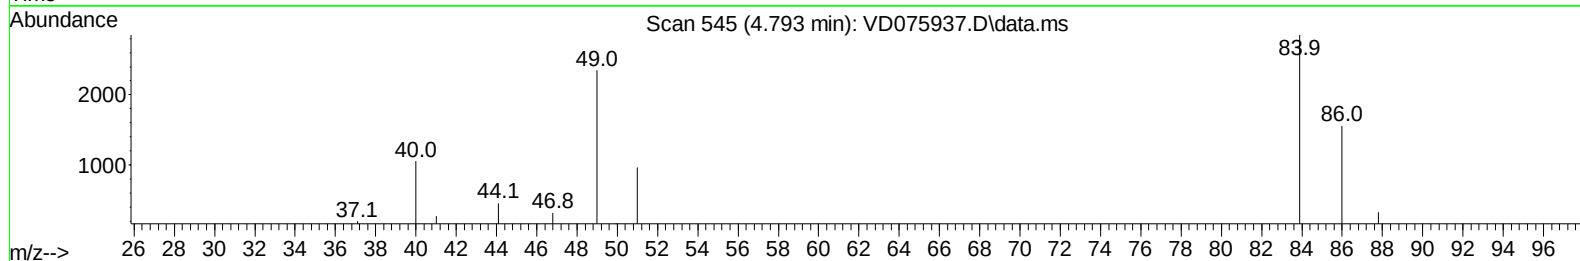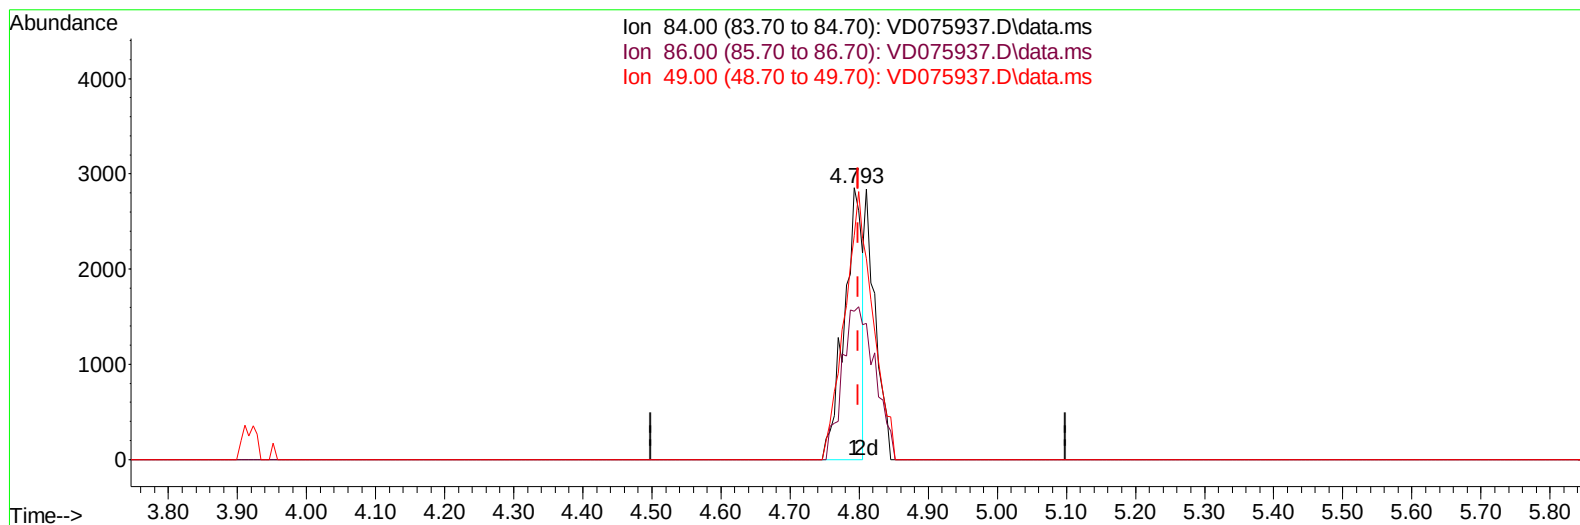

TIC: VD075937.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 2.79 ug/L

response 5187

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	54.52
49.00	86.80	82.40
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
Data File : VD075937.D
Acq On : 01 May 2023 14:01
Operator : KP/SY
Sample : 02548-29RE
Misc : 6.22G/10.00mL/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCQ9RE

Manual IntegrationsAPPROVED

Quant Time: May 02 02:33:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 02:31:38 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Semsettin Yesilyurt 05/02/2023

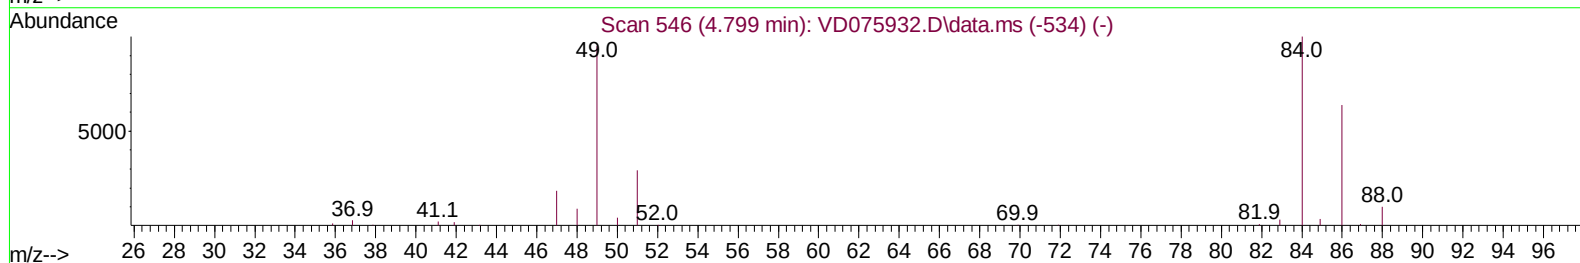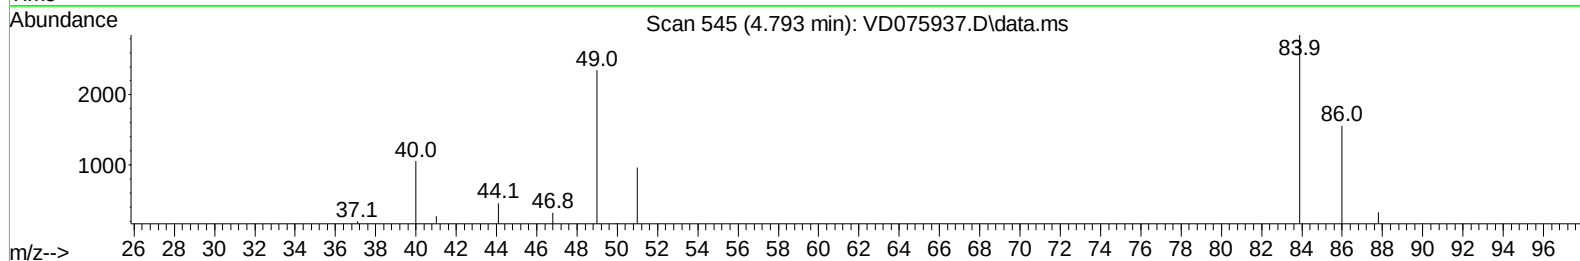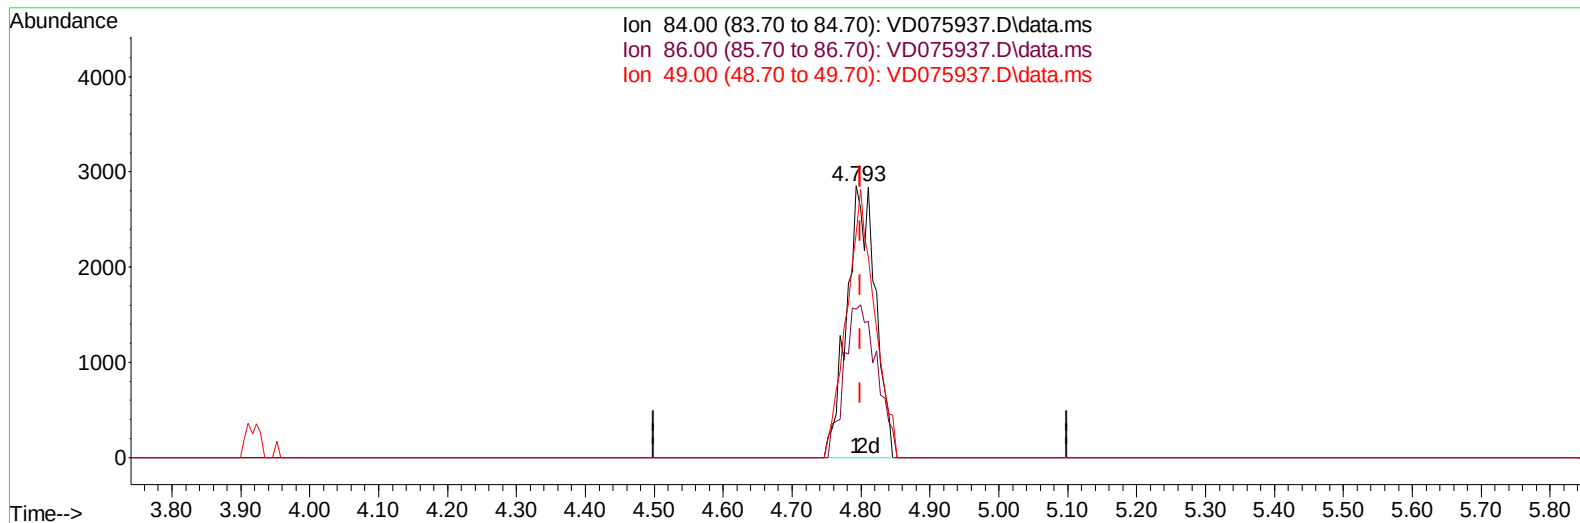

TIC: VD075937.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 4.42 ug/L m

response 8213

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	65.50	54.52
49.00	86.80	82.40
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075937.D
 Acq On : 01 May 2023 14:01
 Operator : KP/SY
 Sample : 02548-29RE
 Misc : 6.22G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCQ9RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Semsettin Yesilyurt 05/02/2023

Quant Time: May 02 02:33:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 02:31:38 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		91559	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		109460	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		53503	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.270	65		35346	17.598	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	70.400%		
7) Chloroethane-d5	2.799	69		39324	22.659	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.640%		
11) 1,1-Dichloroethene-d2	3.911	65		8653	18.686	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	74.760%		
21) 2-Butanone-d5	6.987	46		38476	220.659	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	441.320%#		
24) Chloroform-d	7.569	84		72498	31.664	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	126.640%		
26) 1,2-Dichloroethane-d4	8.234	65		43859	44.857	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	179.440%#		
32) Benzene-d6	8.205	84		121602	19.060	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	76.240%		
36) 1,2-Dichloropropane-d6	9.210	67		45983	26.040	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	104.160%		
41) Toluene-d8	10.269	98		97314	16.293	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	65.160%		
43) trans-1,3-Dichloroprop...	10.522	79		21743	29.789	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	119.160%		
47) 2-Hexanone-d5	10.881	63		29154	137.116	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	274.240%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		80816	59.807	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	239.240%#		
66) 1,2-Dichlorobenzene-d4	13.816	152		51347	27.132	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	108.520%		
Target Compounds							
13) Acetone	4.022	43		14756	98.888	ug/L	91
16) Methylene chloride	4.793	84		8213m	4.422	ug/L	
46) Tetrachloroethene	10.810	164		7284	5.187	ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
Data File : VD075937.D
Acq On : 01 May 2023 14:01
Operator : KP/SY
Sample : 02548-29RE
Misc : 6.22G/10.00mL/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCQ9RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Semsettin Yesilyurt 05/02/2023

Quant Time: May 02 02:33:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 02:31:38 2023
Response via : Initial Calibration

