




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075938.D
 Acq On : 01 May 2023 14:31
 Operator : KP/SY
 Sample : 02548-30
 Misc : 6.03G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR0

Manual IntegrationsAPPROVED

Quant Time: May 02 02:33:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 02:31:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Semsettin Yesilyurt 05/02/2023

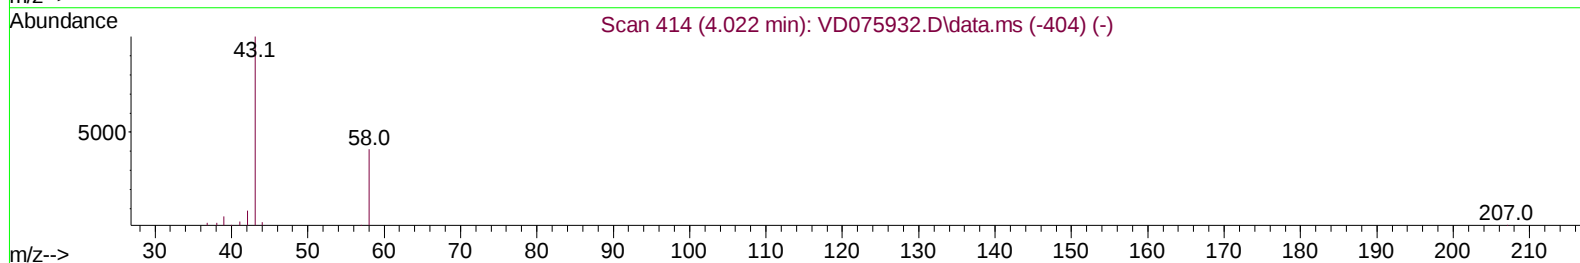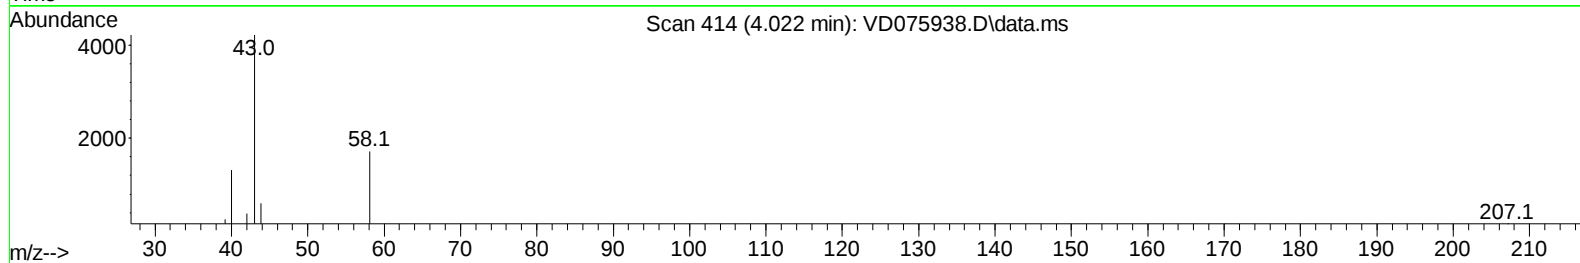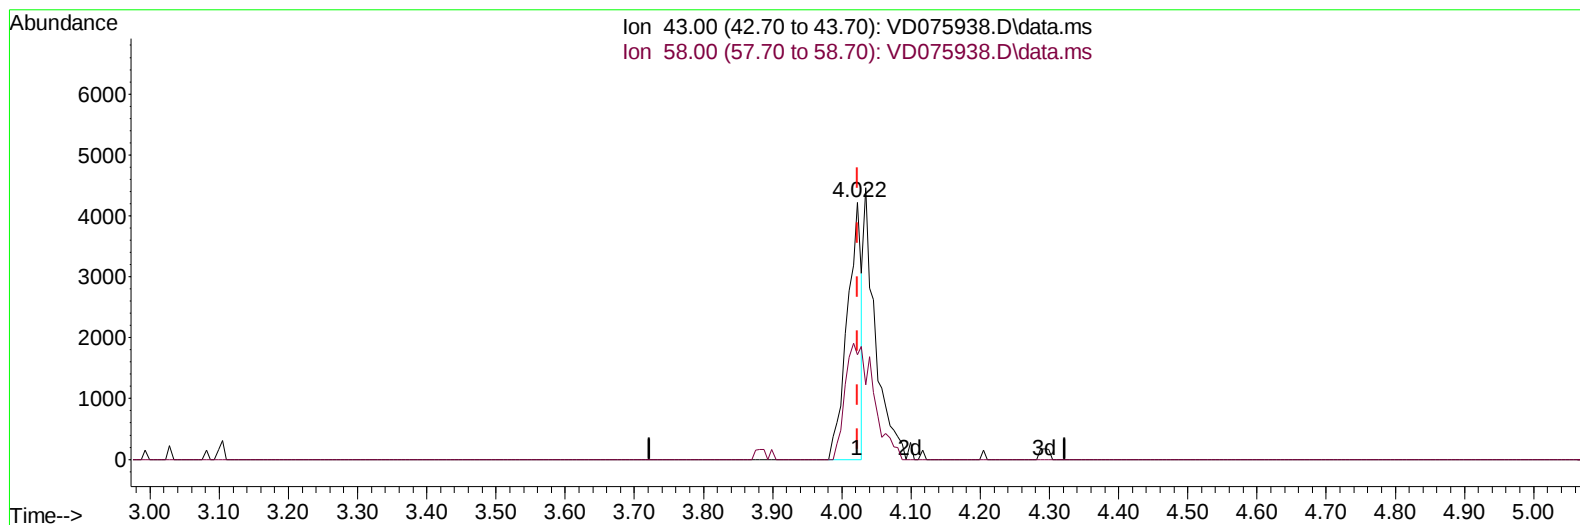

TIC: VD075938.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 7.86 ug/L

response 6059

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	60.27
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075938.D
 Acq On : 01 May 2023 14:31
 Operator : KP/SY
 Sample : 02548-30
 Misc : 6.03G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR0

Manual IntegrationsAPPROVED

Quant Time: May 02 02:33:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 02:31:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Semsettin Yesilyurt 05/02/2023

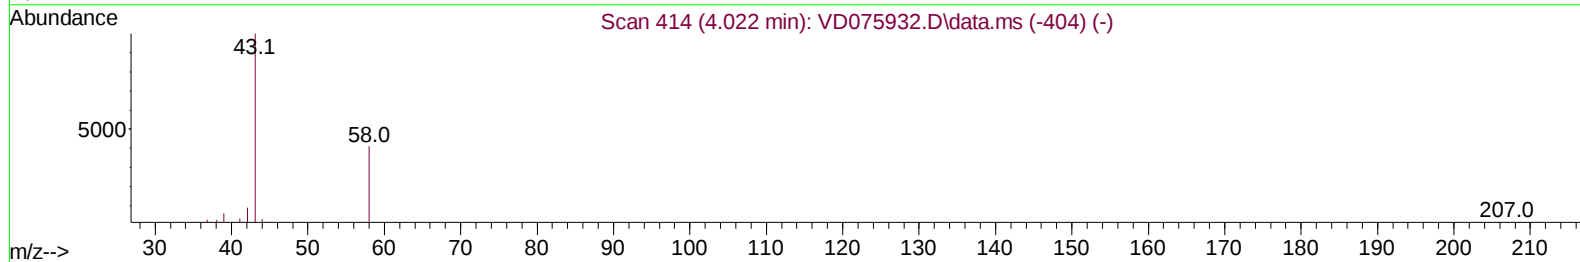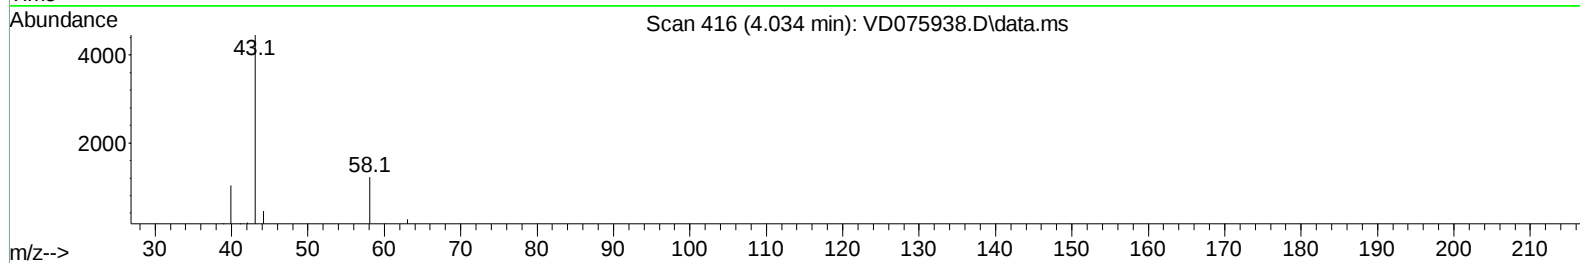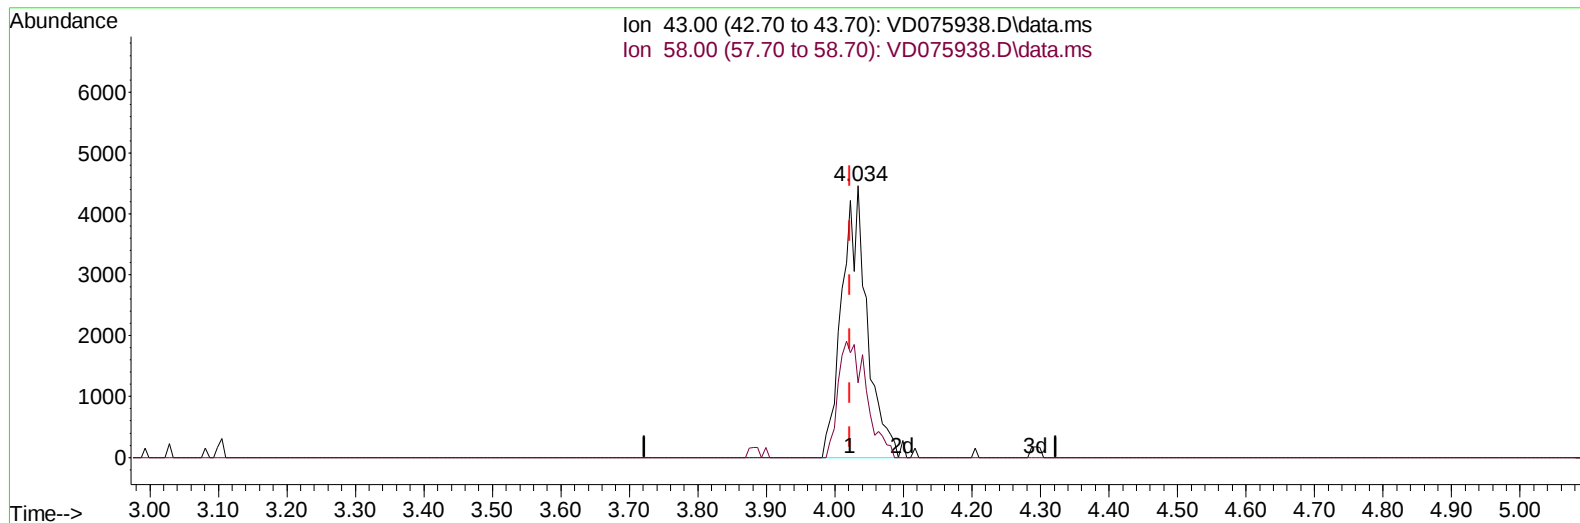

TIC: VD075938.D\data.ms

(13) Acetone (T)

4.034min (+ 0.012) 14.68 ug/L m

response 11317

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	32.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075938.D
 Acq On : 01 May 2023 14:31
 Operator : KP/SY
 Sample : 02548-30
 Misc : 6.03G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 DCCR0

Manual IntegrationsAPPROVED

Quant Time: May 02 02:33:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 02 02:31:38 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/02/2023
 Supervised By :Semsettin Yesilyurt 05/02/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		473138	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.587	117		497083	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		230950	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		140559	13.542	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	54.160%		
7) Chloroethane-d5	2.799	69		141585	15.788	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	63.160%		
11) 1,1-Dichloroethene-d2	3.916	65		33877	14.157	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	56.640%		
21) 2-Butanone-d5	6.987	46		56324	62.508	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	125.020%		
24) Chloroform-d	7.569	84		240021	20.286	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	81.160%		
26) 1,2-Dichloroethane-d4	8.228	65		116508	23.059	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	92.240%		
32) Benzene-d6	8.204	84		439768	15.179	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	60.720%		
36) 1,2-Dichloropropane-d6	9.210	67		154220	19.231	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	76.920%		
41) Toluene-d8	10.269	98		399888	14.743	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	58.960%		
43) trans-1,3-Dichloroprop...	10.528	79		59494	17.949	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.800%		
47) 2-Hexanone-d5	10.881	63		48036	49.749	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	99.500%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84		152049	24.778	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	99.120%		
66) 1,2-Dichlorobenzene-d4	13.816	152		167141	20.460	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	81.840%		
Target Compounds							
13) Acetone	4.034	43		11317m	14.676	ug/L	
16) Methylene chloride	4.799	84		35886	3.739	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
Data File : VD075938.D
Acq On : 01 May 2023 14:31
Operator : KP/SY
Sample : 02548-30
Misc : 6.03G/10.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
DCCR0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/02/2023
Supervised By :Semsettin Yesilyurt 05/02/2023

Quant Time: May 02 02:33:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 02 02:31:38 2023
Response via : Initial Calibration

