
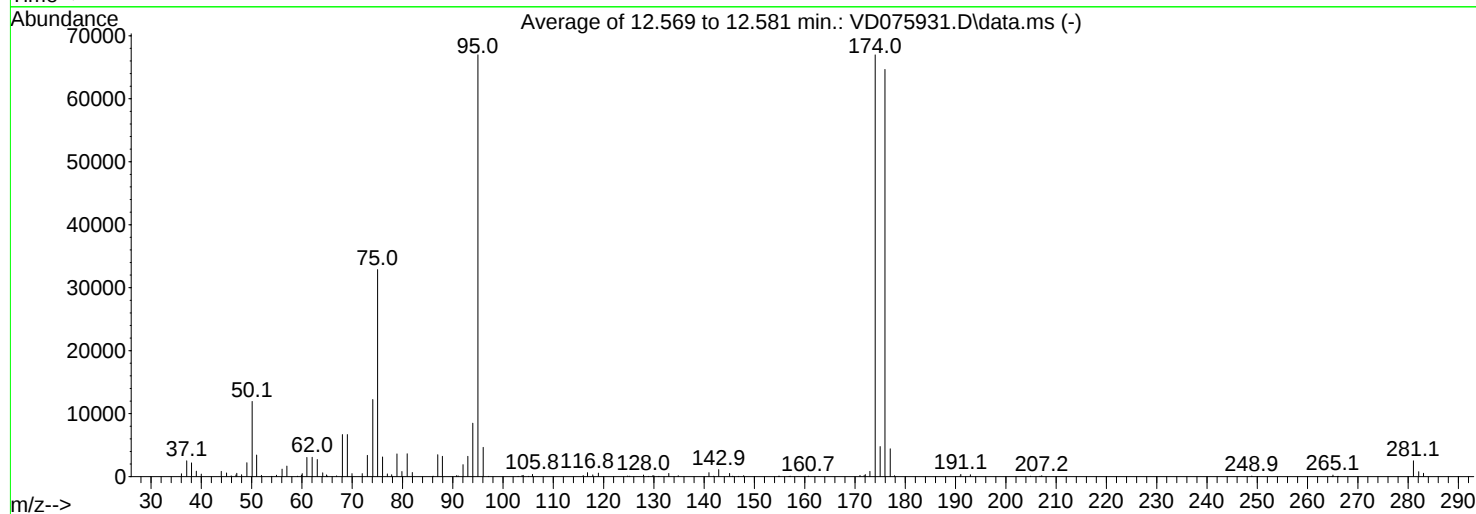


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050123\
 Data File : VD075931.D
 Acq On : 01 May 2023 10:30
 Operator : KP/SY
 Sample : BFB123
 Misc : 5.00G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB123

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Title : SFAM01.0
 Last Update : Tue May 02 02:31:38 2023

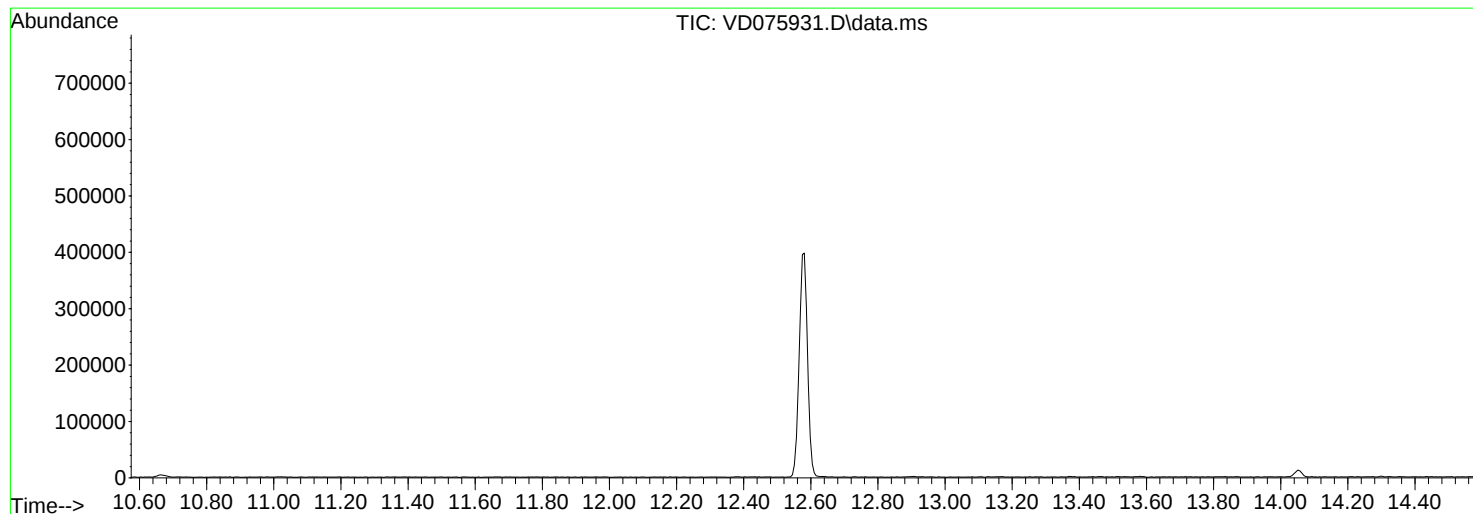

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	11940	PASS
75	95	30	80	49.1	32867	PASS
95	95	100	100	100.0	66963	PASS
96	95	5	9	6.9	4641	PASS
173	174	0.00	2	1.3	839	PASS
174	95	50	120	100.0	66971	PASS
175	174	5	9	7.1	4772	PASS
176	174	95	105	96.6	64664	PASS
177	176	5	10	6.8	4423	PASS

Scan 1860 (12.528 min): VD075931.D\data.ms
BFB123

m/z	Abundance
40.00	856.0
44.20	530.0

Instrument :
MSVOA_D
ClientSampleId :
BFB123

m/z	Abundance
36.10	339.0
37.10	2598.0
38.00	1926.0
39.00	893.0
40.00	1344.0
44.00	966.0
45.10	573.0
46.90	818.0
48.00	294.0
49.00	1884.0
50.10	10030.0
51.00	2897.0
52.00	196.0
54.00	178.0
54.90	183.0
56.10	1042.0
57.00	1576.0
59.90	790.0
61.00	2560.0
62.00	2733.0
63.10	2331.0
64.20	508.0
64.90	451.0
68.10	5552.0
69.00	6272.0
70.00	313.0
72.00	409.0
73.00	3202.0
74.10	11226.0
75.10	28152.0
76.10	2923.0
76.90	525.0
77.90	285.0
78.90	3385.0
79.90	570.0
80.90	3184.0
81.90	568.0
87.10	2729.0
88.00	2420.0
90.70	193.0
91.10	188.0
92.00	1534.0
93.00	2629.0
94.00	7119.0
95.00	54944.0
96.10	4216.0
104.10	157.0
105.80	301.0
115.90	214.0
116.70	504.0
118.00	222.0
119.00	308.0
127.90	177.0
129.80	337.0
131.00	160.0
133.00	390.0
141.00	748.0
142.90	890.0
145.10	276.0
156.90	168.0
172.00	273.0
173.00	1010.0
174.00	52280.0
175.00	3845.0
175.90	50352.0
177.00	3425.0
177.80	207.0
190.90	313.0
192.90	242.0
207.20	247.0
264.90	169.0
281.00	1288.0
282.00	484.0
283.10	344.0

Instrument :
MSVOA_D
ClientSampleId :
BFB123

m/z	Abundance
36.00	380.0
37.10	2319.0
38.10	2389.0
38.90	699.0
40.00	1134.0
43.90	662.0
45.00	765.0
46.00	197.0
47.10	745.0
48.00	353.0
49.10	2248.0
50.10	13421.0
51.00	3862.0
52.00	184.0
55.00	269.0
56.10	1471.0
57.00	1780.0
60.10	624.0
61.00	3641.0
62.00	3449.0
63.00	2923.0
64.00	573.0
64.90	406.0
67.00	180.0
68.00	7427.0
69.00	7099.0
70.00	547.0
72.00	691.0
73.00	3421.0
74.10	12743.0
75.10	35184.0
76.00	3339.0
77.00	321.0
77.90	281.0
78.90	3813.0
79.90	906.0
80.90	4213.0
82.00	792.0
87.00	3801.0
87.90	3863.0
91.00	236.0
92.10	2181.0
93.00	3284.0
94.00	9530.0
95.00	73896.0
96.00	5140.0
103.00	200.0
103.80	547.0
105.10	157.0
105.90	278.0
116.00	351.0
116.80	585.0
117.80	349.0
118.90	700.0
127.80	171.0
128.90	157.0
129.80	200.0
133.00	530.0
134.80	293.0
140.90	543.0
142.90	1138.0
145.00	579.0
147.80	247.0
154.80	218.0
160.70	223.0
171.00	394.0
172.10	744.0
173.00	721.0
174.00	72312.0
175.00	5147.0
176.00	71216.0
177.00	4992.0
191.10	474.0
192.90	227.0
206.80	273.0
265.10	371.0
265.90	171.0
281.10	2767.0
282.10	777.0
283.00	588.0

Instrument :
MSVOA_D
ClientSampleId :
BFB123

m/z	Abundance
36.00	630.0
37.10	2643.0
38.10	2262.0
39.10	976.0
40.10	1278.0
44.00	899.0
44.90	390.0
45.90	157.0
47.00	870.0
48.00	287.0
49.00	2478.0
50.10	12368.0
51.00	3543.0
51.90	203.0
54.90	221.0
56.00	1047.0
57.00	1718.0
59.10	219.0
60.00	797.0
61.00	2977.0
62.10	3065.0
63.10	2902.0
64.20	723.0
65.10	272.0
66.80	216.0
68.10	7037.0
69.10	6679.0
69.90	576.0
71.90	359.0
73.00	3494.0
74.10	12804.0
75.00	35264.0
76.00	3150.0
77.10	434.0
77.80	371.0
78.90	3626.0
79.90	958.0
81.00	3493.0
82.00	612.0
86.10	221.0
86.90	3922.0
87.90	3434.0
90.80	289.0
92.00	1974.0
93.00	3800.0
94.00	8808.0
95.00	72048.0
96.00	4566.0
97.10	196.0
104.00	494.0
105.80	506.0
116.90	814.0
117.80	294.0
119.00	670.0
124.80	345.0
125.20	227.0
128.00	429.0
130.00	426.0
132.90	619.0
134.90	171.0
140.90	654.0
141.90	209.0
142.90	1314.0
145.00	653.0
145.70	207.0
146.80	170.0
147.90	201.0
155.00	213.0
157.10	217.0
171.00	221.0
171.80	543.0
172.90	786.0
174.00	76320.0
175.00	5324.0
176.00	72424.0
177.00	4851.0
177.90	256.0
191.00	614.0
193.00	456.0
204.90	243.0
207.10	244.0
248.90	323.0
265.00	418.0
266.10	195.0
281.10	3473.0
282.20	1083.0
283.10	704.0

Instrument :
MSVOA_D
ClientSampleId :
BFB123