




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050423\
Data File : VD076000.D
Acq On : 04 May 2023 13:06
Operator : KP/SY
Sample : 02589-10
Misc : 4.68G/10.00mL/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREC7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/05/2023
Supervised By :Semsettin Yesilyurt 05/05/2023

Quant Time: May 05 00:49:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 00:35:29 2023
Response via : Initial Calibration

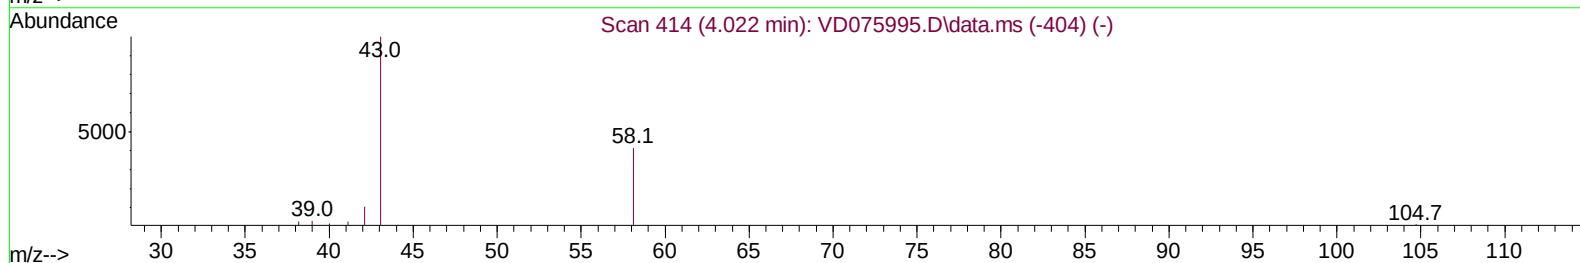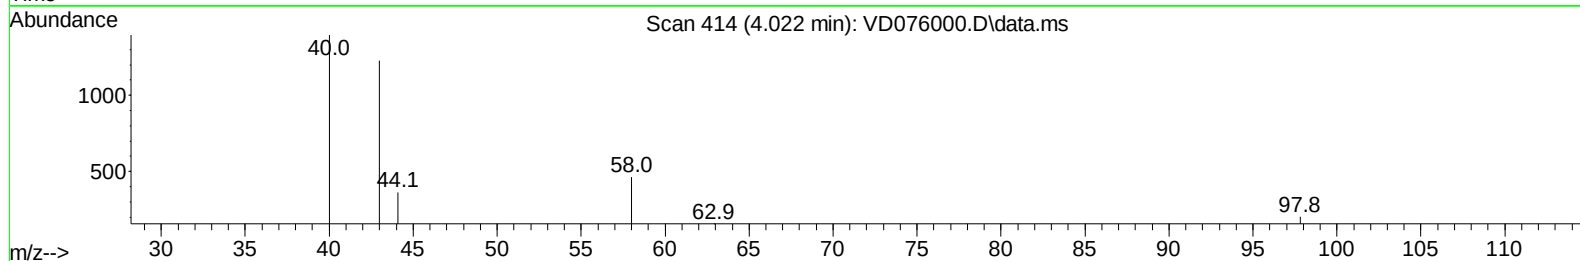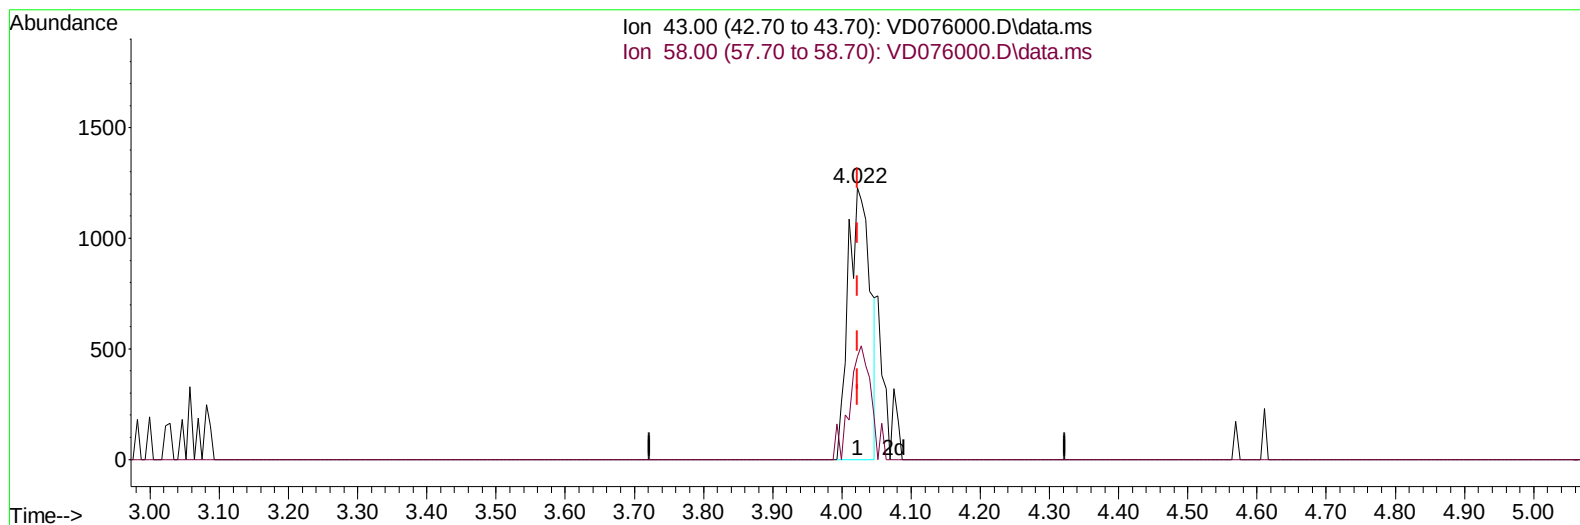

TIC: VD076000.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 3.38 ug/L

response 2675

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	36.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050423\
 Data File : VD076000.D
 Acq On : 04 May 2023 13:06
 Operator : KP/SY
 Sample : 02589-10
 Misc : 4.68G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREC7

Manual IntegrationsAPPROVED

Quant Time: May 05 00:49:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 00:35:29 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/05/2023
 Supervised By :Semsettin Yesilyurt 05/05/2023

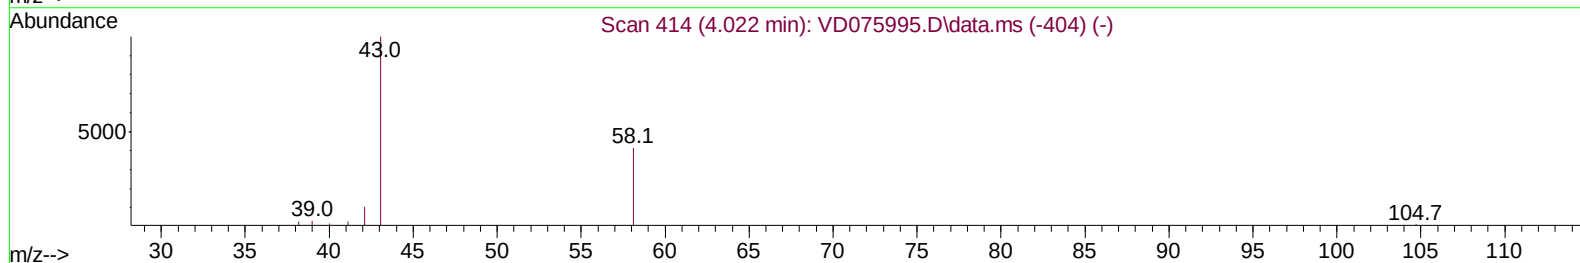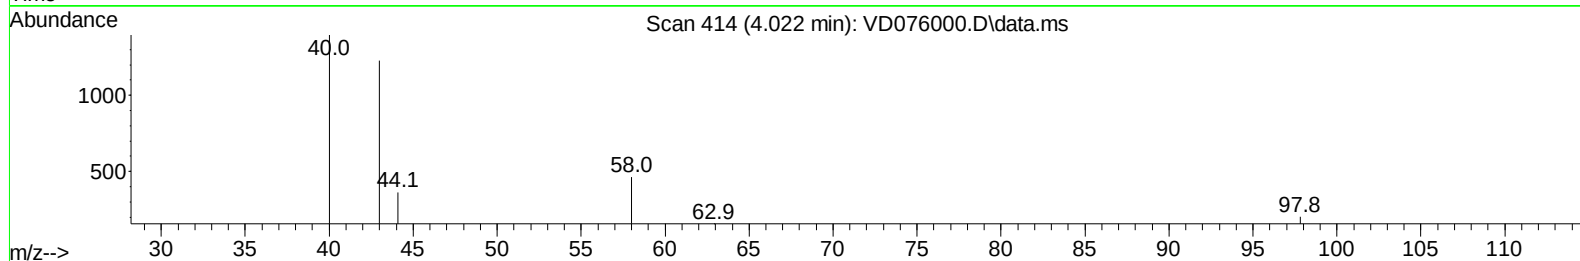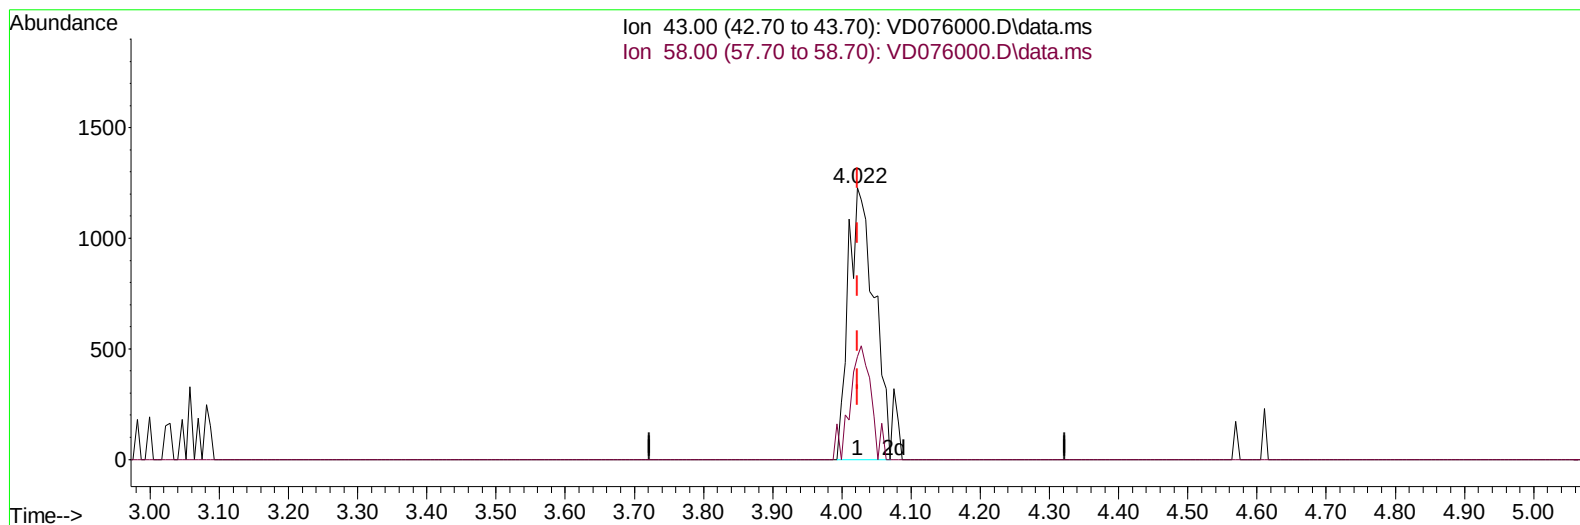

TIC: VD076000.D\data.ms

(13) Acetone (T)

4.022min (+ 0.000) 4.02 ug/L m

response 3183

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	30.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050423\
 Data File : VD076000.D
 Acq On : 04 May 2023 13:06
 Operator : KP/SY
 Sample : 02589-10
 Misc : 4.68G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 JREC7

Manual IntegrationsAPPROVED

Quant Time: May 05 00:49:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 00:35:29 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 05/05/2023
 Supervised By :Semsettin Yesilyurt 05/05/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		486253	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		358619	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		87708	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		173323	16.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	65.000%	
7) Chloroethane-d5	2.799	69		171198	18.575	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	74.280%	
11) 1,1-Dichloroethene-d2	3.922	65		41729	16.968	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	67.880%	
21) 2-Butanone-d5	6.987	46		47110	50.873	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	101.740%	
24) Chloroform-d	7.569	84		265208	21.811	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	87.240%	
26) 1,2-Dichloroethane-d4	8.228	65		113529	21.863	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	87.440%	
32) Benzene-d6	8.199	84		474322	22.693	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	90.760%	
36) 1,2-Dichloropropane-d6	9.210	67		162487	28.086	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	112.360%	
41) Toluene-d8	10.269	98		386399	19.746	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	79.000%	
43) trans-1,3-Dichloroprop...	10.528	79		51017	21.334	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	85.320%	
47) 2-Hexanone-d5	10.875	63		36875	52.935	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	105.880%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		115104	26.000	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	104.000%	
66) 1,2-Dichlorobenzene-d4	13.816	152		74144	23.899	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	95.600%	
Target Compounds							
13) Acetone	4.022	43		3183m	4.017	ug/L	
16) Methylene chloride	4.805	84		22847	2.316	ug/L	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050423\
Data File : VD076000.D
Acq On : 04 May 2023 13:06
Operator : KP/SY
Sample : 02589-10
Misc : 4.68G/10.00mL/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
JREC7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 05/05/2023
Supervised By :Semsettin Yesilyurt 05/05/2023

Quant Time: May 05 00:49:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 00:35:29 2023
Response via : Initial Calibration

