


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050622\
 Data File : VD072843.D
 Acq On : 06 May 2022 10:05
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Title : SW846 8260
 Last Update : Tue May 03 08:33:49 2022

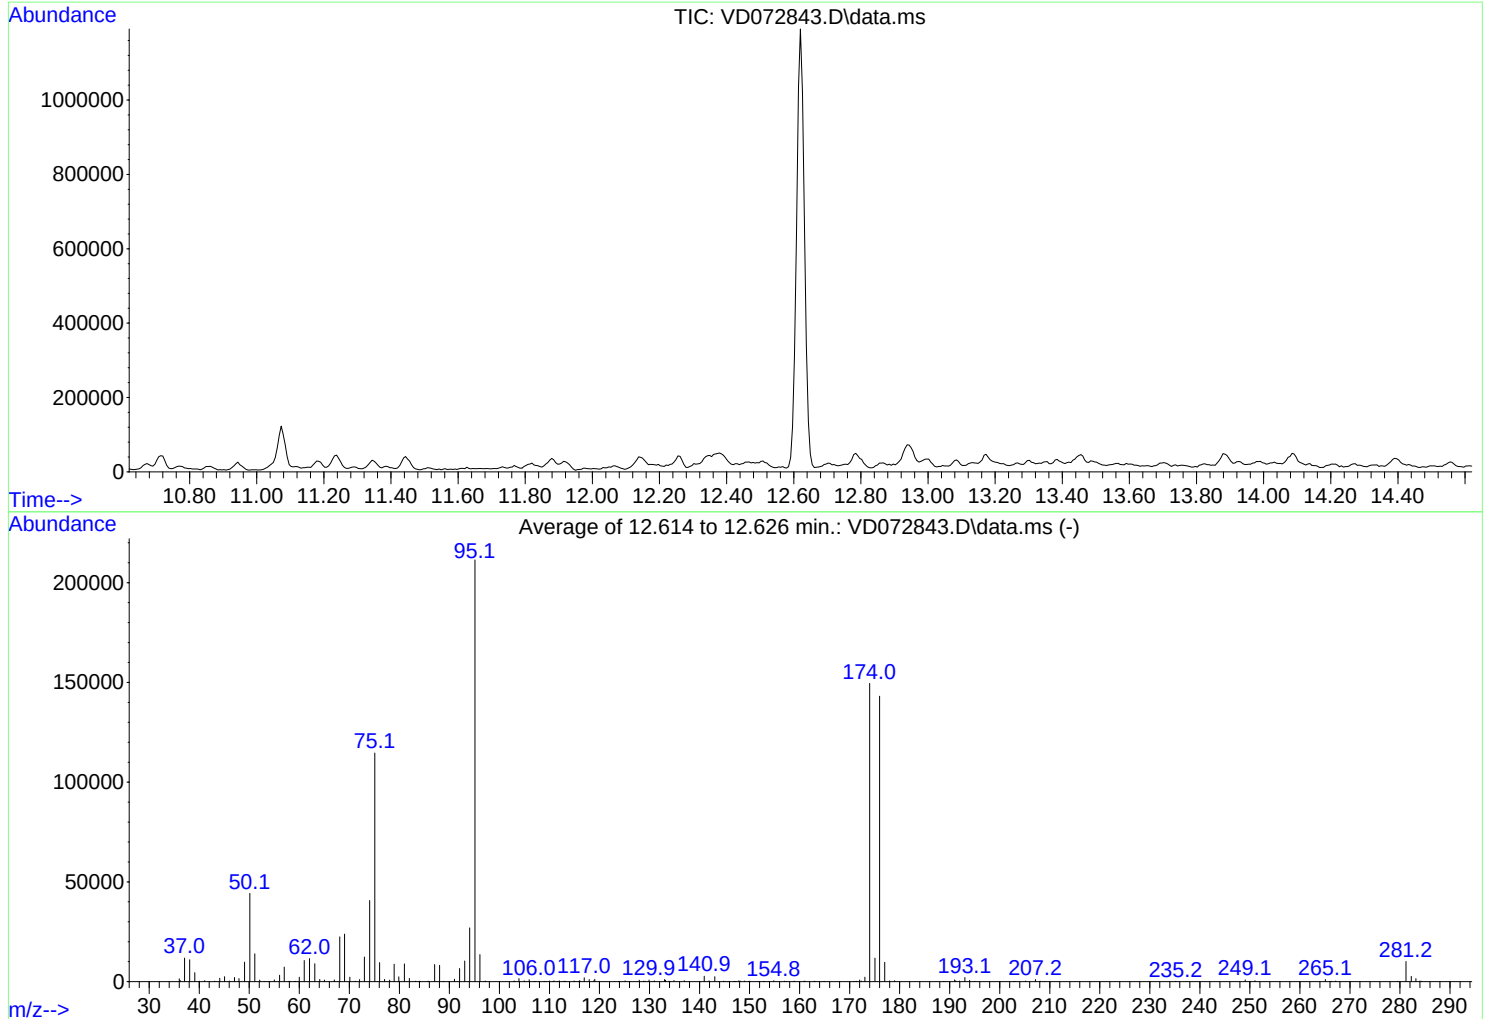

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1805

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	44277	PASS
75	95	30	60	54.2	114648	PASS
95	95	100	100	100.0	211456	PASS
96	95	5	9	6.4	13568	PASS
173	174	0.00	2	1.5	2286	PASS
174	95	50	100	70.7	149483	PASS
175	174	5	9	7.9	11780	PASS
176	174	95	101	95.7	143077	PASS
177	176	5	9	6.8	9678	PASS