
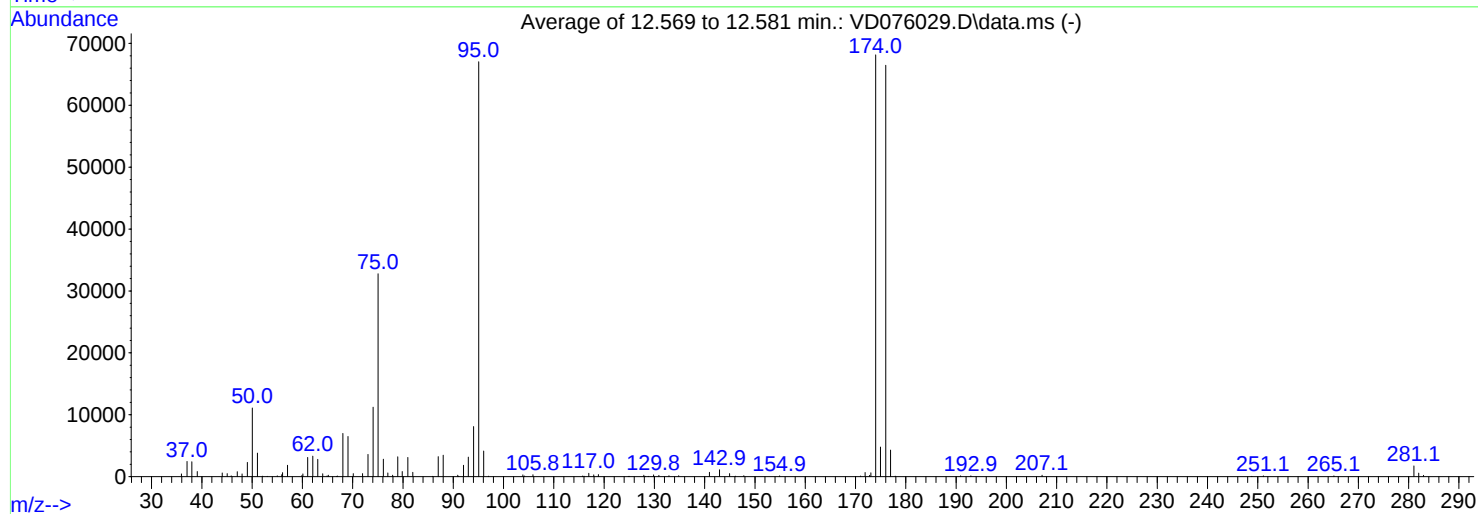


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050823\
Data File : VD076029.D
Acq On : 08 May 2023 09:12
Operator : KP/SY
Sample : BFB128
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB128

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Sat May 06 00:21:26 2023

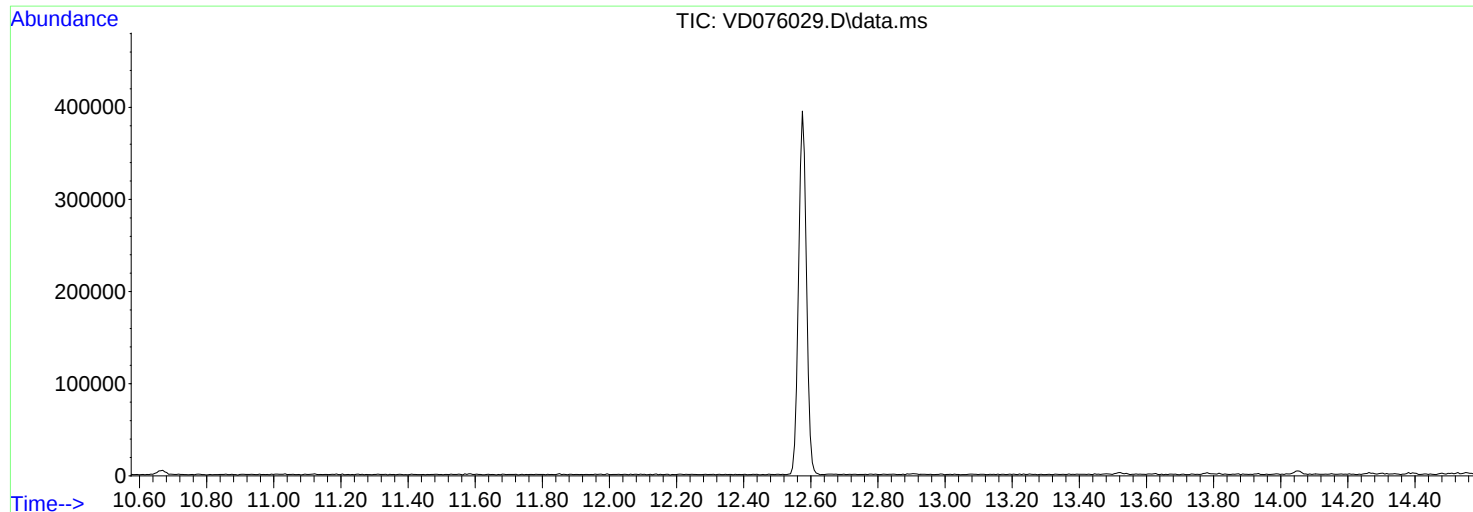

Spectrum Information: Average of 12.569 to 12.581 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	11089	PASS
75	95	30	80	48.9	32795	PASS
95	95	100	100	100.0	67043	PASS
96	95	5	9	6.2	4135	PASS
173	174	0.00	2	0.9	627	PASS
174	95	50	120	101.7	68155	PASS
175	174	5	9	7.0	4790	PASS
176	174	95	105	97.5	66472	PASS
177	176	5	10	6.5	4300	PASS