


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050823\
Data File : VD076029.D
Acq On : 08 May 2023 09:12
Operator : KP/SY
Sample : BFB128
Misc : 5.00G/10.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB128

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Sat May 06 00:21:26 2023

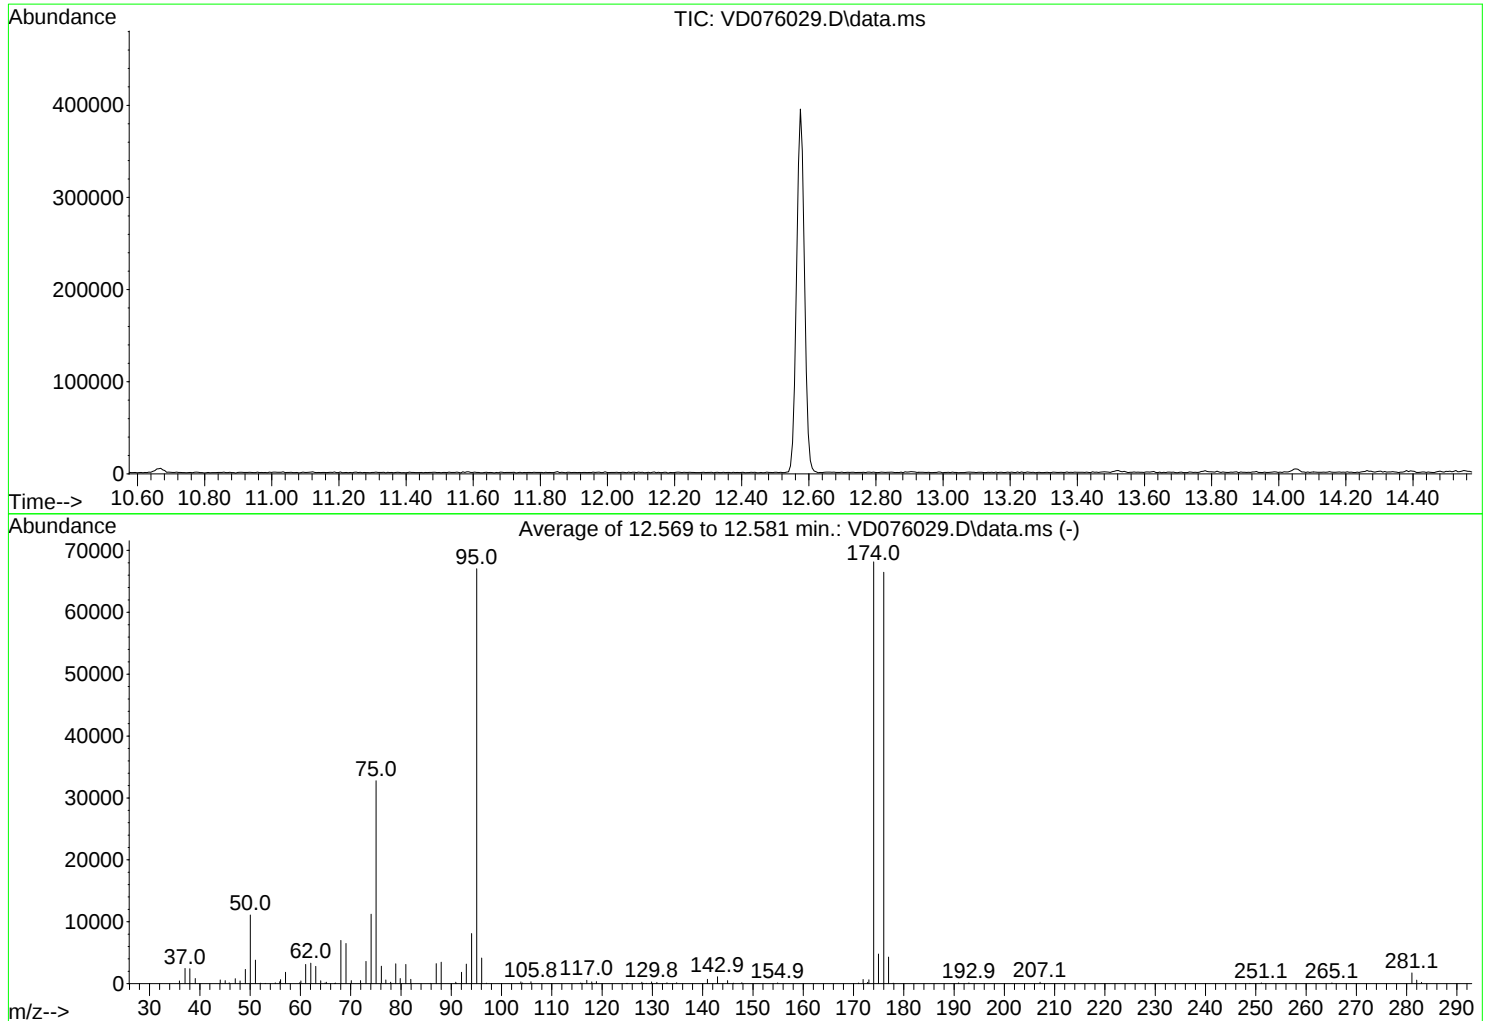

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	11089	PASS
75	95	30	80	48.9	32795	PASS
95	95	100	100	100.0	67043	PASS
96	95	5	9	6.2	4135	PASS
173	174	0.00	2	0.9	627	PASS
174	95	50	120	101.7	68155	PASS
175	174	5	9	7.0	4790	PASS
176	174	95	105	97.5	66472	PASS
177	176	5	10	6.5	4300	PASS

m/z	Abundance
40.00	1155.0
44.20	246.0

Instrument :
MSVOA_D
ClientSampleId :
BFB128

m/z	Abundance
35.90	350.0
37.10	2241.0
38.00	2316.0
39.10	737.0
40.10	1095.0
44.10	995.0
45.10	529.0
47.20	457.0
48.00	474.0
49.00	2176.0
50.00	10912.0
51.10	3339.0
55.00	189.0
55.90	919.0
57.00	1759.0
59.90	549.0
61.00	2921.0
62.10	2869.0
63.10	2886.0
64.10	575.0
65.20	213.0
68.00	6834.0
69.10	6267.0
70.10	552.0
72.00	558.0
73.10	3097.0
74.10	11062.0
75.10	31752.0
76.10	2447.0
77.00	531.0
77.90	352.0
78.90	2788.0
79.80	898.0
80.90	2652.0
81.90	842.0
85.90	174.0
87.00	3036.0
88.00	3157.0
90.90	373.0
92.00	1622.0
93.00	2553.0
94.00	7648.0
95.10	64168.0
96.00	3998.0
103.90	438.0
106.00	328.0
117.00	538.0
118.00	300.0
118.90	346.0
124.80	168.0
128.00	251.0
128.80	169.0
129.90	275.0
130.90	161.0
133.00	240.0
134.90	162.0
141.00	728.0
143.00	862.0
145.00	482.0
155.00	216.0
171.80	563.0
172.80	663.0
174.00	60264.0
174.90	5029.0
176.00	61544.0
176.90	3924.0
207.10	222.0
281.10	1422.0
282.10	315.0
282.90	280.0

Instrument :
MSVOA_D
ClientSampleId :
BFB128

m/z	Abundance
36.00	673.0
37.00	2530.0
38.00	2671.0
39.10	884.0
40.00	1178.0
44.10	732.0
45.10	448.0
45.80	187.0
47.00	873.0
48.10	402.0
49.10	2615.0
50.10	12324.0
51.00	4666.0
56.10	1021.0
57.10	2073.0
60.10	653.0
61.10	3383.0
62.00	3990.0
63.00	3262.0
64.00	364.0
64.90	295.0
66.80	183.0
68.10	7931.0
69.00	7208.0
70.10	500.0
71.90	420.0
73.10	4509.0
74.00	11807.0
75.00	35048.0
76.10	3415.0
77.10	689.0
79.00	3625.0
79.90	902.0
81.00	3686.0
82.00	561.0
87.00	3570.0
88.00	3651.0
91.10	191.0
92.10	2203.0
93.00	3380.0
94.10	8618.0
95.10	73304.0
96.00	4534.0
103.80	406.0
105.80	350.0
115.70	310.0
117.00	590.0
117.90	266.0
118.80	296.0
125.00	180.0
127.90	299.0
129.80	266.0
130.90	199.0
134.90	163.0
141.00	676.0
143.00	1394.0
144.90	574.0
146.10	207.0
147.80	154.0
154.80	183.0
171.00	301.0
171.90	833.0
173.00	1132.0
174.00	75576.0
174.90	5099.0
176.00	73160.0
177.00	4905.0
177.90	266.0
191.00	153.0
192.90	203.0
207.20	159.0
251.10	191.0
265.10	185.0
281.00	1663.0
281.90	477.0

Instrument :
MSVOA_D
ClientSampleId :
BFB128

m/z	Abundance
36.00	331.0
37.00	2566.0
38.00	2262.0
39.10	842.0
40.00	1110.0
44.00	772.0
45.00	477.0
45.90	176.0
47.00	1063.0
47.90	434.0
49.00	2121.0
50.00	10030.0
51.10	3402.0
52.10	231.0
53.00	156.0
55.00	180.0
56.00	961.0
57.10	1712.0
60.10	656.0
61.00	3008.0
62.10	3051.0
63.00	2248.0
64.10	449.0
65.10	484.0
67.00	299.0
68.00	6173.0
69.00	6028.0
70.10	467.0
72.00	526.0
73.00	3151.0
74.00	10766.0
75.10	31584.0
76.10	2625.0
76.90	534.0
78.00	340.0
78.90	3218.0
79.90	676.0
80.90	2971.0
81.90	685.0
87.00	3134.0
88.00	3629.0
90.90	336.0
92.00	1722.0
93.00	3550.0
94.00	7988.0
95.00	63656.0
96.10	3873.0
97.00	269.0
104.20	281.0
105.80	240.0
116.00	226.0
116.80	550.0
118.00	283.0
118.90	341.0
127.80	173.0
128.20	157.0
129.80	298.0
130.90	286.0
132.80	211.0
134.80	164.0
140.90	662.0
142.90	1046.0
144.90	385.0
147.80	331.0
172.00	636.0
173.10	749.0
174.00	68624.0
175.00	4241.0
176.00	64712.0
177.00	4070.0
190.80	211.0
193.00	210.0
207.00	306.0
248.80	161.0
251.10	171.0
265.20	214.0
281.10	2093.0
282.00	888.0
283.00	349.0

Instrument :
MSVOA_D
ClientSampleId :
BFB128