

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD051519\
 Data File : VD062397.D
 Acq On : 15 May 2019 19:25
 Operator : FY/SY
 Sample : K2837-01
 Misc : 6.88g/5mL/MSVOA D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: May 16 03:59:16 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 07 14:26:29 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.02
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.19
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-12.35
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-14.51

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD051519\
Data File : VD062397.D
Acq On : 15 May 2019 19:25
Operator : FY/SY
Sample : K2837-01
Misc : 6.88g/5mL/MSVOA D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: May 16 03:59:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Quant Title : SW846 8260
QLast Update : Tue May 07 14:26:29 2019
Response via : Initial Calibration

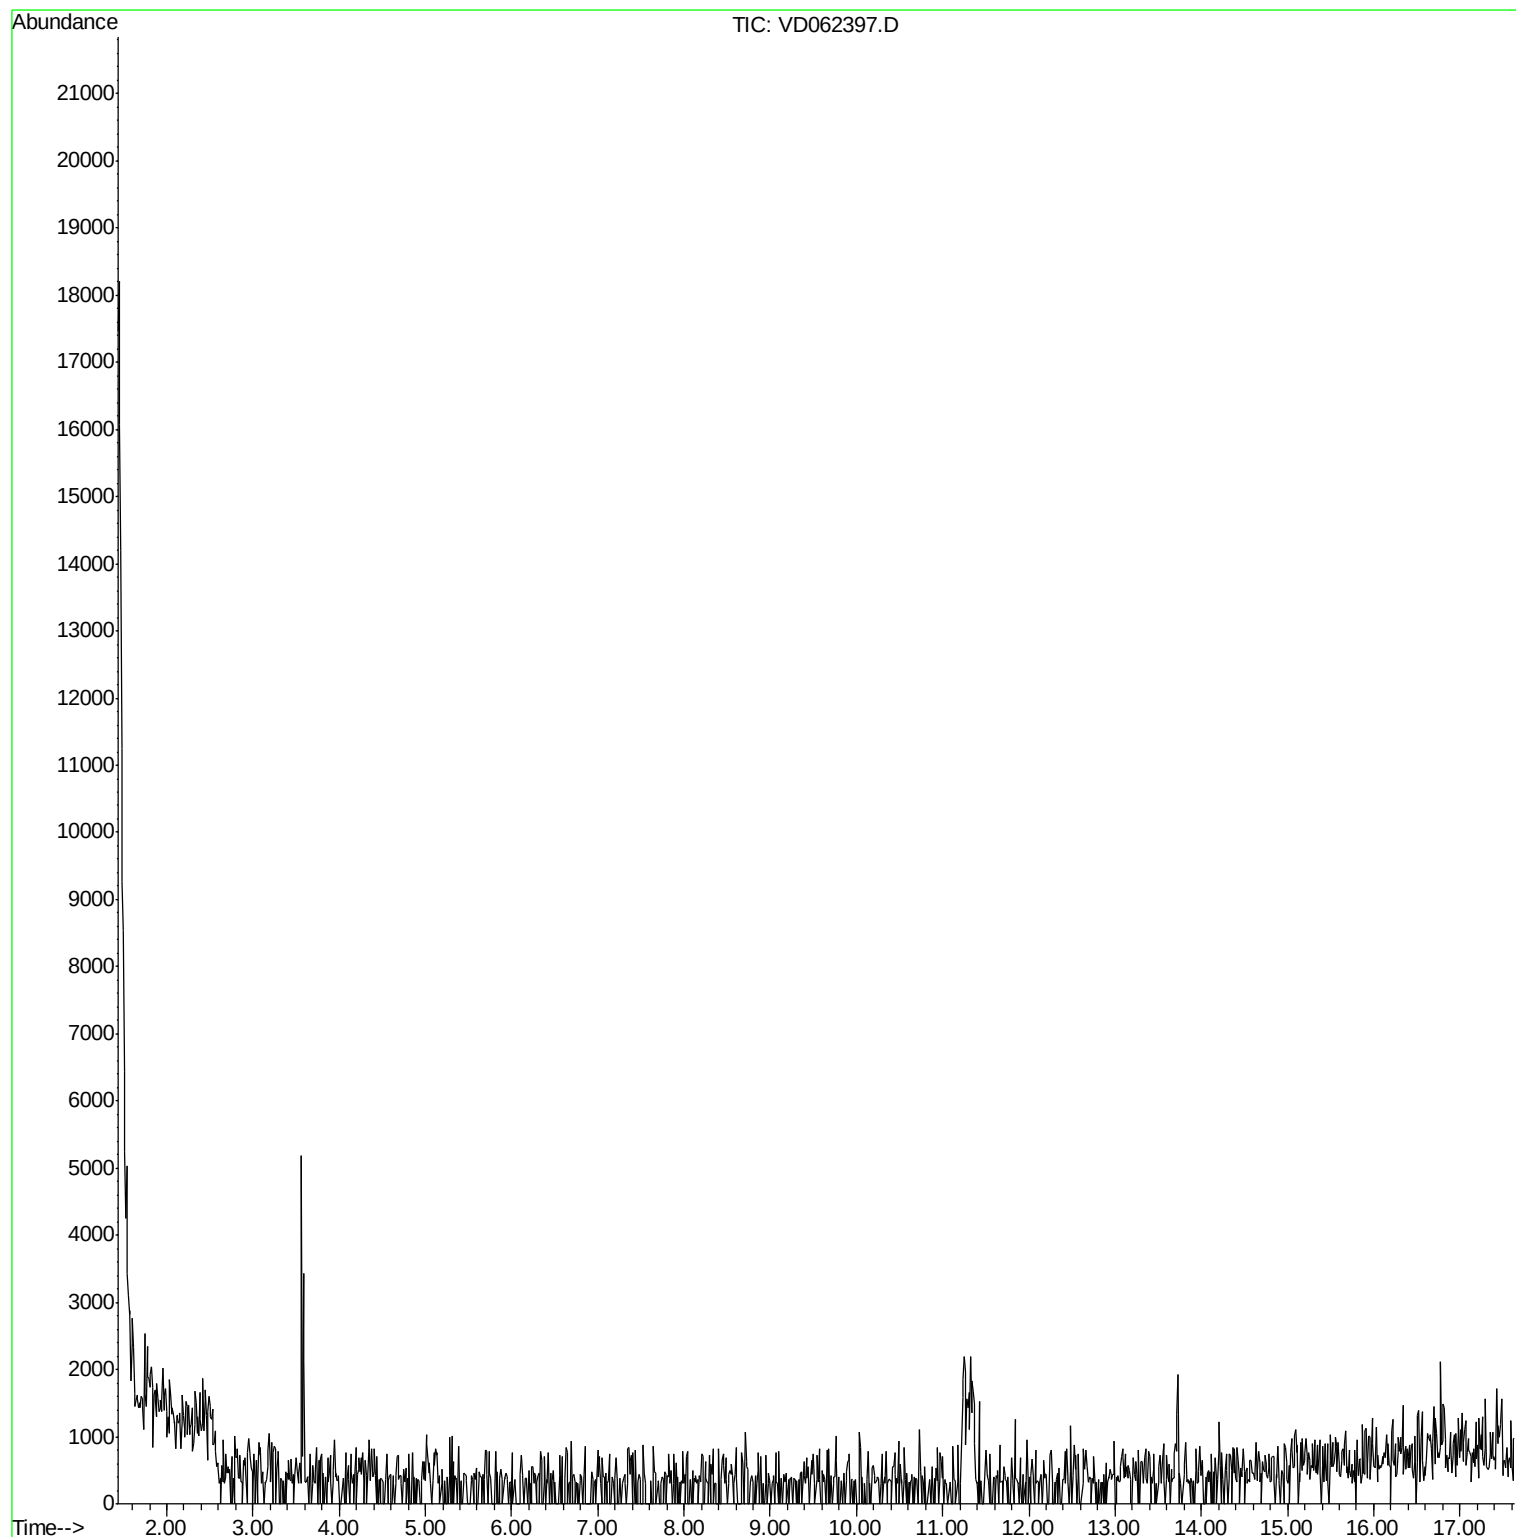

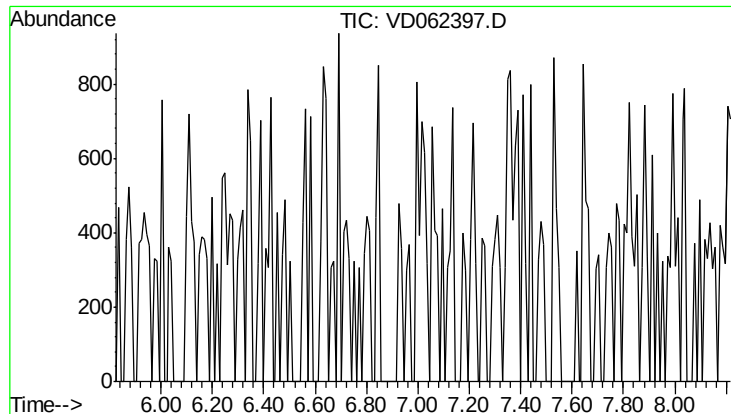

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.02 min

Lab File: VD062397.D

Acq: 15 May 2019 19:25

Tot Ion: 168

Sig Exp Ratio



168 100

99 58.1

Instrument :

MSVOA_D

ClientSampleId :

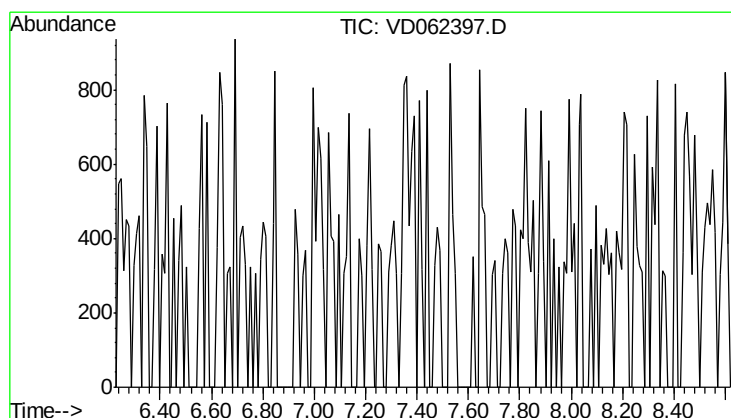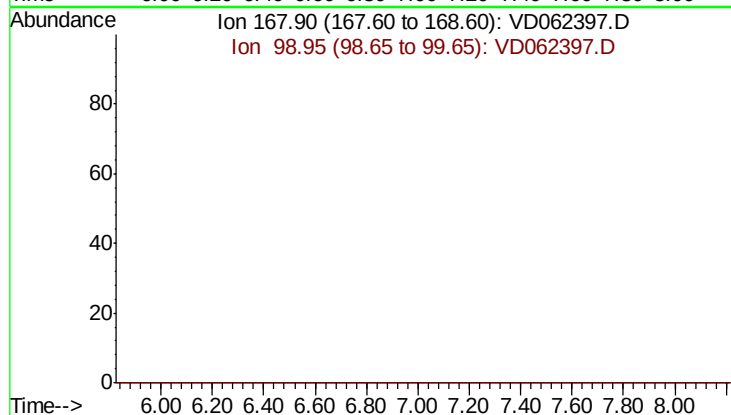

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 7.42 min

Lab File: VD062397.D


Acq: 15 May 2019 19:25


Tgt Ion: 65

Sig Exp Ratio

65 100

67 49.0

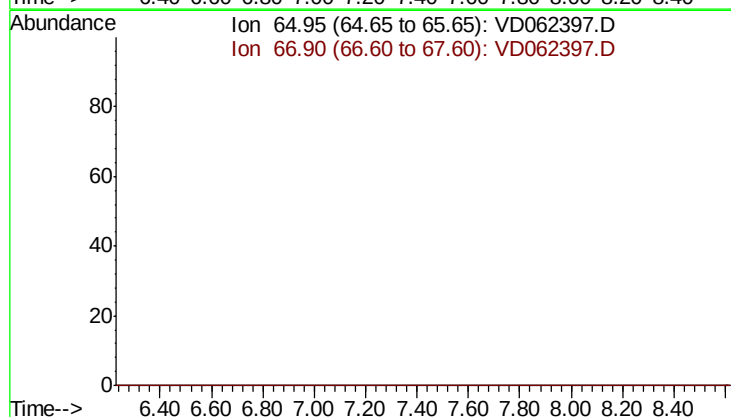

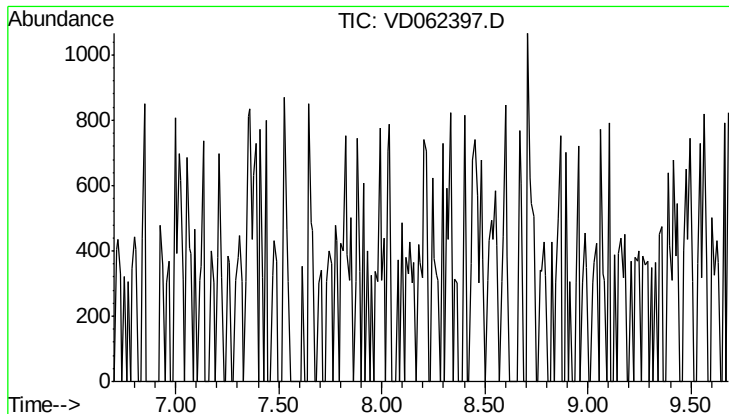

#34

1,4-Difluorobenzene

Concen: 0.000 ug/l

Expected RT: 8.19 min

Lab File: VD062397.D

Acq: 15 May 2019 19:25

Instrument :

MSVOA_D

ClientSampleId :



Tot Ion: 114

Sig Exp Ratio

114 100

63 16.2

88 16.8

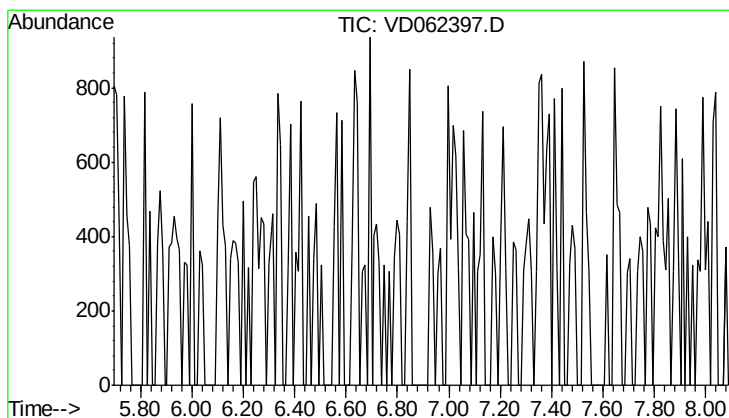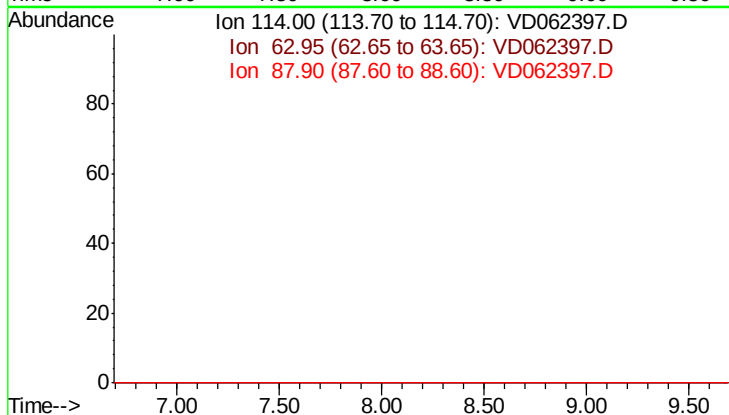

#35

Dibromofluoromethane

Concen: 0.000 ug/l

Expected RT: 6.89 min

Lab File: VD062397.D

Acq: 15 May 2019 19:25


Tgt Ion: 113


Sig Exp Ratio

113 100

111 98.1

192 16.2

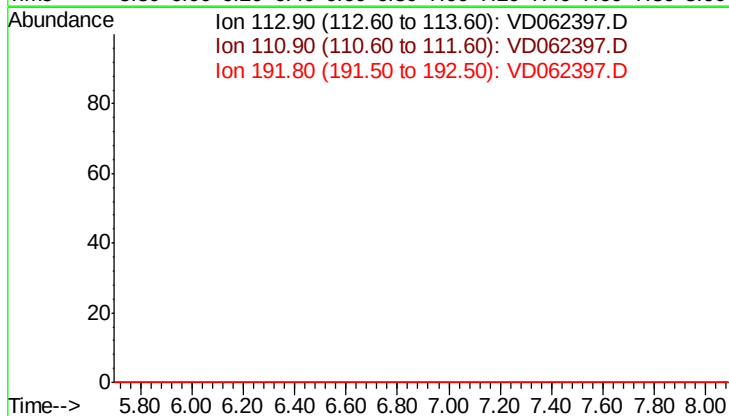


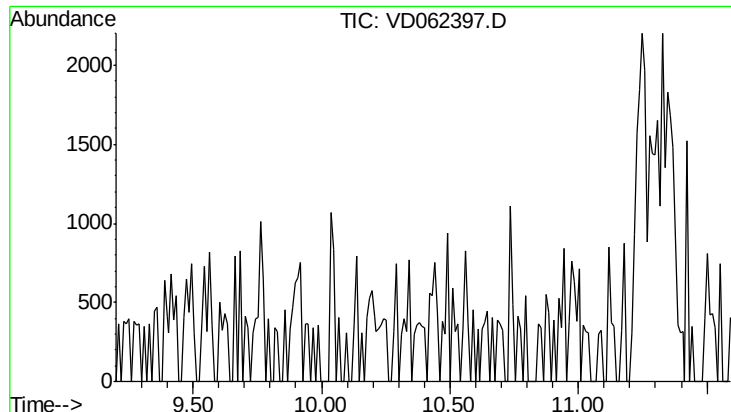


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.40 min

Lab File: VD062397.D
Acq: 15 May 2019 19:25

Instrument :
MSVOA_D
ClientSampleId :


Tot Ion	98
Sig	Exp Ratio
98	100
100	67.3

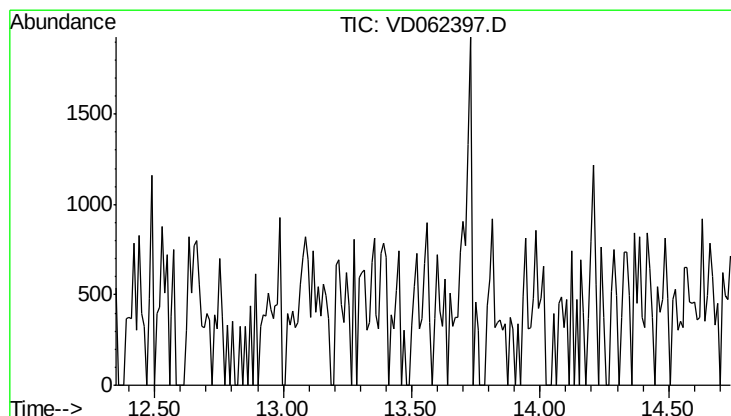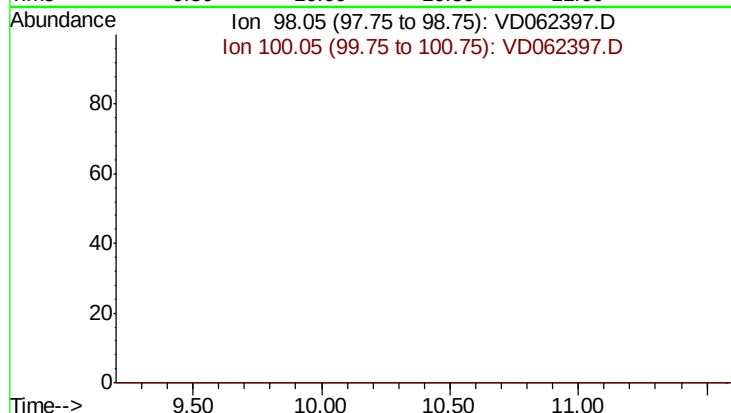


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 13.55 min

Lab File: VD062397.D
Acq: 15 May 2019 19:25

Tgt Ion	95
Sig	Exp Ratio
95	100
174	90.9
176	87.2


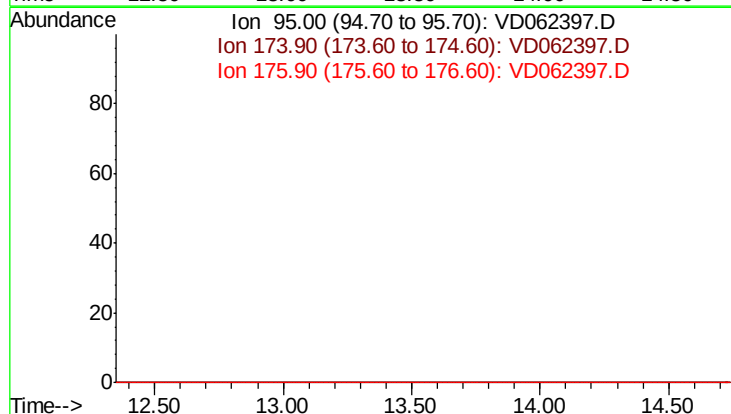


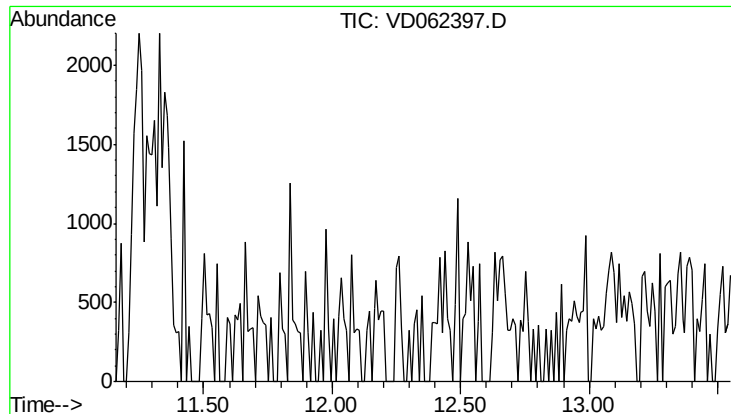

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 12.35 min
 Lab File: VD062397.D
 Acq: 15 May 2019 19:25

Instrument :
 MSVOA_D
 ClientSampleId :

Tot Ion	117
Sig	Exp Ratio
117	100
82	45.2
119	32.8

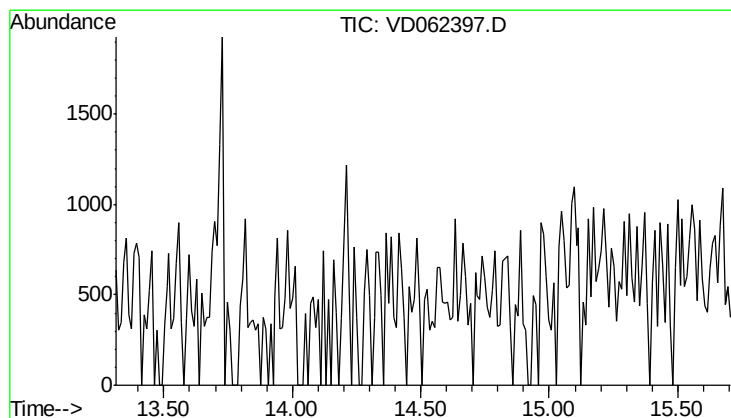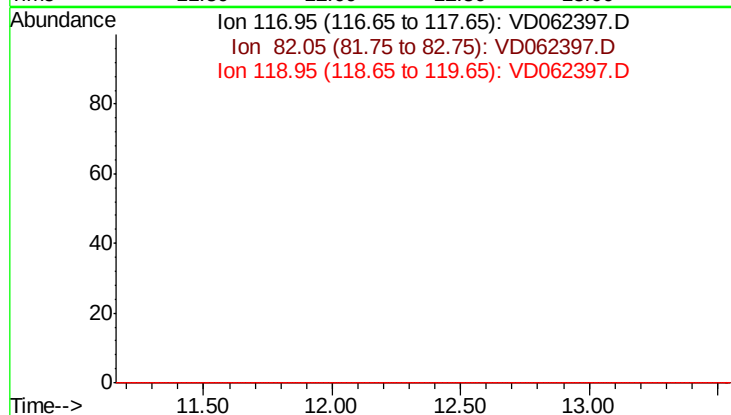

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 14.51 min
 Lab File: VD062397.D
 Acq: 15 May 2019 19:25

Tgt Ion	152
Sig	Exp Ratio
152	100
115	61.8
150	157.4

