


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD051519\
 Data File : VD062384.D
 Acq On : 15 May 2019 13:08
 Operator : FY/SY
 Sample : BFB
 Misc : 5.00µ/5mL/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
 Title : SW846 8260
 Last Update : Tue May 07 14:26:29 2019

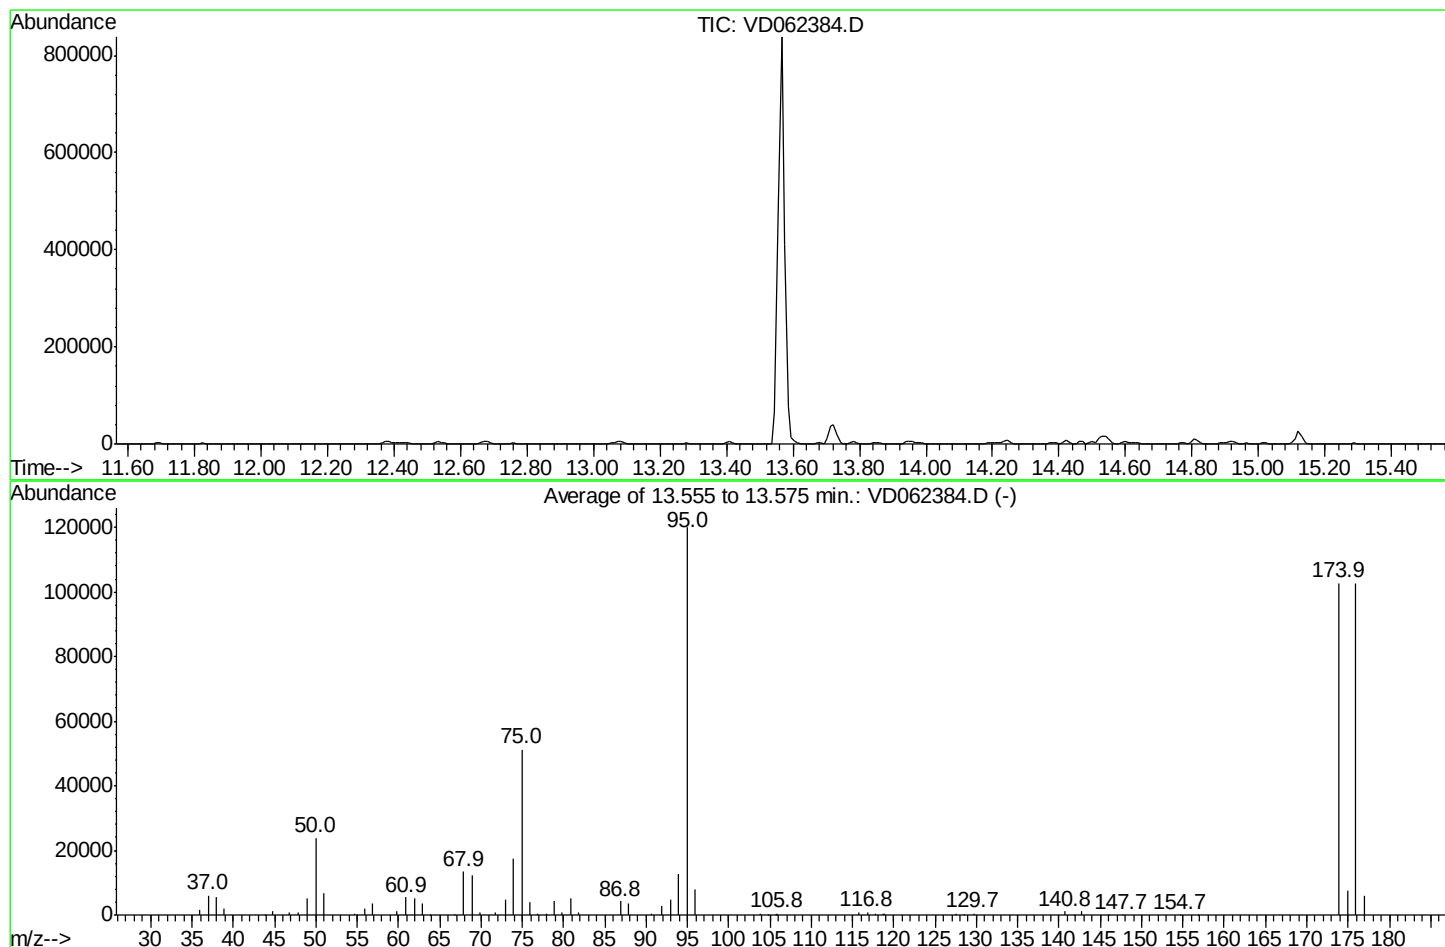

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	23803	PASS
75	95	30	60	42.7	51213	PASS
95	95	100	100	100.0	119984	PASS
96	95	5	9	6.6	7908	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.6	102712	PASS
175	174	5	9	7.3	7482	PASS
176	174	95	101	99.8	102514	PASS
177	176	5	9	5.8	5917	PASS