


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD051619\
Data File : VD062409.D
Acq On : 16 May 2019 9:33
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D050719S.M
Title : SW846 8260
Last Update : Tue May 07 14:26:29 2019

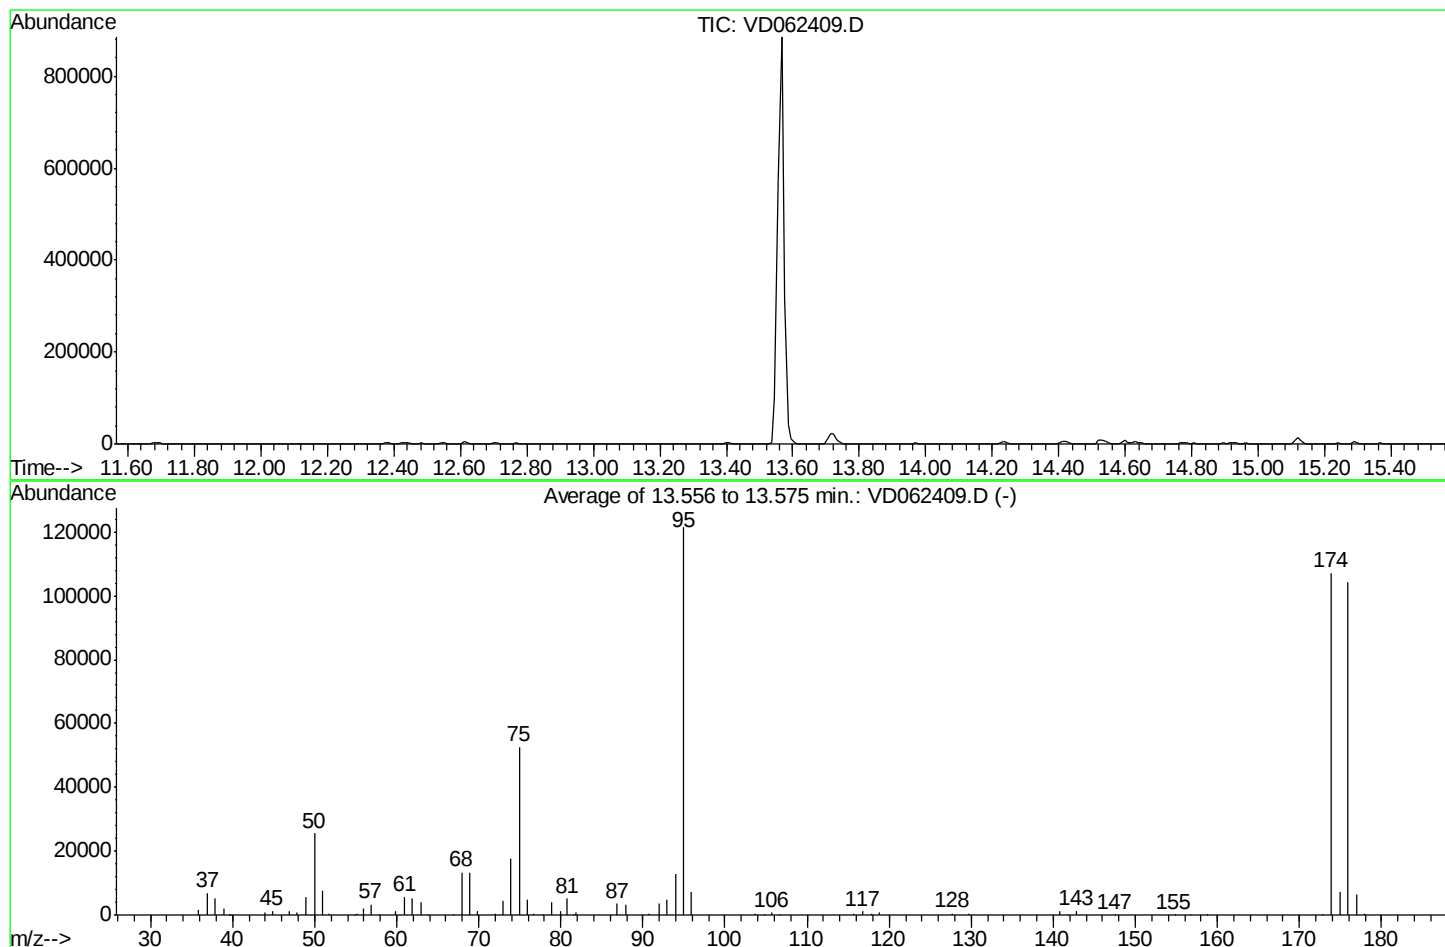

AutoFind: Scans 1233, 1234, 1235; Background Corrected with Scan 1228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	25554	PASS
75	95	30	60	43.3	52608	PASS
95	95	100	100	100.0	121445	PASS
96	95	5	9	5.9	7162	PASS
173	174	0.00	2	0.1	158	PASS
174	95	50	100	88.2	107144	PASS
175	174	5	9	6.8	7279	PASS
176	174	95	101	97.4	104330	PASS
177	176	5	9	6.1	6403	PASS