

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051823\
 Data File : VD076146.D
 Acq On : 18 May 2023 17:59
 Operator : KP/SY
 Sample : 02816-08
 Misc : 5.73G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CB-22-K2-SO-39-051623

Quant Time: May 19 01:54:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 10:08:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	133140	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	249498	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	247998	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	113592	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	100564	78.153	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	156.300%
35) Dibromofluoromethane	7.805	113	119344	69.202	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	138.400%
50) Toluene-d8	10.269	98	359547	53.481	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	106.960%
62) 4-Bromofluorobenzene	12.575	95	109827	58.809	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	117.620%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051823\
Data File : VD076146.D
Acq On : 18 May 2023 17:59
Operator : KP/SY
Sample : 02816-08
Misc : 5.73G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CB-22-K2-SO-39-051623

Quant Time: May 19 01:54:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Quant Title : SW846 8260
QLast Update : Tue May 16 10:08:53 2023
Response via : Initial Calibration




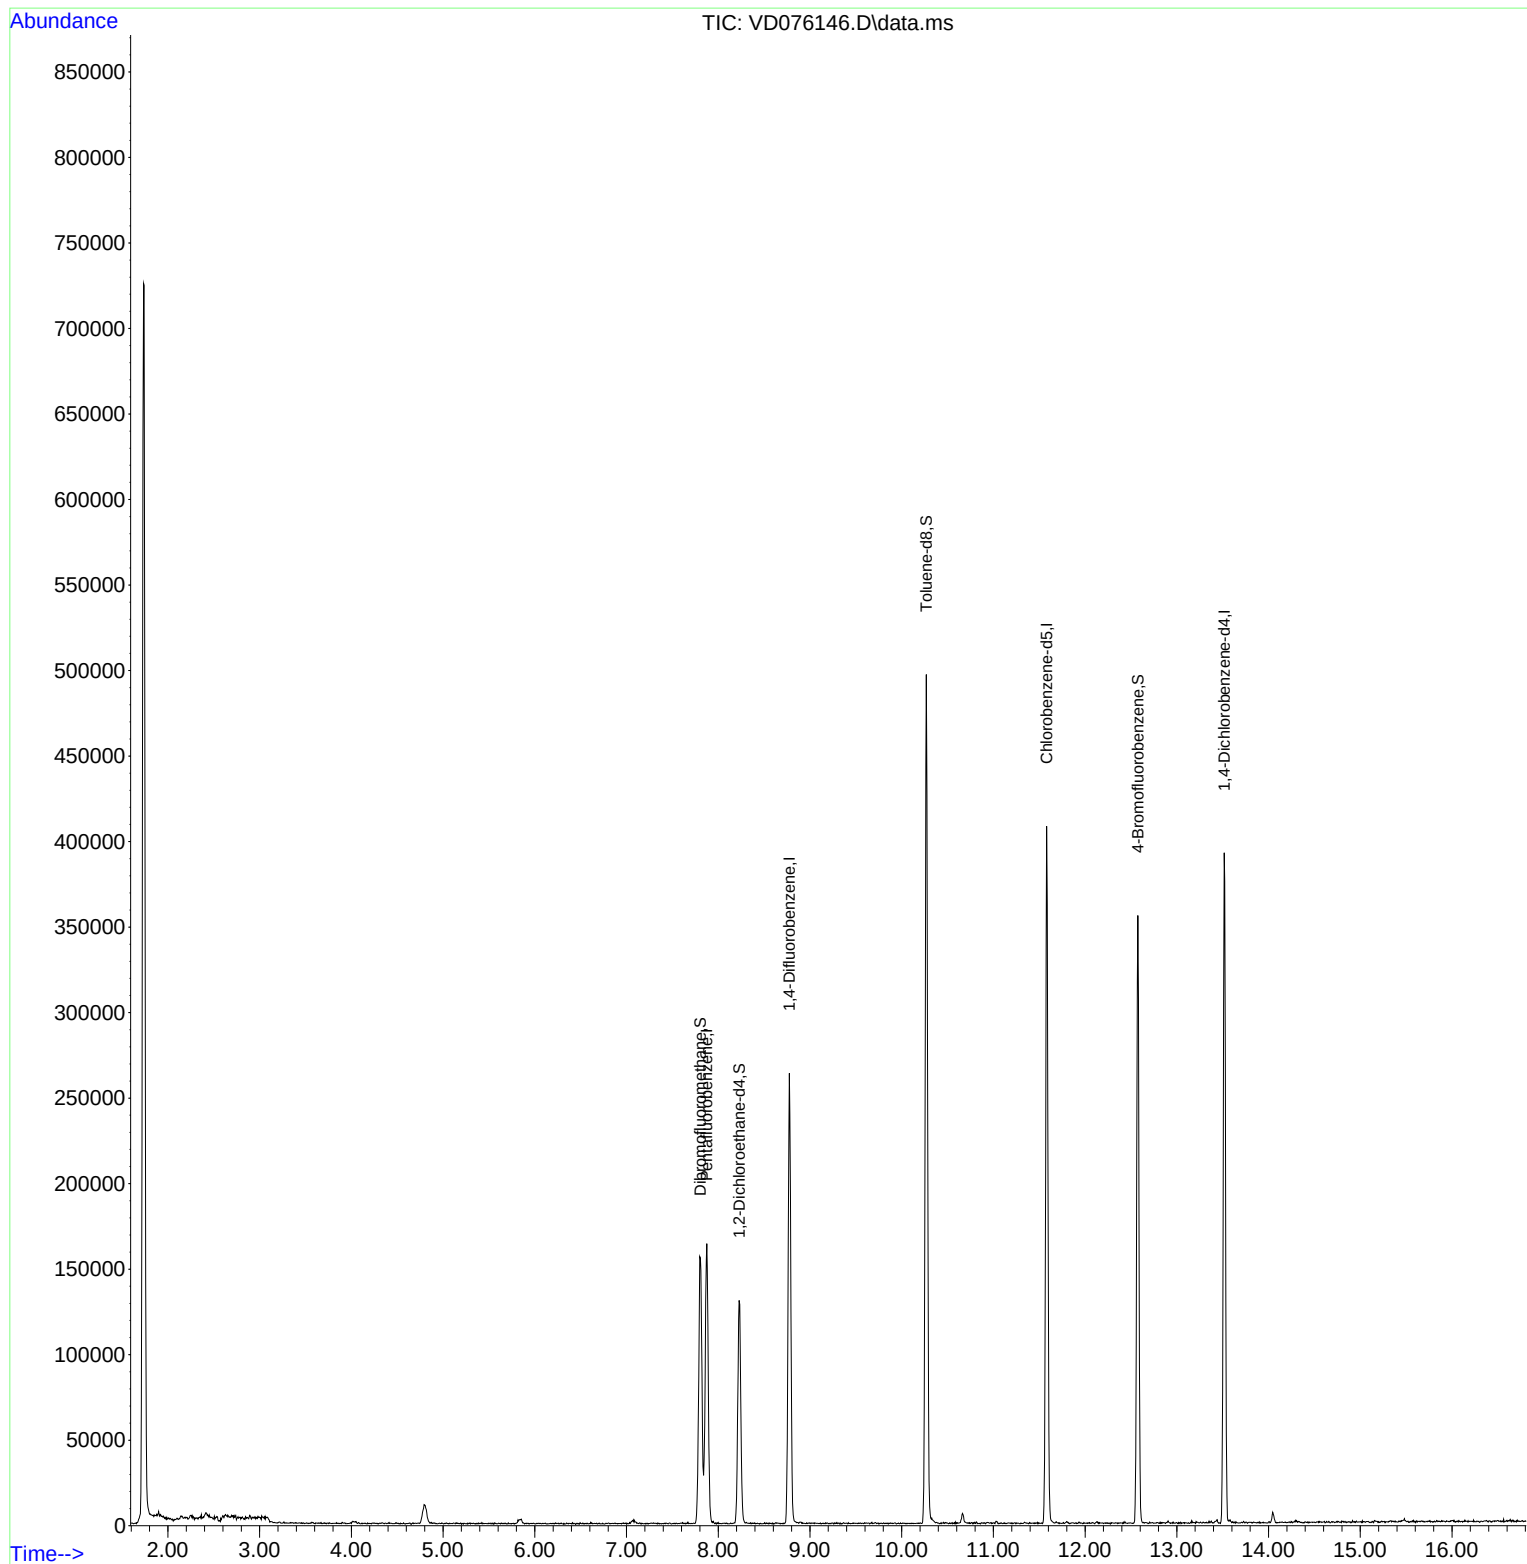


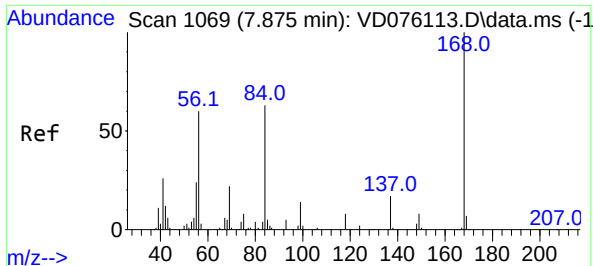

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59




Instrument :
MSVOA_D
ClientSampleId :
CB-22-K2-SO-39-051623


Tgt Ion:168 Resp: 133140
Ion Ratio Lower Upper
168 100
99 48.8 43.8 65.6

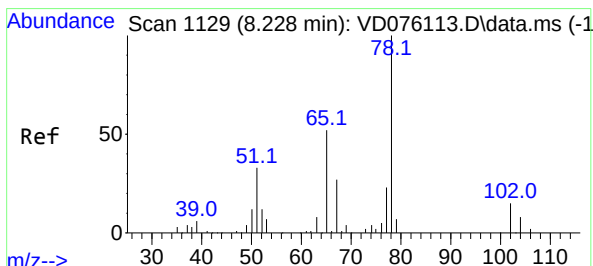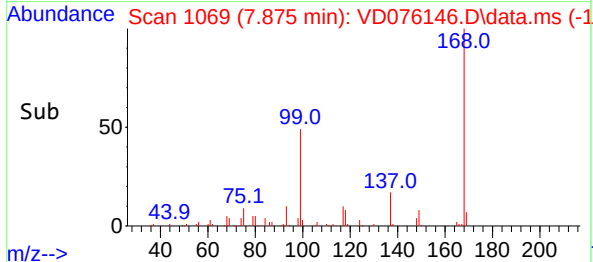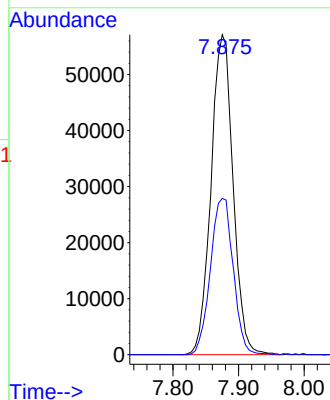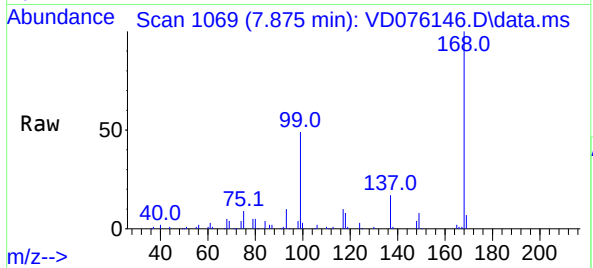

#33
1,2-Dichloroethane-d4
Concen: 78.153 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59

Tgt Ion: 65 Resp: 100564
Ion Ratio Lower Upper
65 100
67 55.7 0.0 102.2

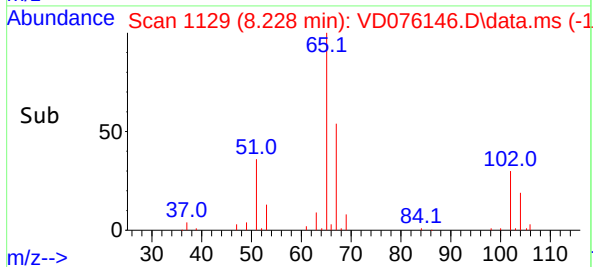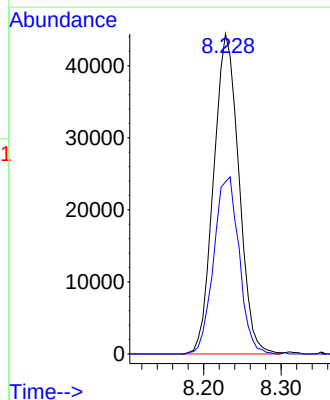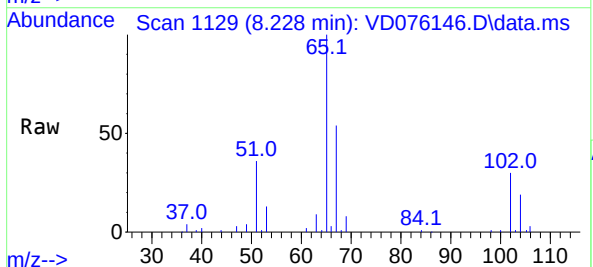

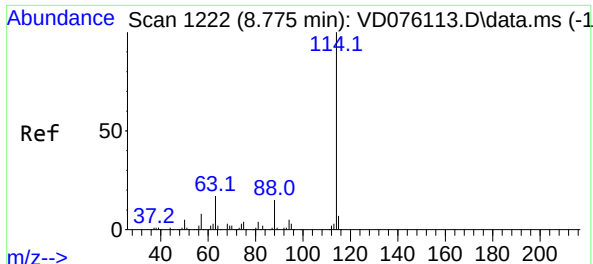

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. 0.000 min

Lab File: VD076146.D

Acq: 18 May 2023 17:59

Instrument :

MSVOA_D

ClientSampleId :

CB-22-K2-SO-39-051623





Tgt Ion:114 Resp: 249498

Ion Ratio Lower Upper

114 100

63 15.8 0.0 41.6

88 13.3 0.0 30.6

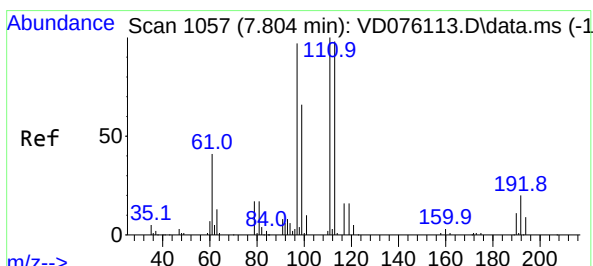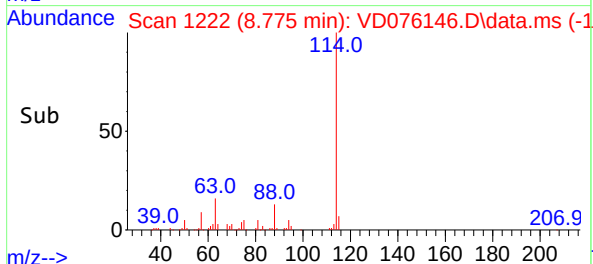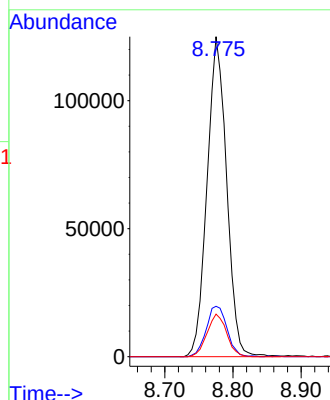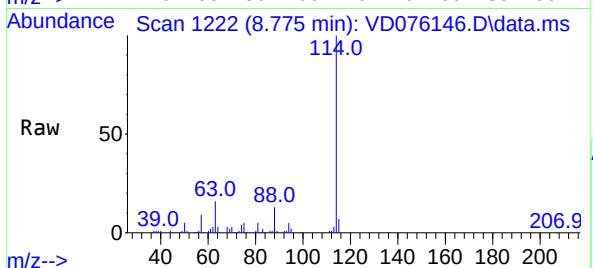

#35

Dibromofluoromethane

Concen: 69.202 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076146.D

Acq: 18 May 2023 17:59




Tgt Ion:113 Resp: 119344


Ion Ratio Lower Upper

113 100

111 101.5 81.4 122.0

192 18.8 15.2 22.8


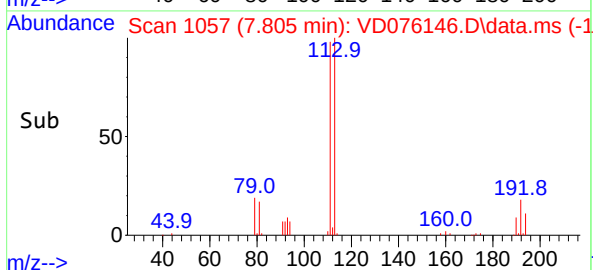
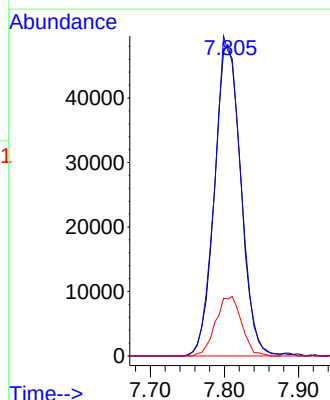
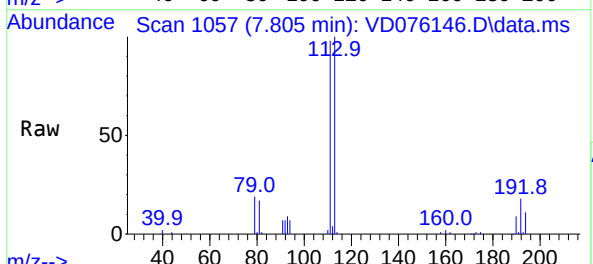


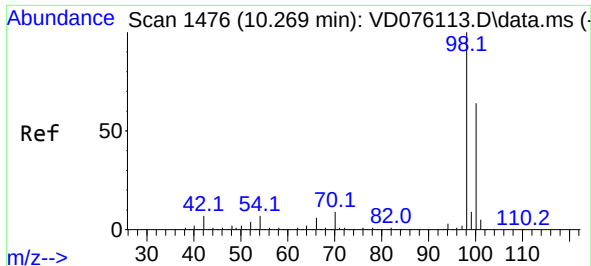

#50
Toluene-d8
Concen: 53.481 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59




Instrument :
MSVOA_D
ClientSampleId :
CB-22-K2-SO-39-051623


Tgt Ion: 98 Resp: 359547
Ion Ratio Lower Upper
98 100
100 62.9 52.1 78.1

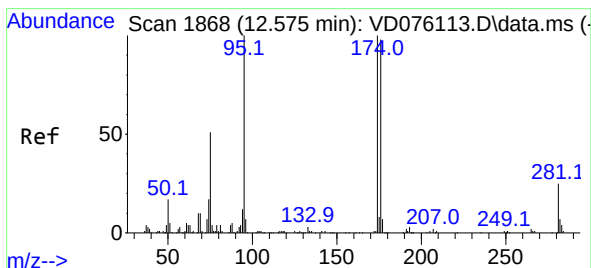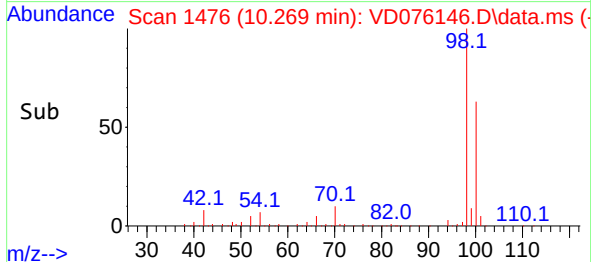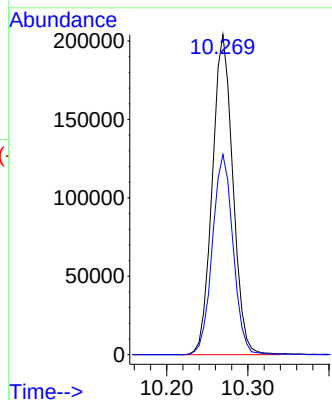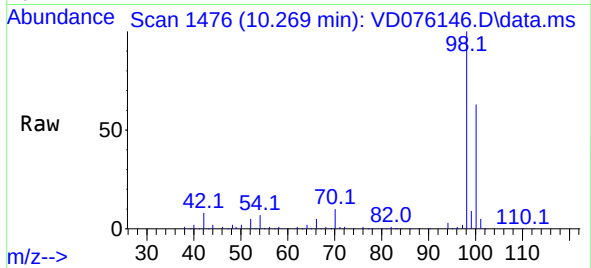

#62
4-Bromofluorobenzene
Concen: 58.809 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59

Tgt Ion: 95 Resp: 109827
Ion Ratio Lower Upper
95 100
174 91.4 0.0 164.0
176 88.6 0.0 156.8


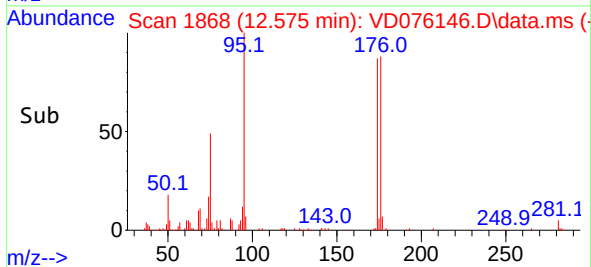
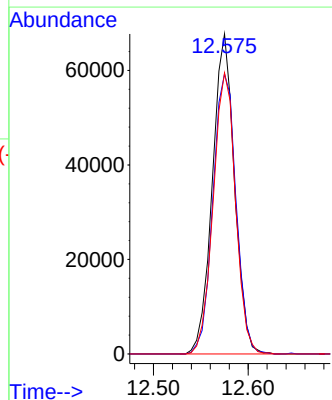
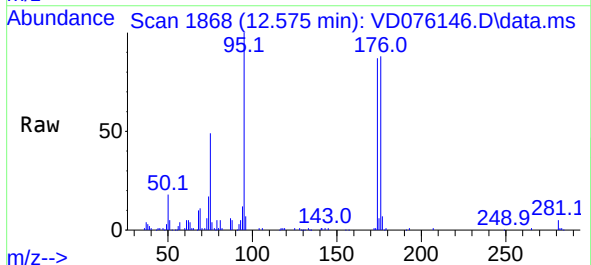


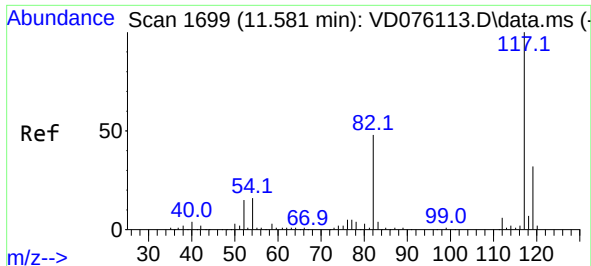

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59

Instrument :
MSVOA_D
ClientSampleId :
CB-22-K2-SO-39-051623

Tgt Ion:117 Resp: 247998
Ion Ratio Lower Upper
117 100
82 51.8 44.0 66.0
119 32.5 25.1 37.7

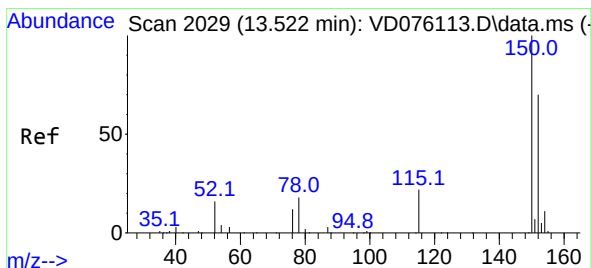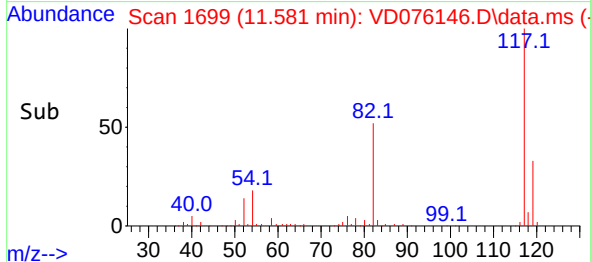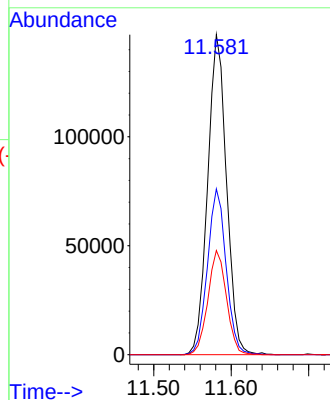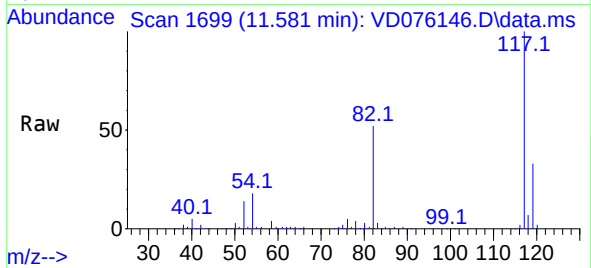

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076146.D
Acq: 18 May 2023 17:59

Tgt Ion:152 Resp: 113592
Ion Ratio Lower Upper
152 100
115 54.4 30.1 90.3
150 157.5 0.0 364.8

