

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051923\
 Data File : VD076154.D
 Acq On : 19 May 2023 13:33
 Operator : KP/SY
 Sample : 02811-01RE
 Misc : 5.07G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 72-11995RE

Quant Time: May 19 15:18:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 10:08:53 2023
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	142340	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	293773	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	289920	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	112695	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	126177	91.720	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 183.440%#	
35) Dibromofluoromethane	7.804	113	146662	72.226	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 144.460%	
50) Toluene-d8	10.269	98	410239	51.825	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 103.640%	
62) 4-Bromofluorobenzene	12.575	95	118441	53.863	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 107.720%	
Target Compounds						
3) Chloromethane	2.140	50	253	Below Cal	#	40
16) Acetone	4.016	43	1158	4.231	ug/l #	44
20) Methylene Chloride	4.805	84	9815	Below Cal	#	62
31) Cyclohexane	7.875	56	3197	1.517	ug/l #	39
36) 1,1-Dichloropropene	7.875	75	10707	3.904	ug/l #	51
38) Carbon Tetrachloride	7.869	117	13836	5.585	ug/l #	16
51) 4-Methyl-2-Pentanone	10.269	43	1373	1.455	ug/l #	1
76) 1,2,3-Trichloropropane	12.575	75	59192	60.022	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.575	75	59192	125.916	ug/l #	5

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 19 15:18:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Quant Title : SW846 8260
QLast Update : Tue May 16 10:08:53 2023
Response via : Initial Calibration






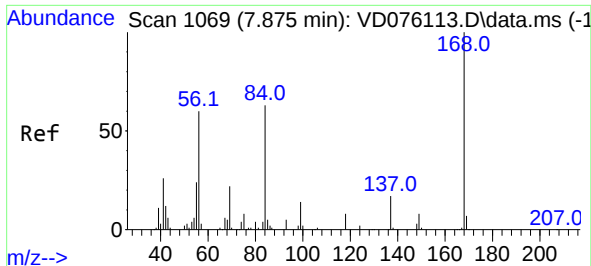

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33




Instrument :
MSVOA_D
ClientSampleId :
72-11995RE

Tgt Ion:168 Resp: 142340
Ion Ratio Lower Upper
168 100
99 53.3 43.8 65.6

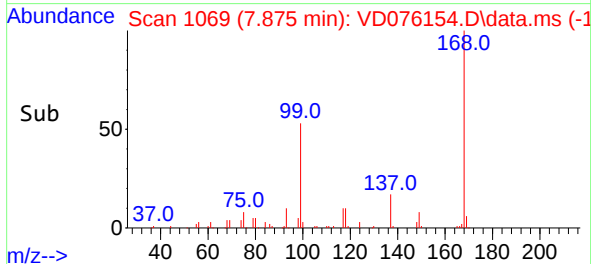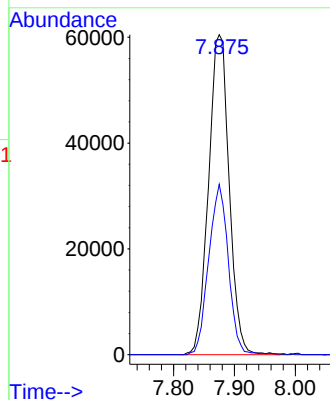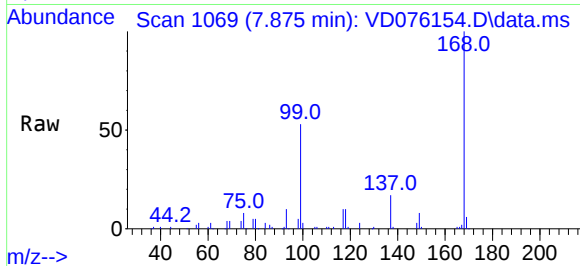

#3
Chloromethane
Concen: Below Cal
RT: 2.140 min Scan# 94
Delta R.T. -0.006 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 50 Resp: 253
Ion Ratio Lower Upper
50 100
52 0.0 27.8 41.8#


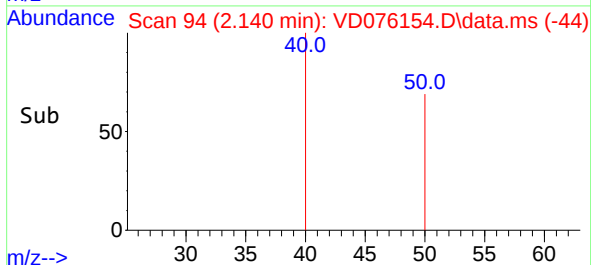
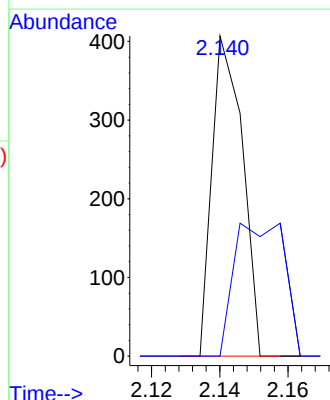
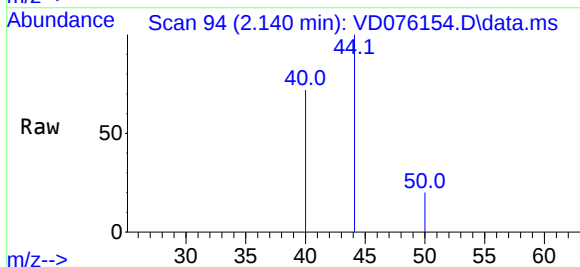




#16
Acetone
Concen: 4.231 ug/l
RT: 4.016 min Scan# 41
Delta R.T. -0.006 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33




Instrument :
MSVOA_D
ClientSampleId :
72-11995RE


Tgt Ion: 43 Resp: 1158
Ion Ratio Lower Upper
43 100
58 0.0 24.4 36.6#

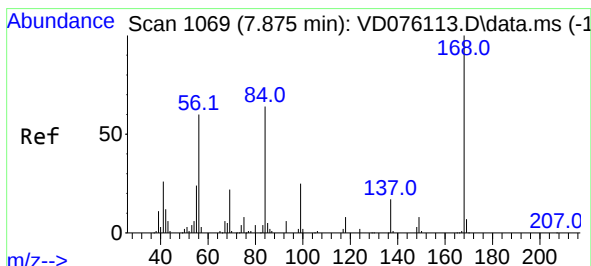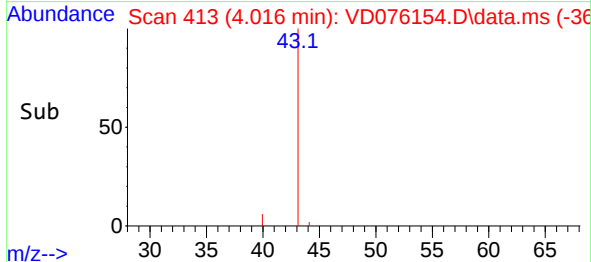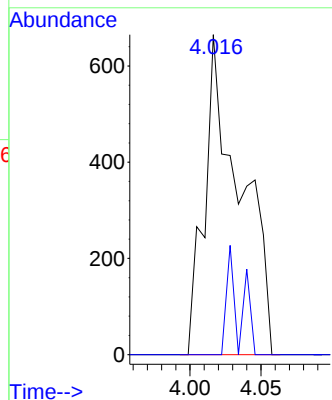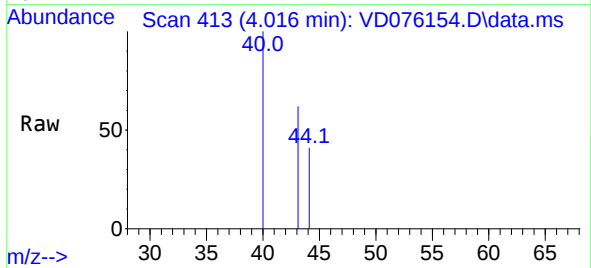

#31
Cyclohexane
Concen: 1.517 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 56 Resp: 3197
Ion Ratio Lower Upper
56 100
69 120.3 25.5 38.3#
84 110.1 69.6 104.4#


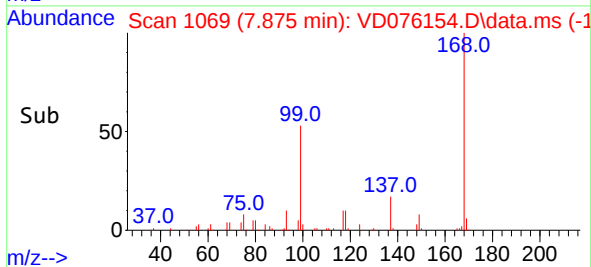
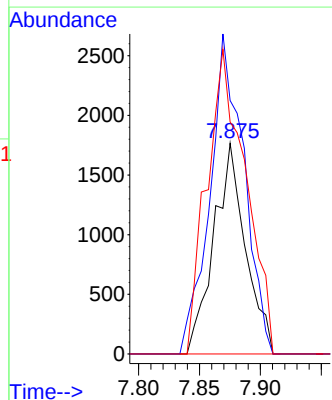
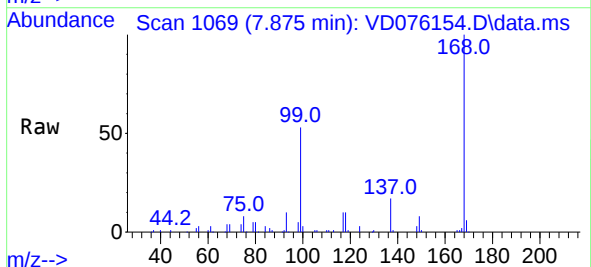


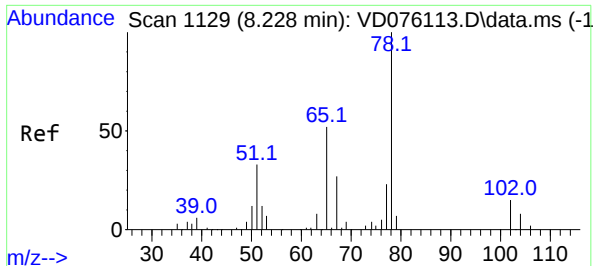

#33
1,2-Dichloroethane-d4
Concen: 91.720 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33




Instrument :
MSVOA_D
ClientSampleId :
72-11995RE


Tgt Ion: 65 Resp: 126177
Ion Ratio Lower Upper
65 100
67 56.0 0.0 102.2

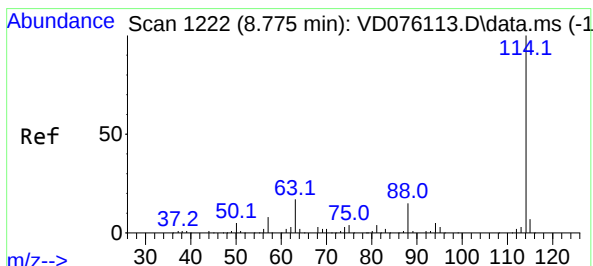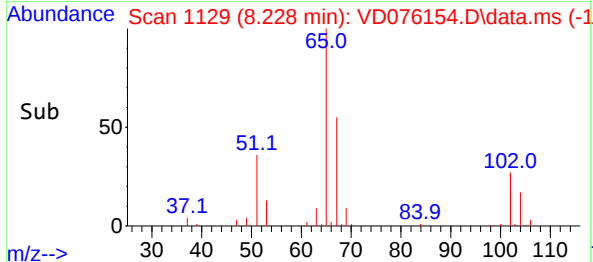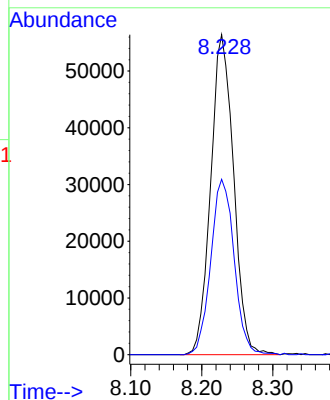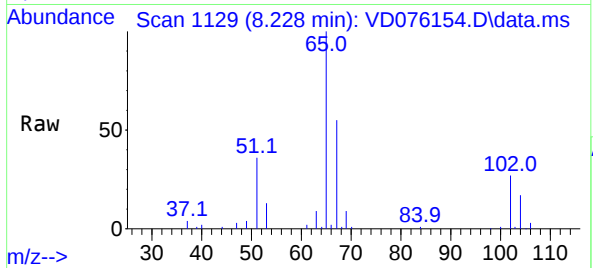

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.775 min Scan# 1222
Delta R.T. 0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 114 Resp: 293773
Ion Ratio Lower Upper
114 100
63 16.7 0.0 41.6
88 13.9 0.0 30.6

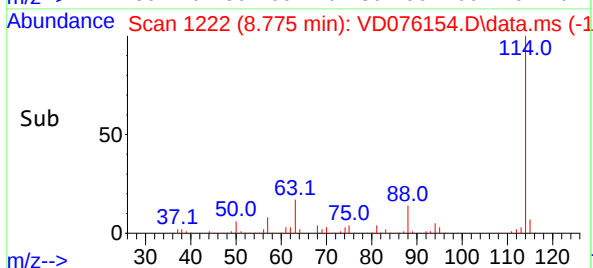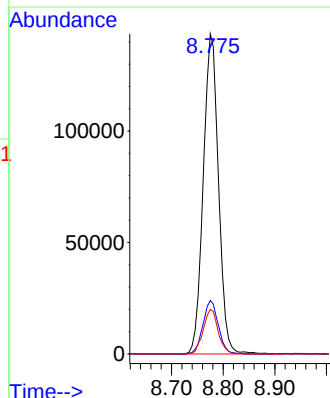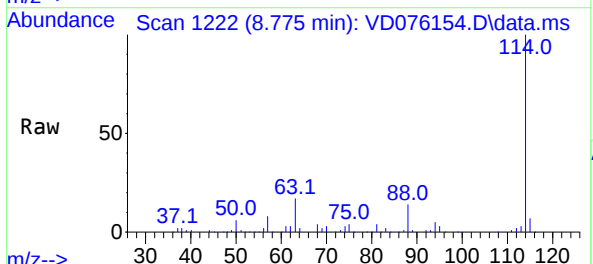

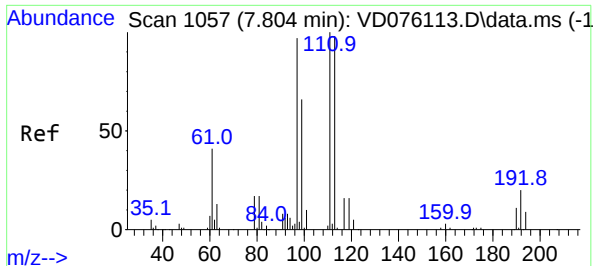

#35

Dibromofluoromethane

Concen: 72.226 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD076154.D

Acq: 19 May 2023 13:33

Instrument :

MSVOA_D

ClientSampleId :

72-11995RE





Tgt Ion:113 Resp: 146662

Ion Ratio Lower Upper

113 100

111 103.3 81.4 122.0

192 18.7 15.2 22.8

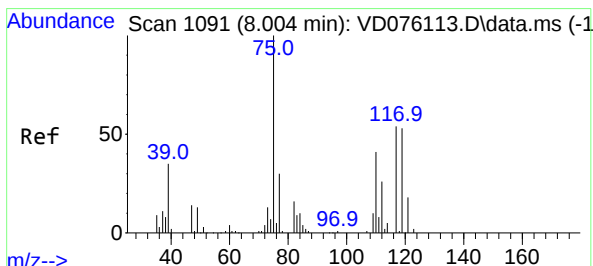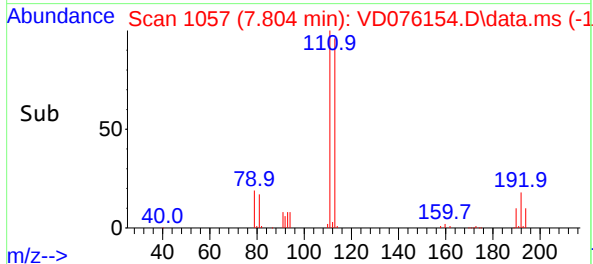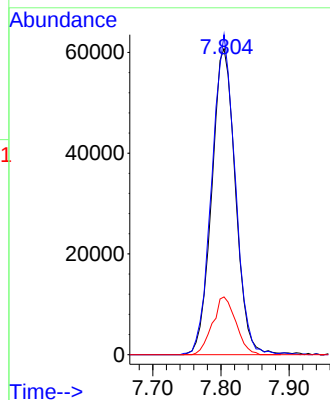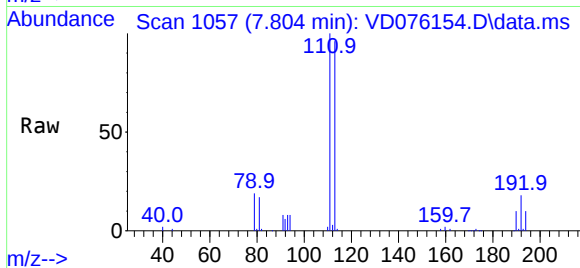

#36

1,1-Dichloropropene

Concen: 3.904 ug/l

RT: 7.875 min Scan# 1069

Delta R.T. -0.135 min

Lab File: VD076154.D

Acq: 19 May 2023 13:33




Tgt Ion: 75 Resp: 10707


Ion Ratio Lower Upper

75 100

110 10.1 17.1 51.2#


77 0.0 24.6 36.8#

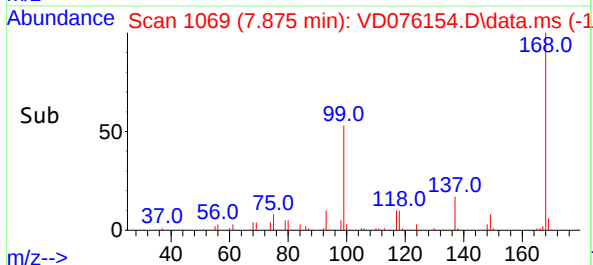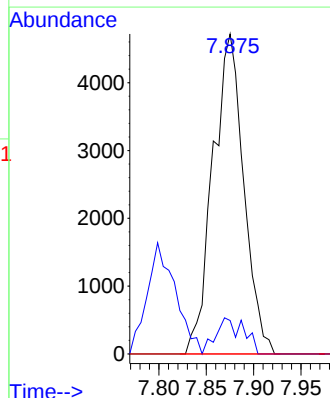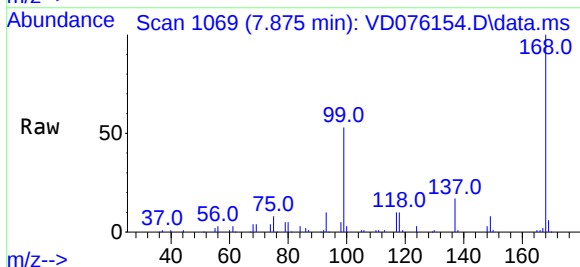



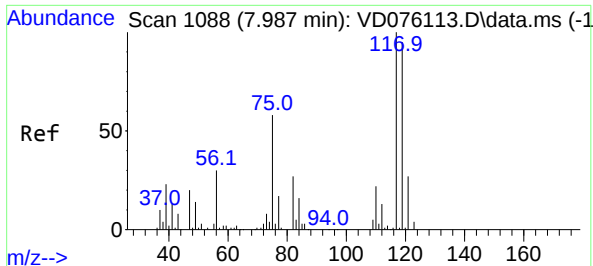


#38
Carbon Tetrachloride
Concen: 5.585 ug/l
RT: 7.869 min Scan# 1068
Delta R.T. -0.124 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Instrument :
MSVOA_D
ClientSampleId :
72-11995RE



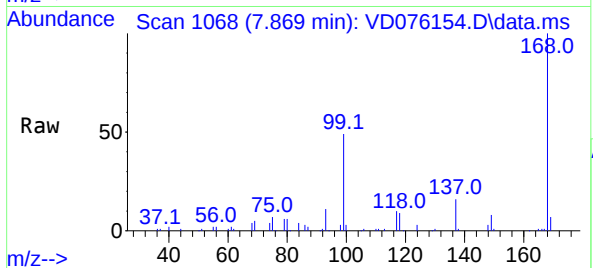



Tgt Ion:117 Resp: 13836
Ion Ratio Lower Upper
117 100
119 4.2 74.7 112.1#
121 0.0 25.9 38.9#

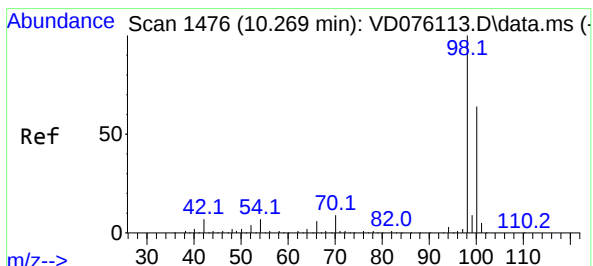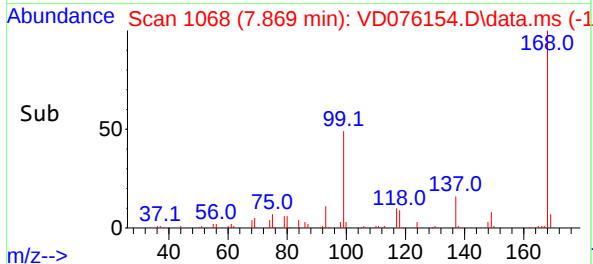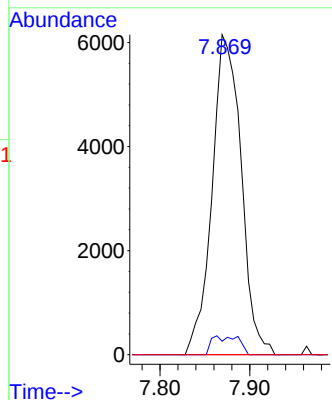

#50
Toluene-d8
Concen: 51.825 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 98 Resp: 410239
Ion Ratio Lower Upper
98 100
100 62.5 52.1 78.1


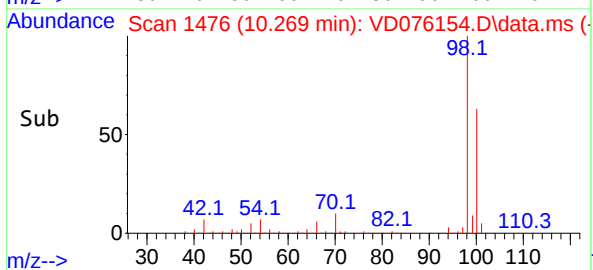
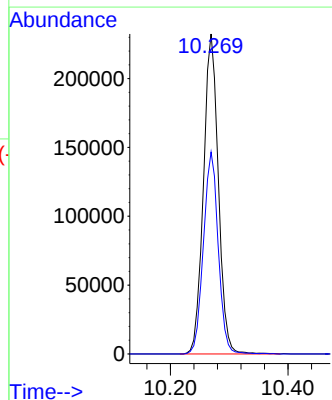
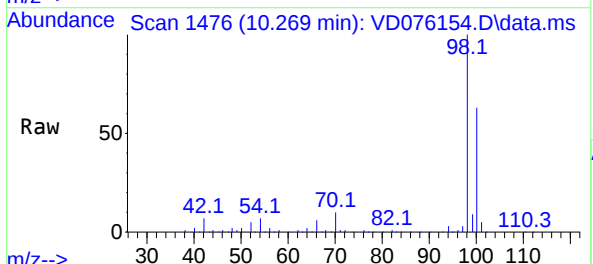


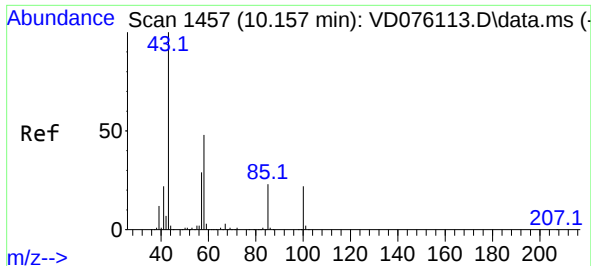

#51
4-Methyl-2-Pentanone
Concen: 1.455 ug/l
RT: 10.269 min Scan# 1457
Delta R.T. 0.112 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33




Instrument :
MSVOA_D
ClientSampleId :
72-11995RE


Tgt Ion: 43 Resp: 1373
Ion Ratio Lower Upper
43 100
58 180.7 29.5 44.3#

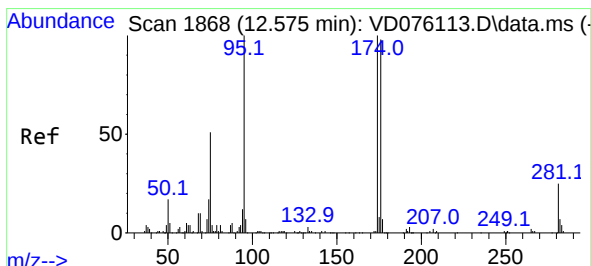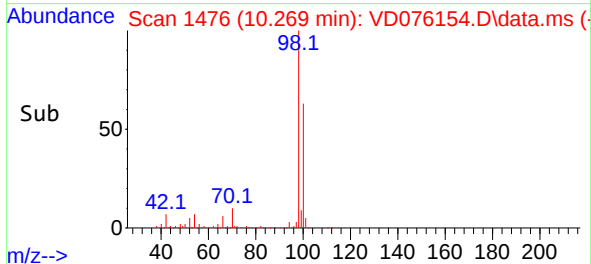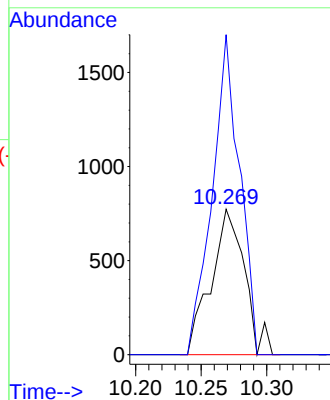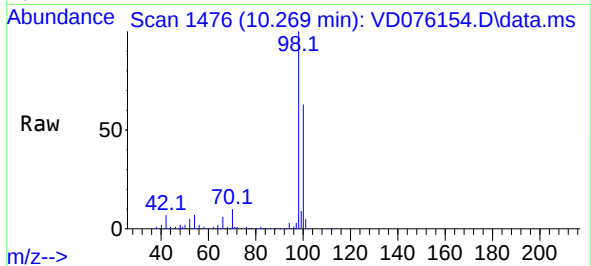

#62
4-Bromofluorobenzene
Concen: 53.863 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 95 Resp: 118441
Ion Ratio Lower Upper
95 100
174 91.7 0.0 164.0
176 87.1 0.0 156.8


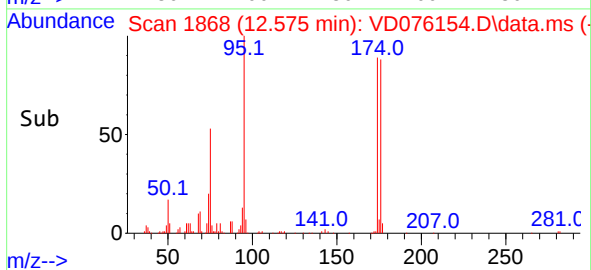
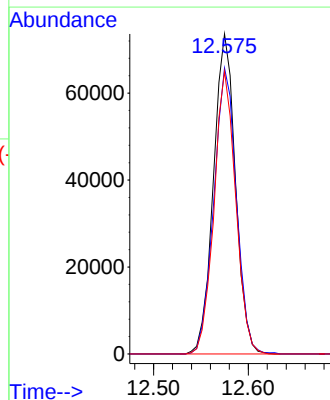
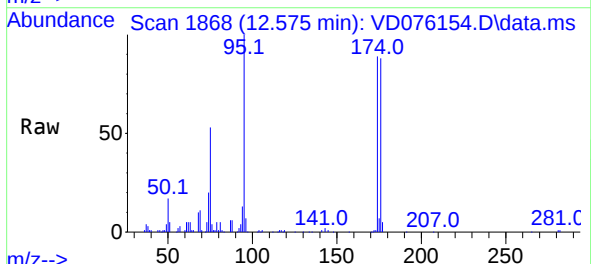


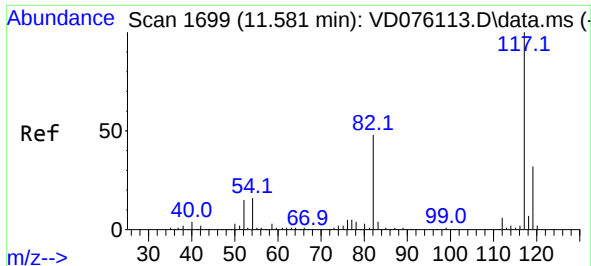

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33




Instrument :
MSVOA_D
ClientSampleId :
72-11995RE


Tgt Ion:117 Resp: 289920
Ion Ratio Lower Upper
117 100
82 50.3 44.0 66.0
119 32.0 25.1 37.7

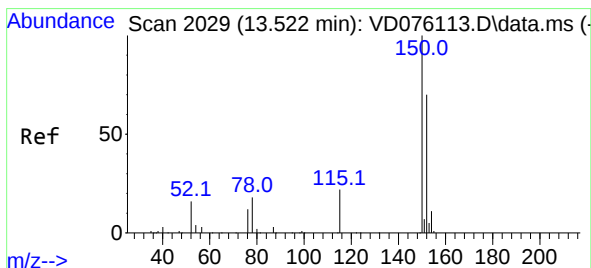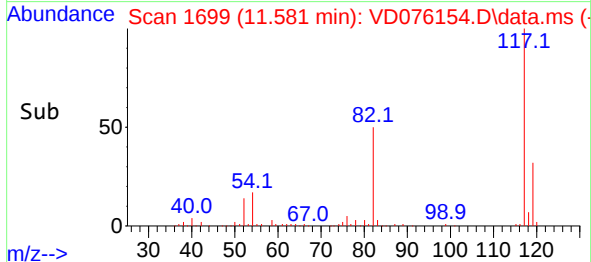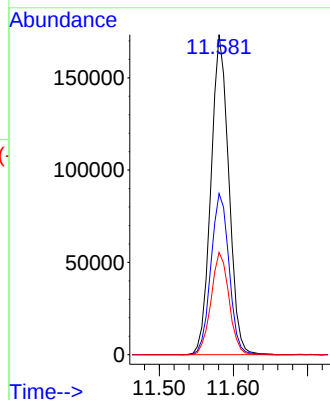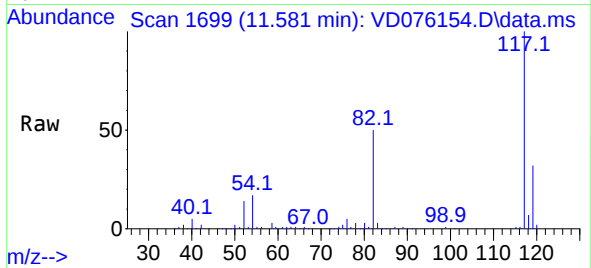

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion:152 Resp: 112695
Ion Ratio Lower Upper
152 100
115 54.7 30.1 90.3
150 155.6 0.0 364.8


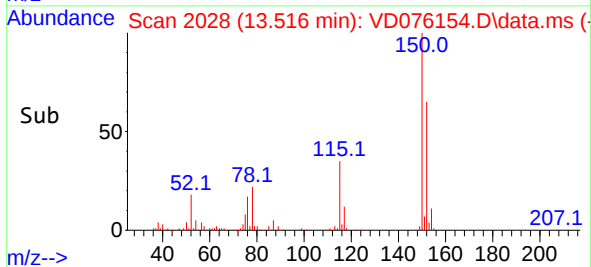
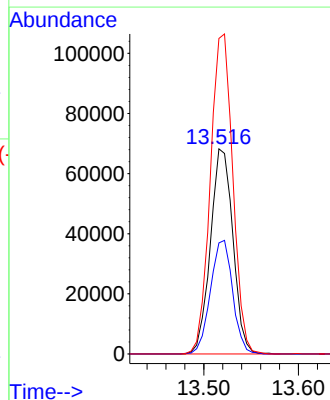
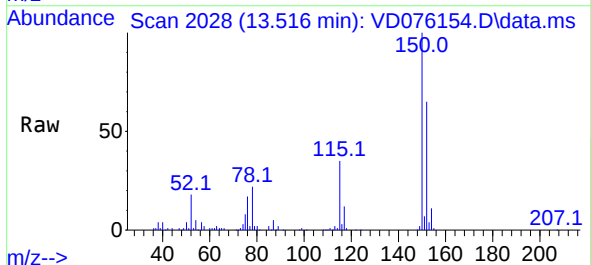


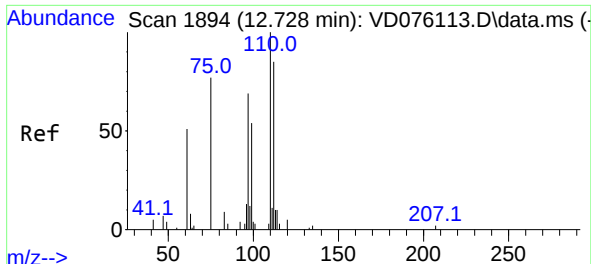

#76
1,2,3-Trichloropropane
Concen: 60.022 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.153 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Instrument :
MSVOA_D
ClientSampleId :
72-11995RE

Tgt Ion: 75 Resp: 59192
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

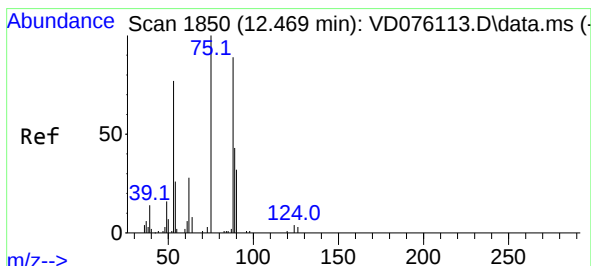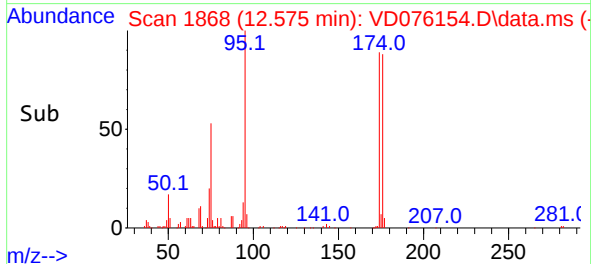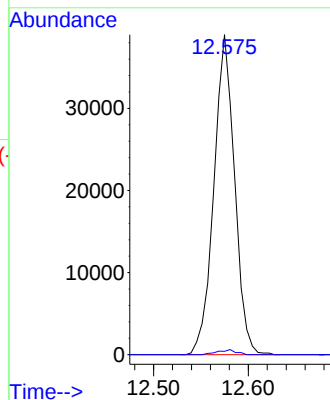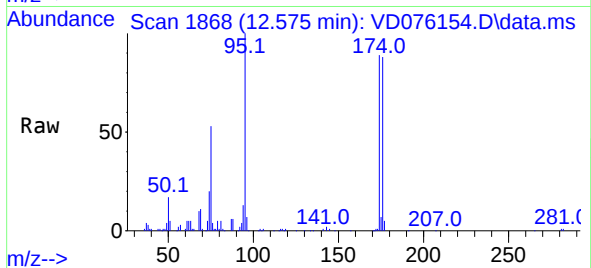

#81
trans-1,4-Dichloro-2-butene
Concen: 125.916 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.100 min
Lab File: VD076154.D
Acq: 19 May 2023 13:33

Tgt Ion: 75 Resp: 59192
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 40.2 60.4#

