

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051923\
 Data File : VD076165.D
 Acq On : 19 May 2023 19:39
 Operator : KP/SY
 Sample : 02849-31
 Misc : 4.92G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP10

Quant Time: May 22 01:31:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 10:08:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	6576	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	13490	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	14347	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	5338	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	7486	117.787	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	235.580%#
35) Dibromofluoromethane	7.799	113	6729	72.165	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	144.320%
50) Toluene-d8	10.269	98	12770	35.131	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	70.260%
62) 4-Bromofluorobenzene	12.575	95	4789	47.428	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	94.860%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051923\
Data File : VD076165.D
Acq On : 19 May 2023 19:39
Operator : KP/SY
Sample : 02849-31
Misc : 4.92G/5.00ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP10

Quant Time: May 22 01:31:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Quant Title : SW846 8260
QLast Update : Tue May 16 10:08:53 2023
Response via : Initial Calibration




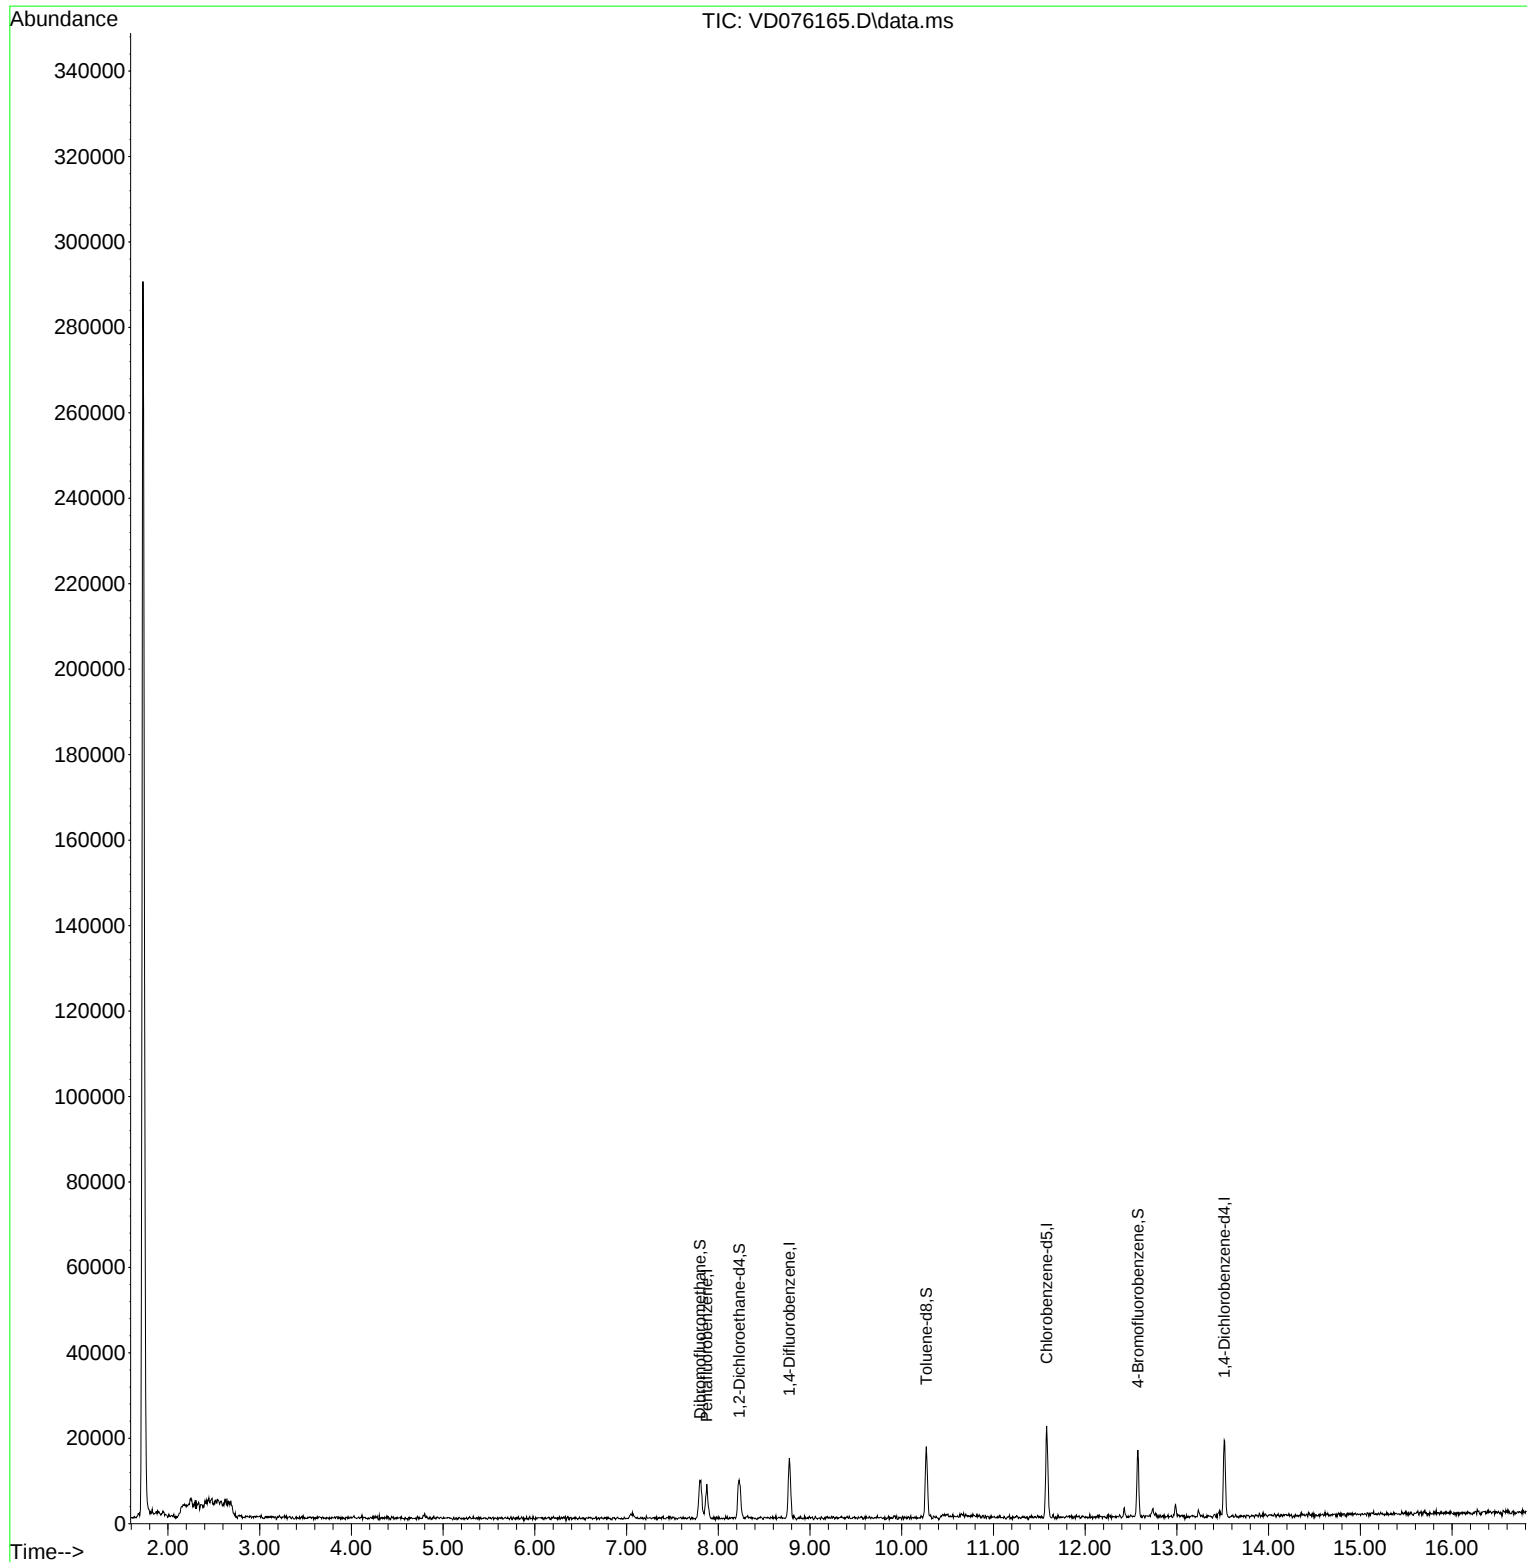


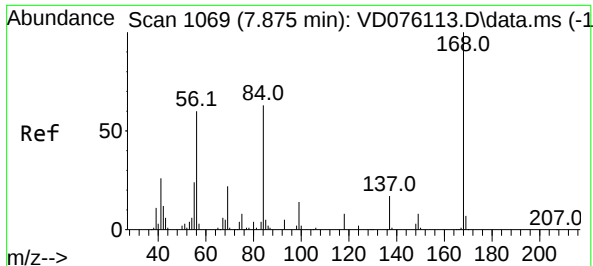

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39




Instrument :
MSVOA_D
ClientSampleId :
TP10


Tgt Ion:168 Resp: 6576
Ion Ratio Lower Upper
168 100
99 46.7 43.8 65.6

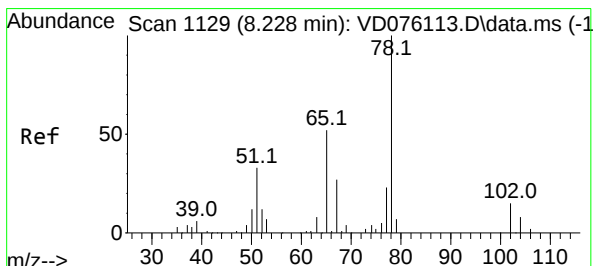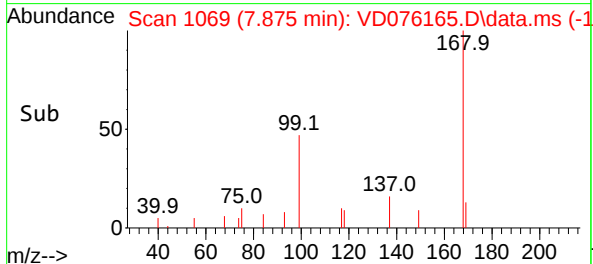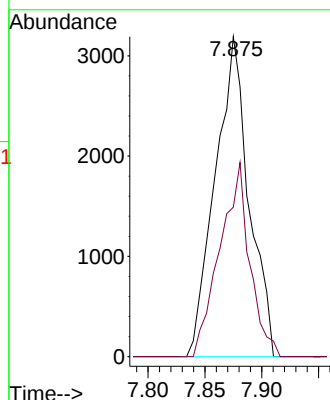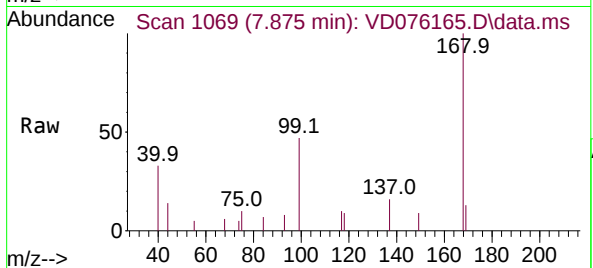

#33
1,2-Dichloroethane-d4
Concen: 117.787 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.006 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39

Tgt Ion: 65 Resp: 7486
Ion Ratio Lower Upper
65 100
67 60.5 0.0 102.2

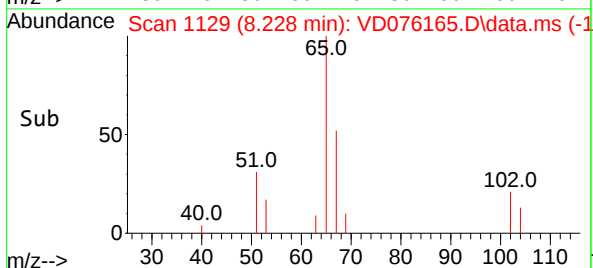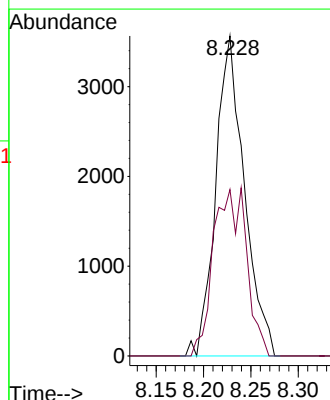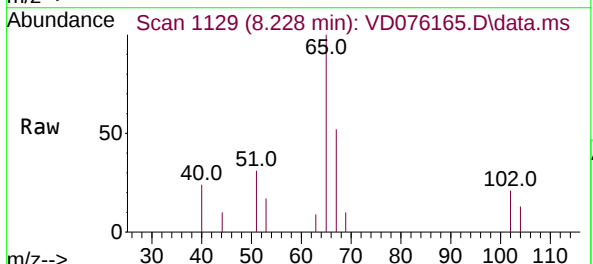

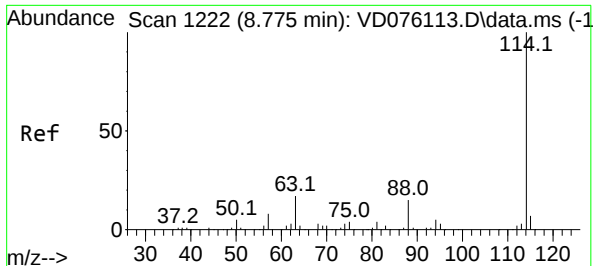

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD076165.D

Acq: 19 May 2023 19:39

Instrument :

MSVOA_D

ClientSampleId :

TP10





Tgt Ion:114 Resp: 13490

Ion Ratio Lower Upper

114 100

63 15.5 0.0 41.6

88 19.0 0.0 30.6

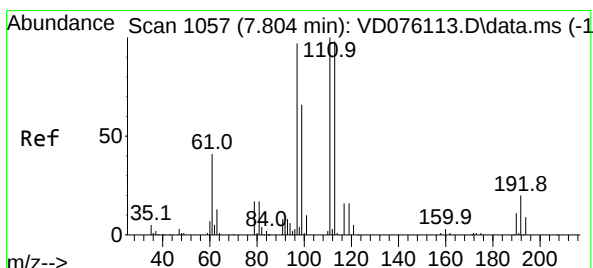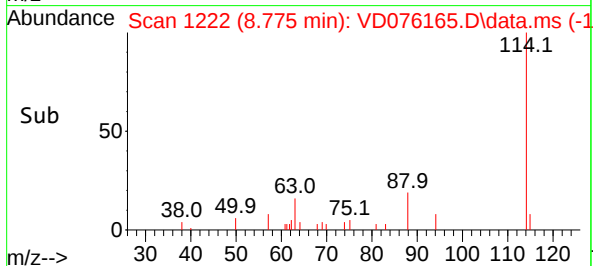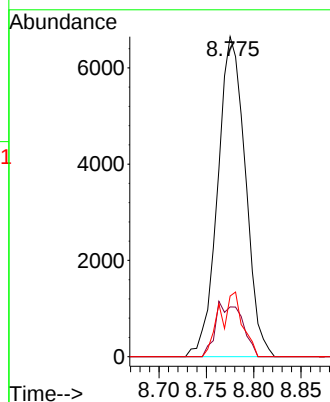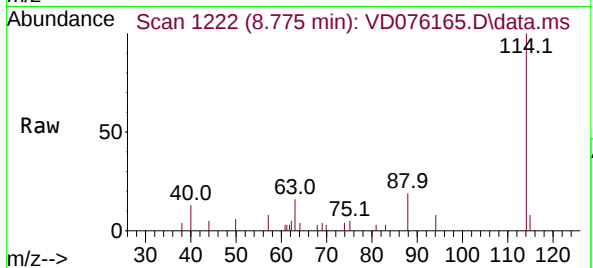

#35

Dibromofluoromethane

Concen: 72.165 ug/l

RT: 7.799 min Scan# 1056

Delta R.T. -0.006 min

Lab File: VD076165.D

Acq: 19 May 2023 19:39




Tgt Ion:113 Resp: 6729


Ion Ratio Lower Upper

113 100

111 109.7 81.4 122.0

192 19.0 15.2 22.8


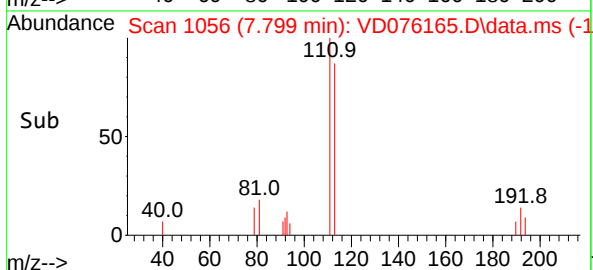
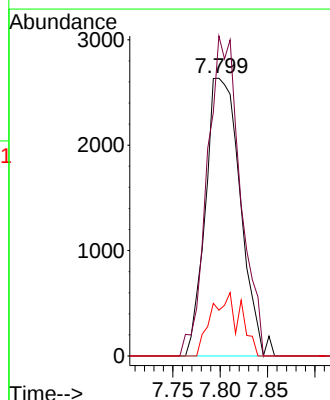
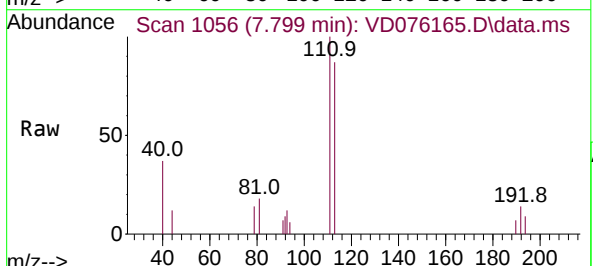


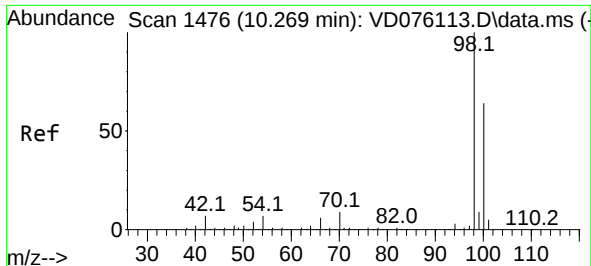

#50
Toluene-d8
Concen: 35.131 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39




Instrument :
MSVOA_D
ClientSampleId :
TP10


Tgt Ion: 98 Resp: 12770
Ion Ratio Lower Upper
98 100
100 57.1 52.1 78.1

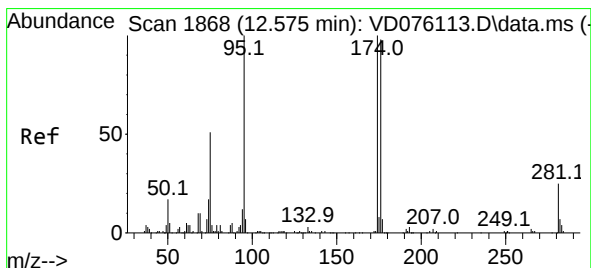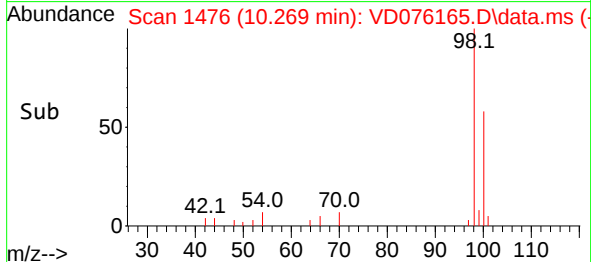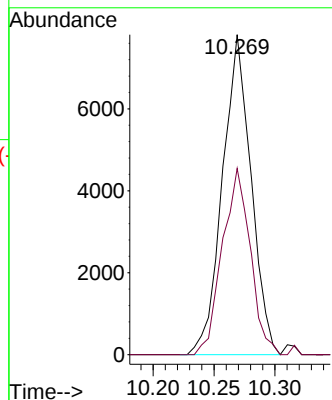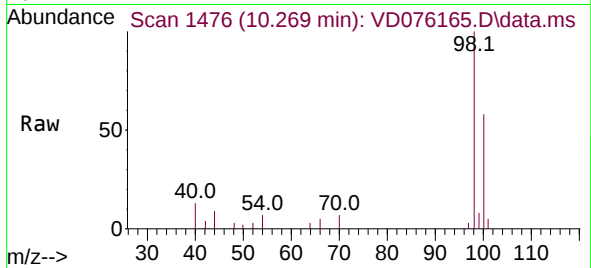

#62
4-Bromofluorobenzene
Concen: 47.428 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39

Tgt Ion: 95 Resp: 4789
Ion Ratio Lower Upper
95 100
174 101.2 0.0 164.0
176 88.7 0.0 156.8


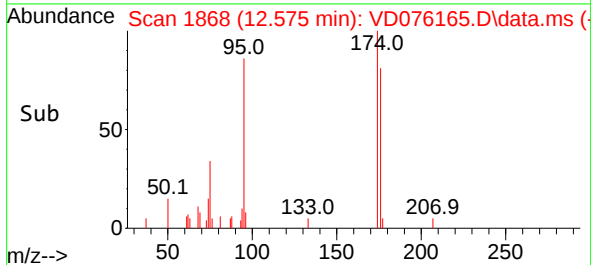
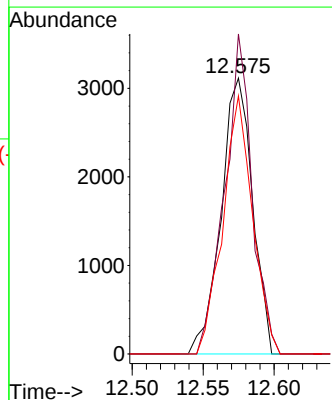
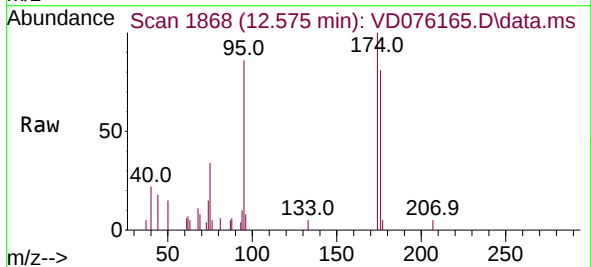


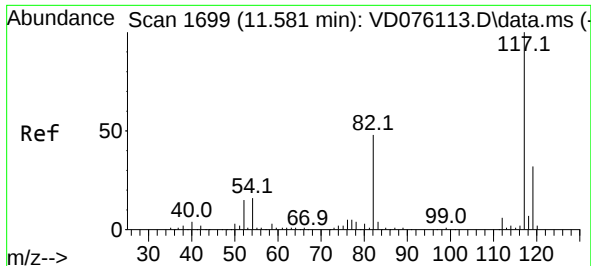

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39

Instrument :
MSVOA_D
ClientSampleId :
TP10

Tgt Ion:117 Resp: 14347
Ion Ratio Lower Upper
117 100
82 47.8 44.0 66.0
119 34.8 25.1 37.7

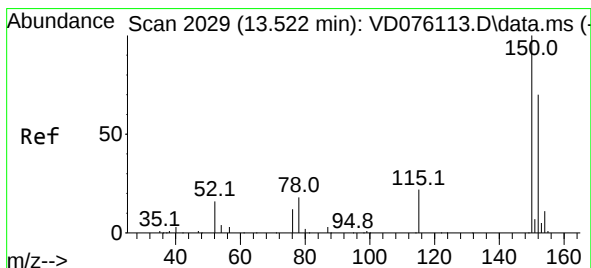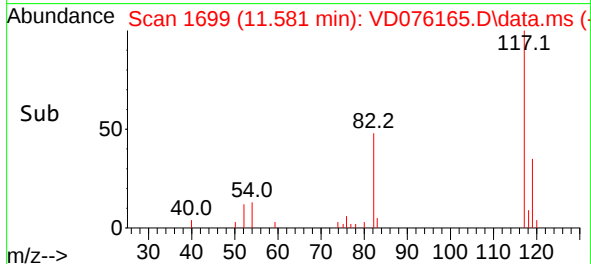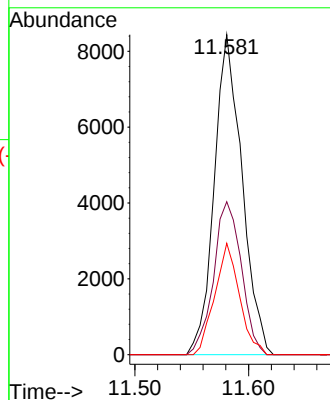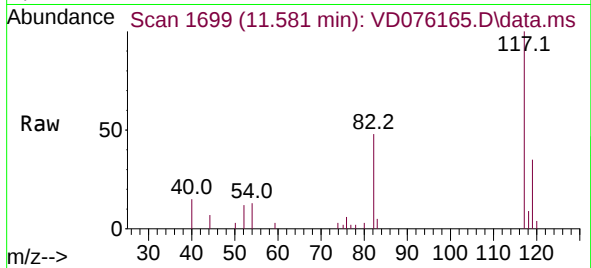

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.006 min
Lab File: VD076165.D
Acq: 19 May 2023 19:39

Tgt Ion:152 Resp: 5338
Ion Ratio Lower Upper
152 100
115 53.7 30.1 90.3
150 162.9 0.0 364.8

