

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052423\
 Data File : VD076208.D
 Acq On : 24 May 2023 12:13
 Operator : KP/SY
 Sample : VD0524SBL01
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0524SBL01

Quant Time: May 24 16:24:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 10:08:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.881	168	154952	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	300897	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	273236	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	117508	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.234	65	88682	59.217	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	118.440%
35) Dibromofluoromethane	7.804	113	102659	49.359	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.720%
50) Toluene-d8	10.269	98	353533	43.604	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	87.200%
62) 4-Bromofluorobenzene	12.575	95	91147	40.470	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	80.940%
Target Compounds						
					Qvalue	
3) Chloromethane	2.146	50	623	Below Cal	#	40
16) Acetone	4.034	43	873	2.930	ug/l #	44
17) Carbon Disulfide	4.258	76	59	Below Cal	#	73
31) Cyclohexane	7.875	56	3296	1.437	ug/l #	1
36) 1,1-Dichloropropene	7.881	75	12090	4.304	ug/l #	49
38) Carbon Tetrachloride	7.881	117	14659	5.778	ug/l #	15
76) 1,2,3-Trichloropropane	12.575	75	46091	44.823	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.575	75	46091	94.031	ug/l #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052423\
Data File : VD076208.D
Acq On : 24 May 2023 12:13
Operator : KP/SY
Sample : VD0524SBL01
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01

Quant Time: May 24 16:24:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Quant Title : SW846 8260
QLast Update : Tue May 16 10:08:53 2023
Response via : Initial Calibration




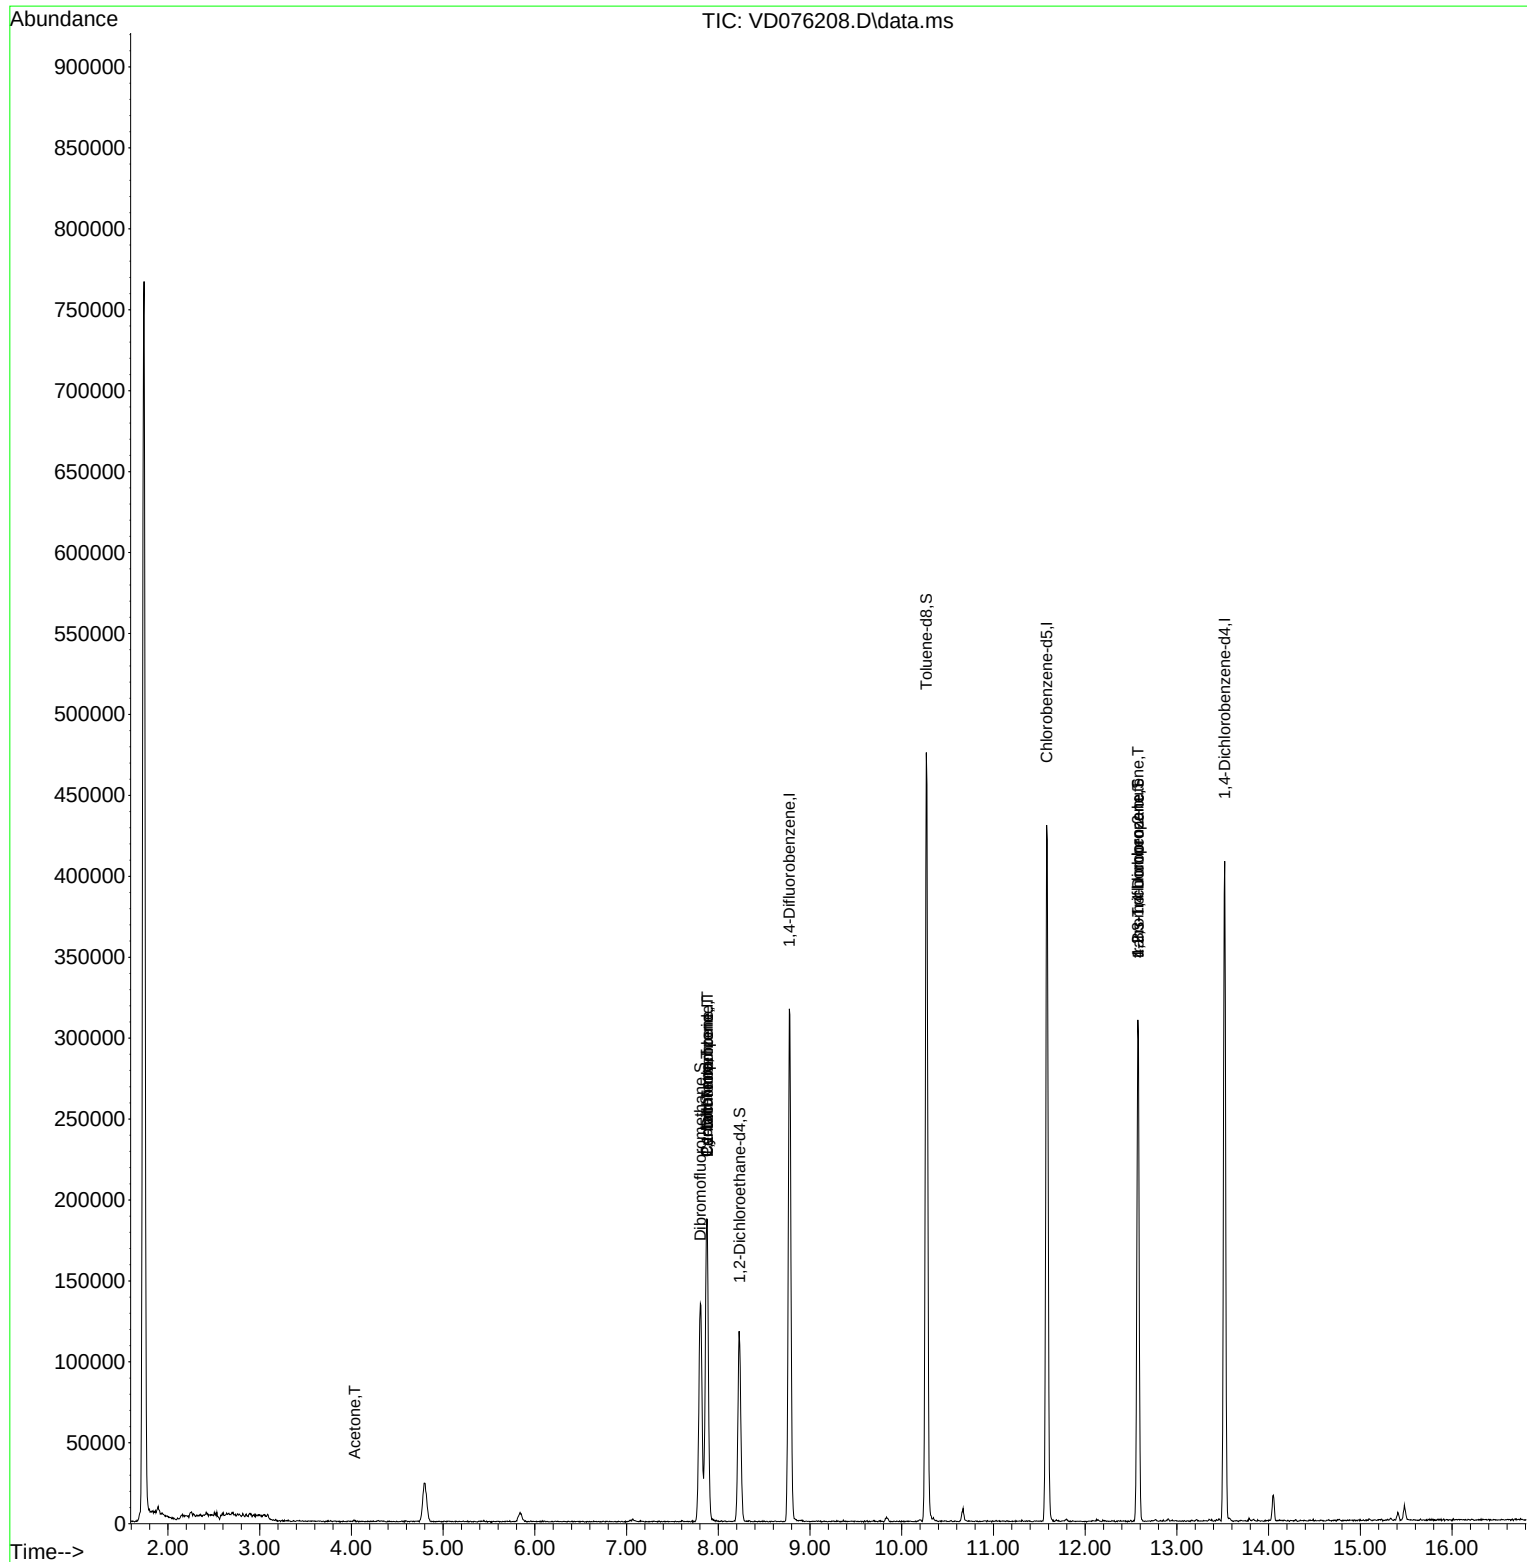


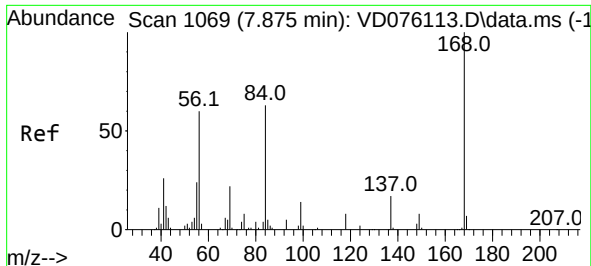

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 10
Delta R.T. 0.006 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13




Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01


Tgt Ion:168 Resp: 154952
Ion Ratio Lower Upper
168 100
99 51.6 43.8 65.6

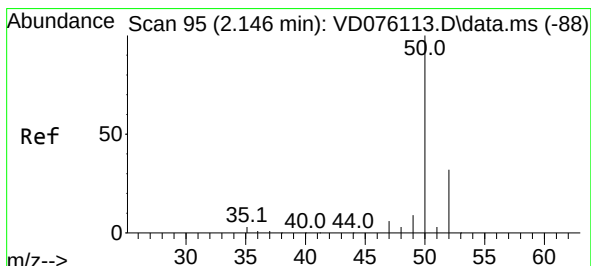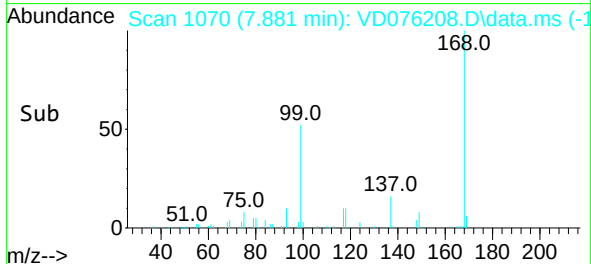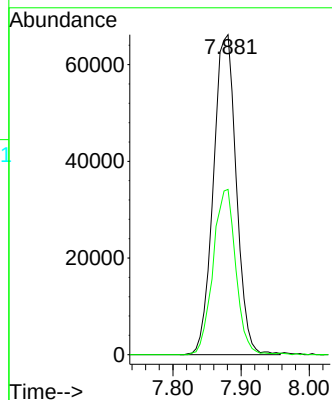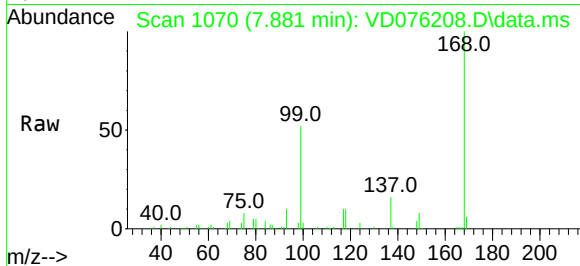

#3
Chloromethane
Concen: Below Cal
RT: 2.146 min Scan# 95
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Tgt Ion: 50 Resp: 623
Ion Ratio Lower Upper
50 100
52 0.0 27.8 41.8#

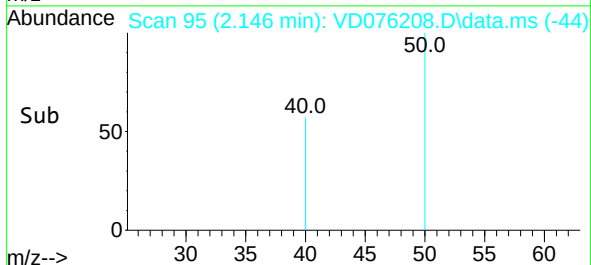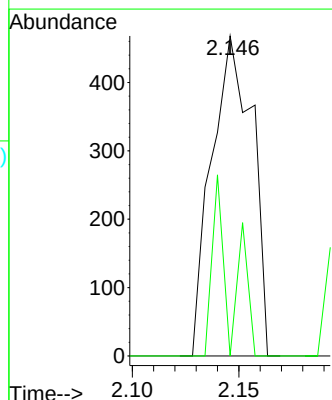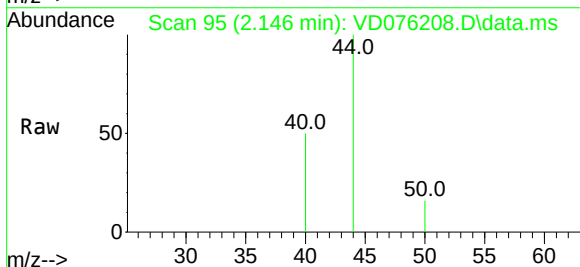

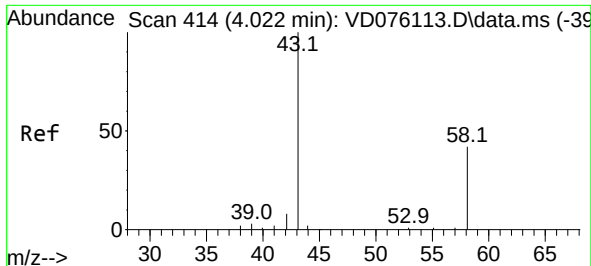

#16

Acetone

Concen: 2.930 ug/l

RT: 4.034 min Scan# 41

Delta R.T. 0.012 min

Lab File: VD076208.D

Acq: 24 May 2023 12:13

Instrument :

MSVOA_D

ClientSampleId :





VD0524SBL01

Tgt Ion: 43 Resp: 873

Ion Ratio Lower Upper

43 100

58 0.0 24.4 36.6#

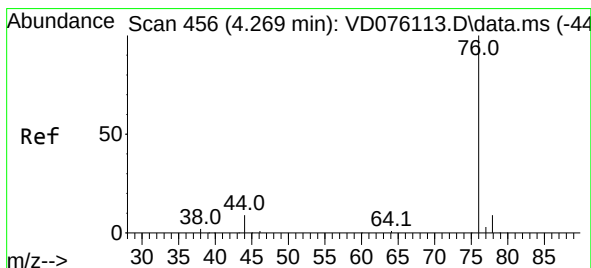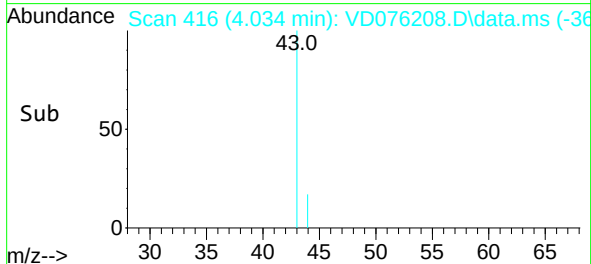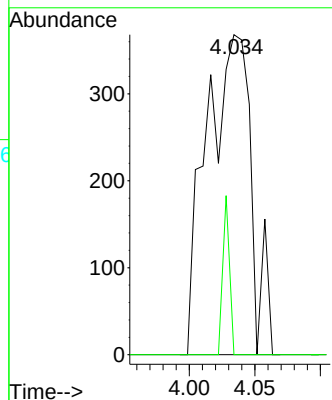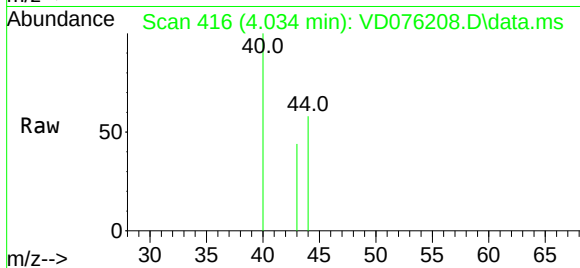

#17

Carbon Disulfide

Concen: Below Cal

RT: 4.258 min Scan# 454

Delta R.T. -0.011 min

Lab File: VD076208.D




Acq: 24 May 2023 12:13


Tgt Ion: 76 Resp: 59

Ion Ratio Lower Upper

76 100


78 0.0 8.0 12.0#

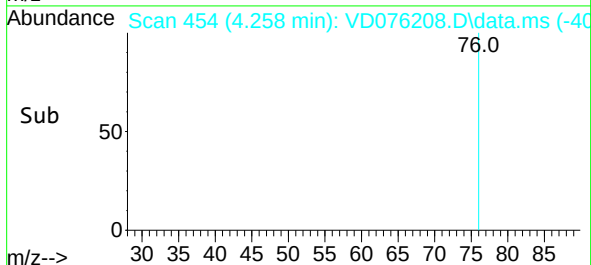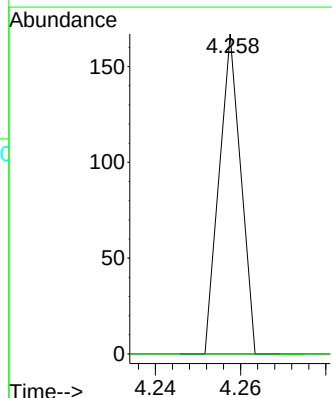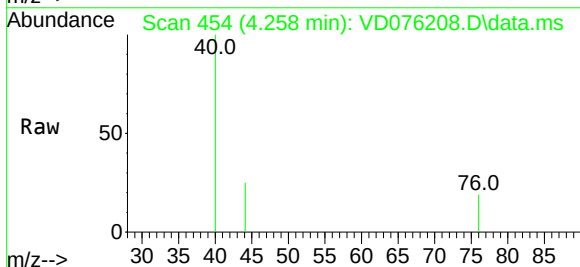



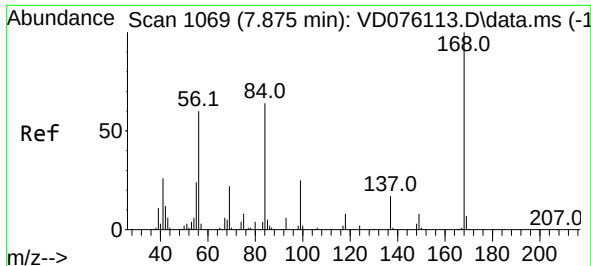


#31
Cyclohexane
Concen: 1.437 ug/l
RT: 7.875 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01



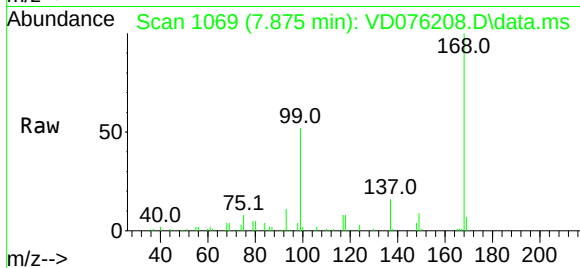



Tgt Ion: 56 Resp: 3296
Ion Ratio Lower Upper
56 100
69 176.4 25.5 38.3#
84 177.4 69.6 104.4#

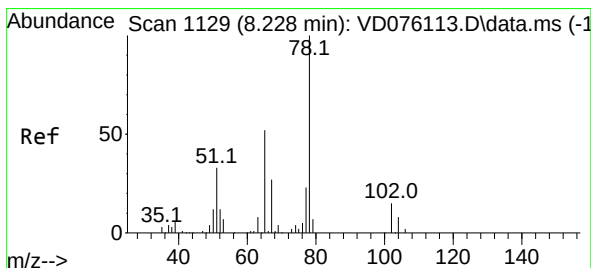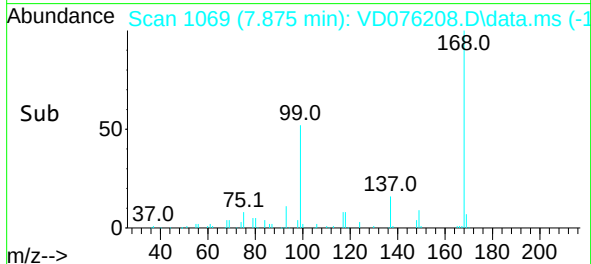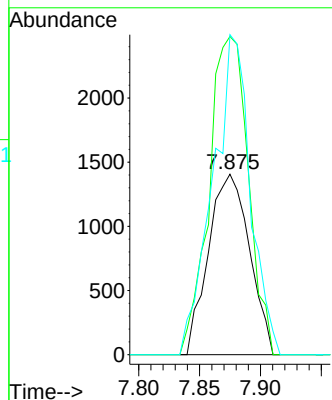

#33
1,2-Dichloroethane-d4
Concen: 59.217 ug/l
RT: 8.234 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Tgt Ion: 65 Resp: 88682
Ion Ratio Lower Upper
65 100
67 55.1 0.0 102.2

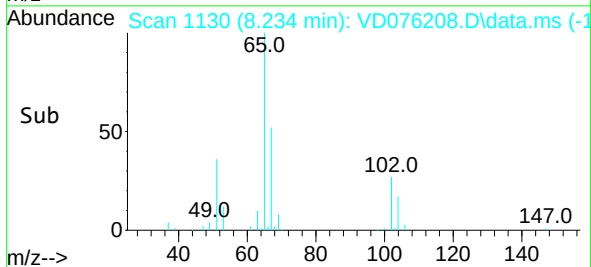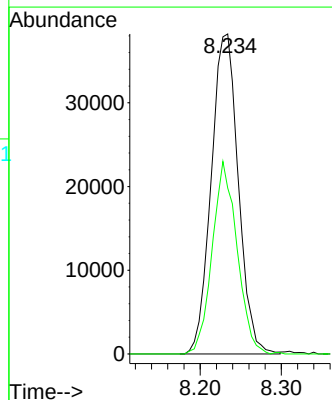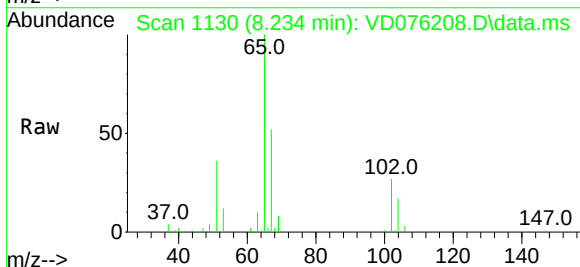

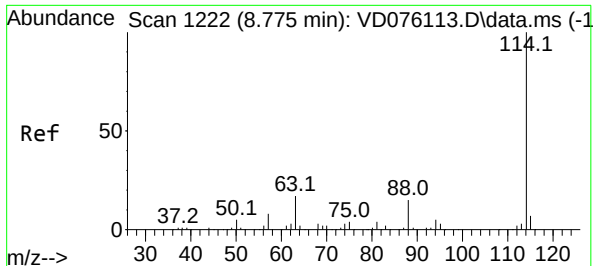

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076208.D

Acq: 24 May 2023 12:13

Instrument :

MSVOA_D

ClientSampleId :

VD0524SBL01





Tgt Ion:114 Resp: 300897

Ion Ratio Lower Upper

114 100

63 17.1 0.0 41.6

88 14.1 0.0 30.6

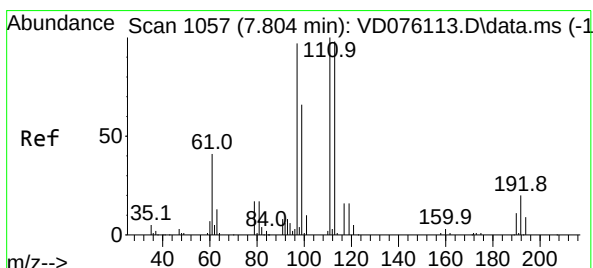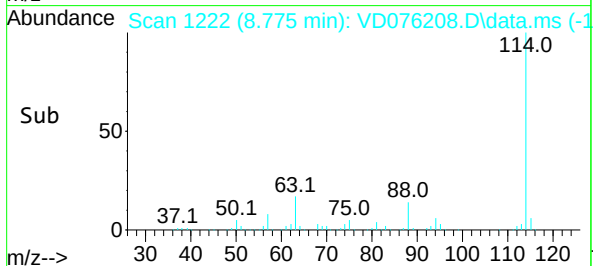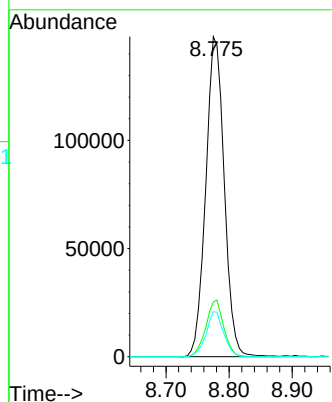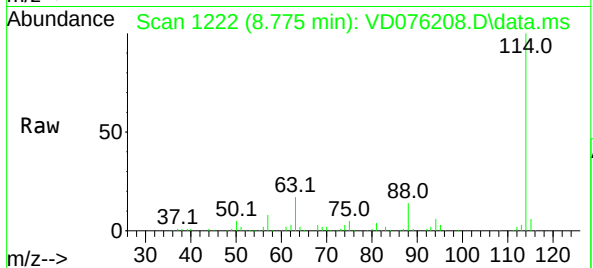

#35

Dibromofluoromethane

Concen: 49.359 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.001 min

Lab File: VD076208.D

Acq: 24 May 2023 12:13




Tgt Ion:113 Resp: 102659


Ion Ratio Lower Upper

113 100

111 101.1 81.4 122.0

192 18.8 15.2 22.8

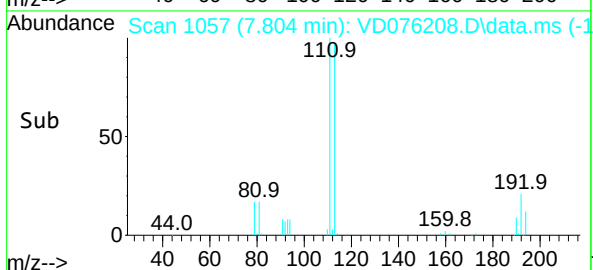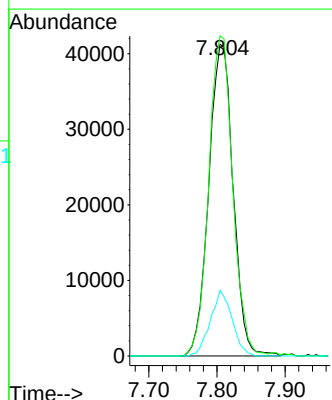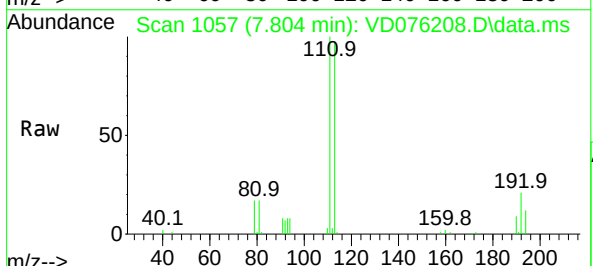

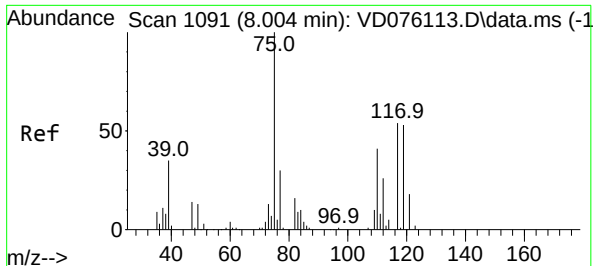

#36

1,1-Dichloropropene

Concen: 4.304 ug/l

RT: 7.881 min Scan# 1070

Delta R.T. -0.129 min

Lab File: VD076208.D

Acq: 24 May 2023 12:13

Instrument :

MSVOA_D

ClientSampleId :

VD0524SBL01





Tgt Ion: 75 Resp: 12090

Ion Ratio Lower Upper

75 100

110 7.7 17.1 51.2#

77 0.0 24.6 36.8#

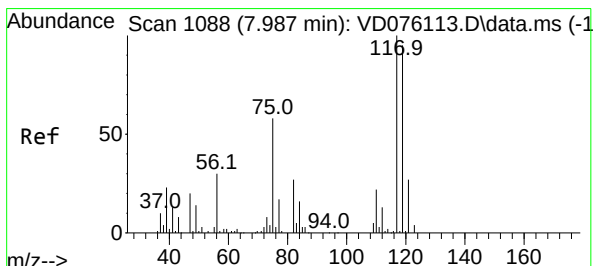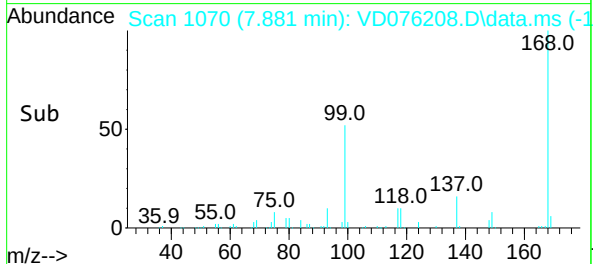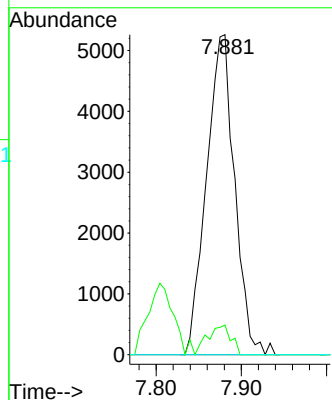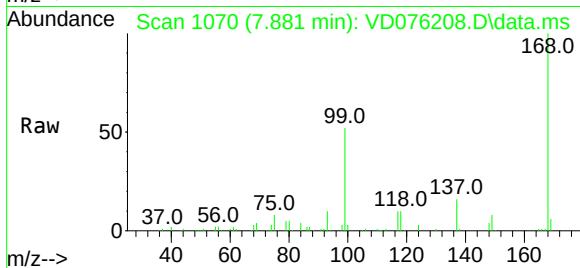

#38

Carbon Tetrachloride

Concen: 5.778 ug/l

RT: 7.881 min Scan# 1070

Delta R.T. -0.112 min

Lab File: VD076208.D

Acq: 24 May 2023 12:13




Tgt Ion: 117 Resp: 14659


Ion Ratio Lower Upper

117 100

119 2.8 74.7 112.1#

121 0.0 25.9 38.9#


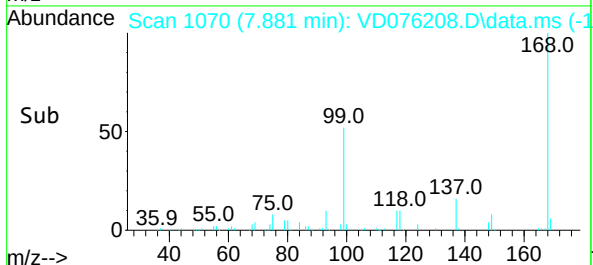
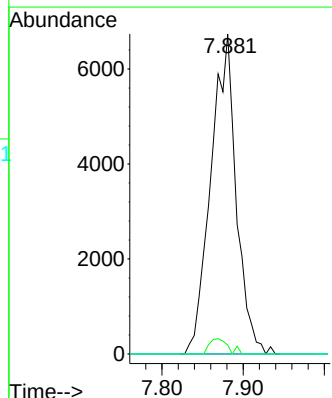
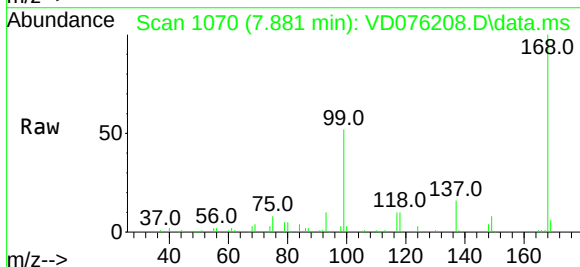


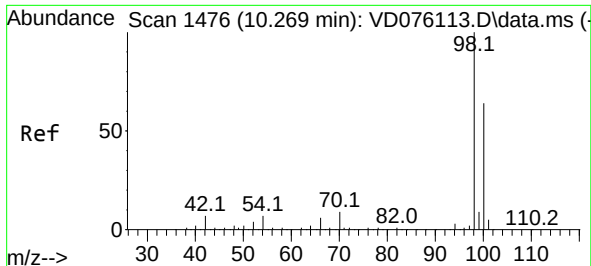

#50
Toluene-d8
Concen: 43.604 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13




Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01


Tgt Ion: 98 Resp: 353533
Ion Ratio Lower Upper
98 100
100 62.6 52.1 78.1

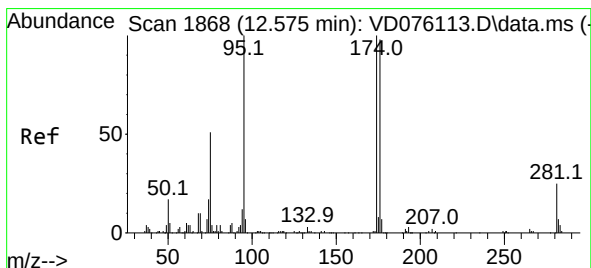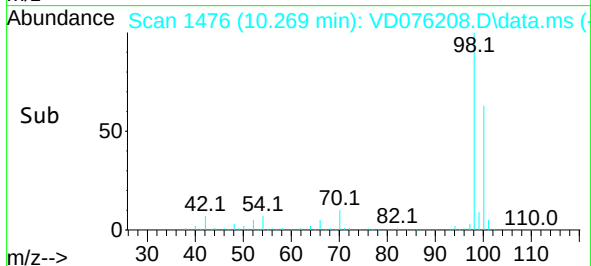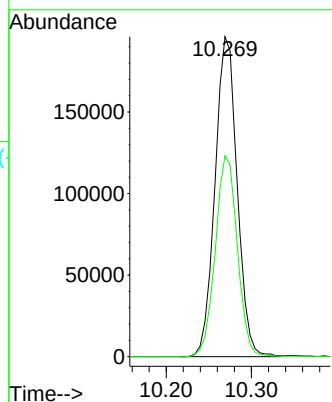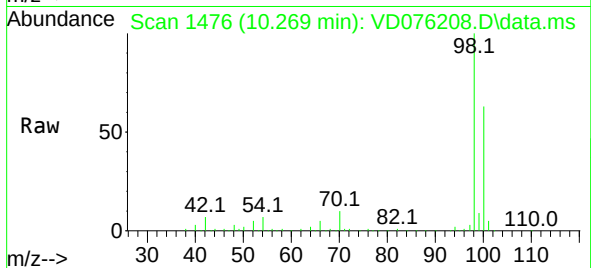

#62
4-Bromofluorobenzene
Concen: 40.470 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Tgt Ion: 95 Resp: 91147
Ion Ratio Lower Upper
95 100
174 90.8 0.0 164.0
176 85.4 0.0 156.8


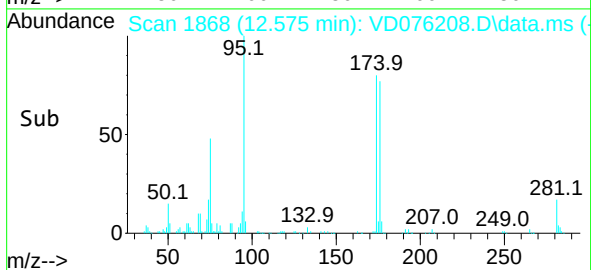
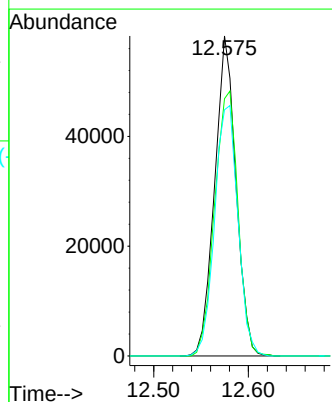
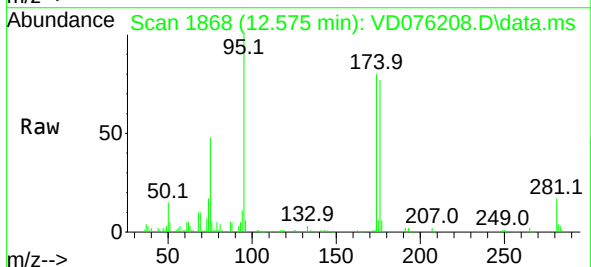


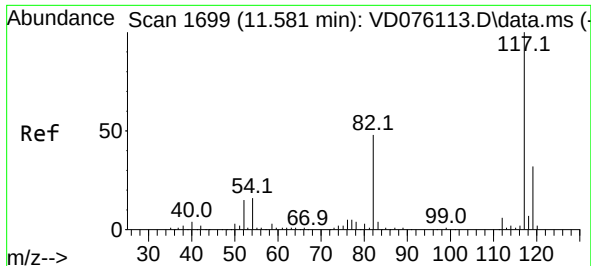

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13




Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01


Tgt Ion:117 Resp: 273236
Ion Ratio Lower Upper
117 100
82 52.4 44.0 66.0
119 31.7 25.1 37.7

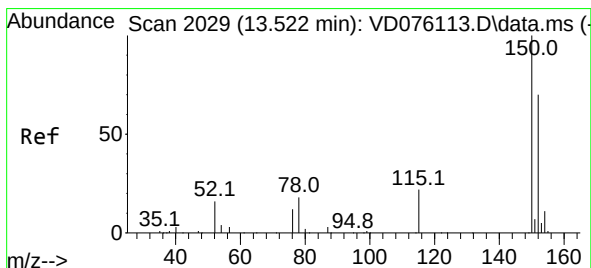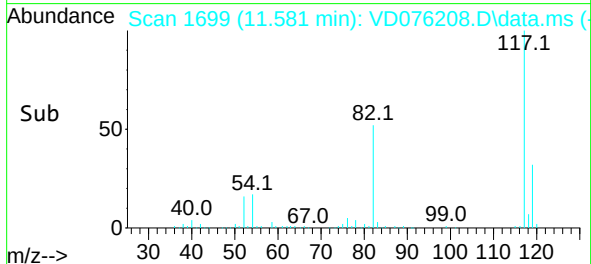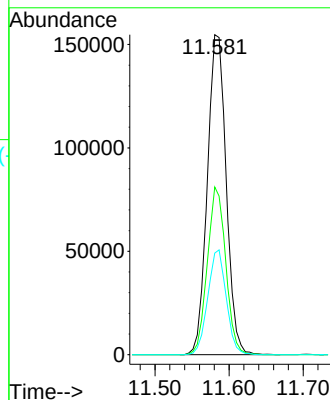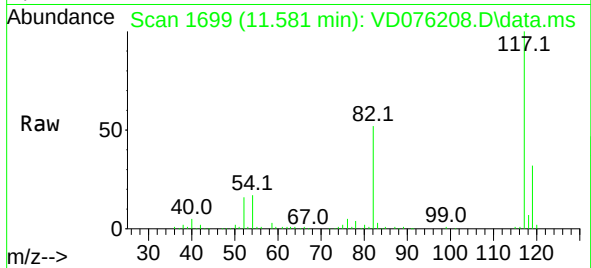

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Tgt Ion:152 Resp: 117508
Ion Ratio Lower Upper
152 100
115 53.5 30.1 90.3
150 157.9 0.0 364.8


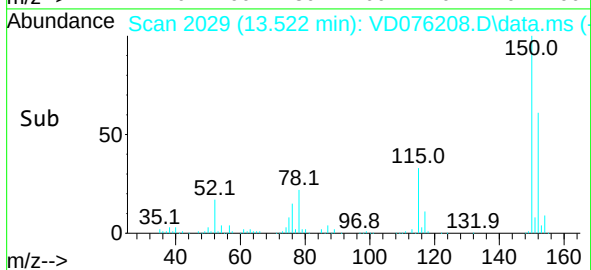
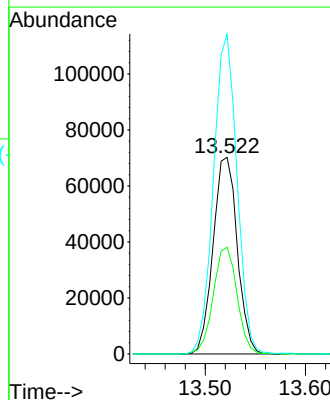
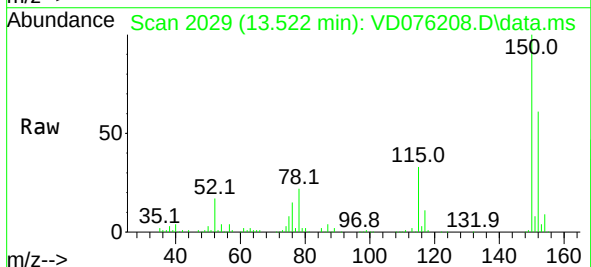


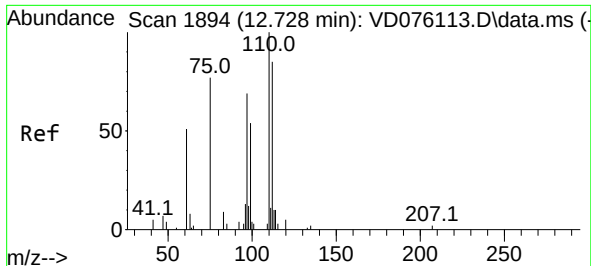

#76
1,2,3-Trichloropropane
Concen: 44.823 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.153 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Instrument :
MSVOA_D
ClientSampleId :
VD0524SBL01

Tgt Ion: 75 Resp: 46091
Ion Ratio Lower Upper
75 100
77 1.6 0.0 0.0#

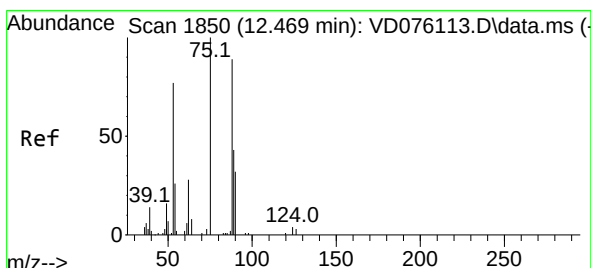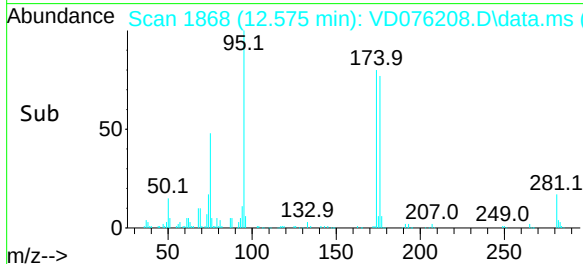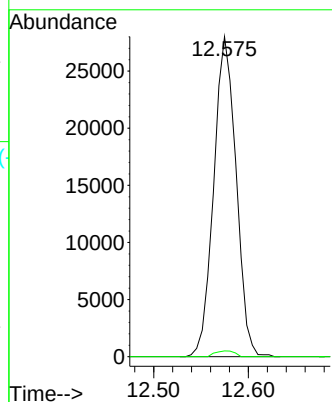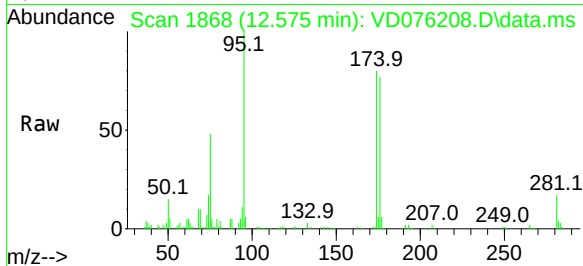

#81
trans-1,4-Dichloro-2-butene
Concen: 94.031 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.100 min
Lab File: VD076208.D
Acq: 24 May 2023 12:13

Tgt Ion: 75 Resp: 46091
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.2 40.2 60.4#

