

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052722\
 Data File : VD073411.D
 Acq On : 27 May 2022 15:11
 Operator : VA/SY
 Sample : N3080-04
 Misc : 5.28G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 WC-5

Quant Time: May 28 09:44:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
 Quant Title : SW846 8260
 QLast Update : Thu May 19 15:13:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	273462	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	490431	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	542523	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	246112	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	149800	49.567	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.140%
35) Dibromofluoromethane	7.909	113	167093	51.633	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.260%
50) Toluene-d8	10.332	98	613074	51.392	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.780%
62) 4-Bromofluorobenzene	12.620	95	232743	55.593	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052722\
Data File : VD073411.D
Acq On : 27 May 2022 15:11
Operator : VA/SY
Sample : N3080-04
Misc : 5.28G/5.00ml/MSVOA_D/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
WC-5

Quant Time: May 28 09:44:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
Quant Title : SW846 8260
QLast Update : Thu May 19 15:13:42 2022
Response via : Initial Calibration

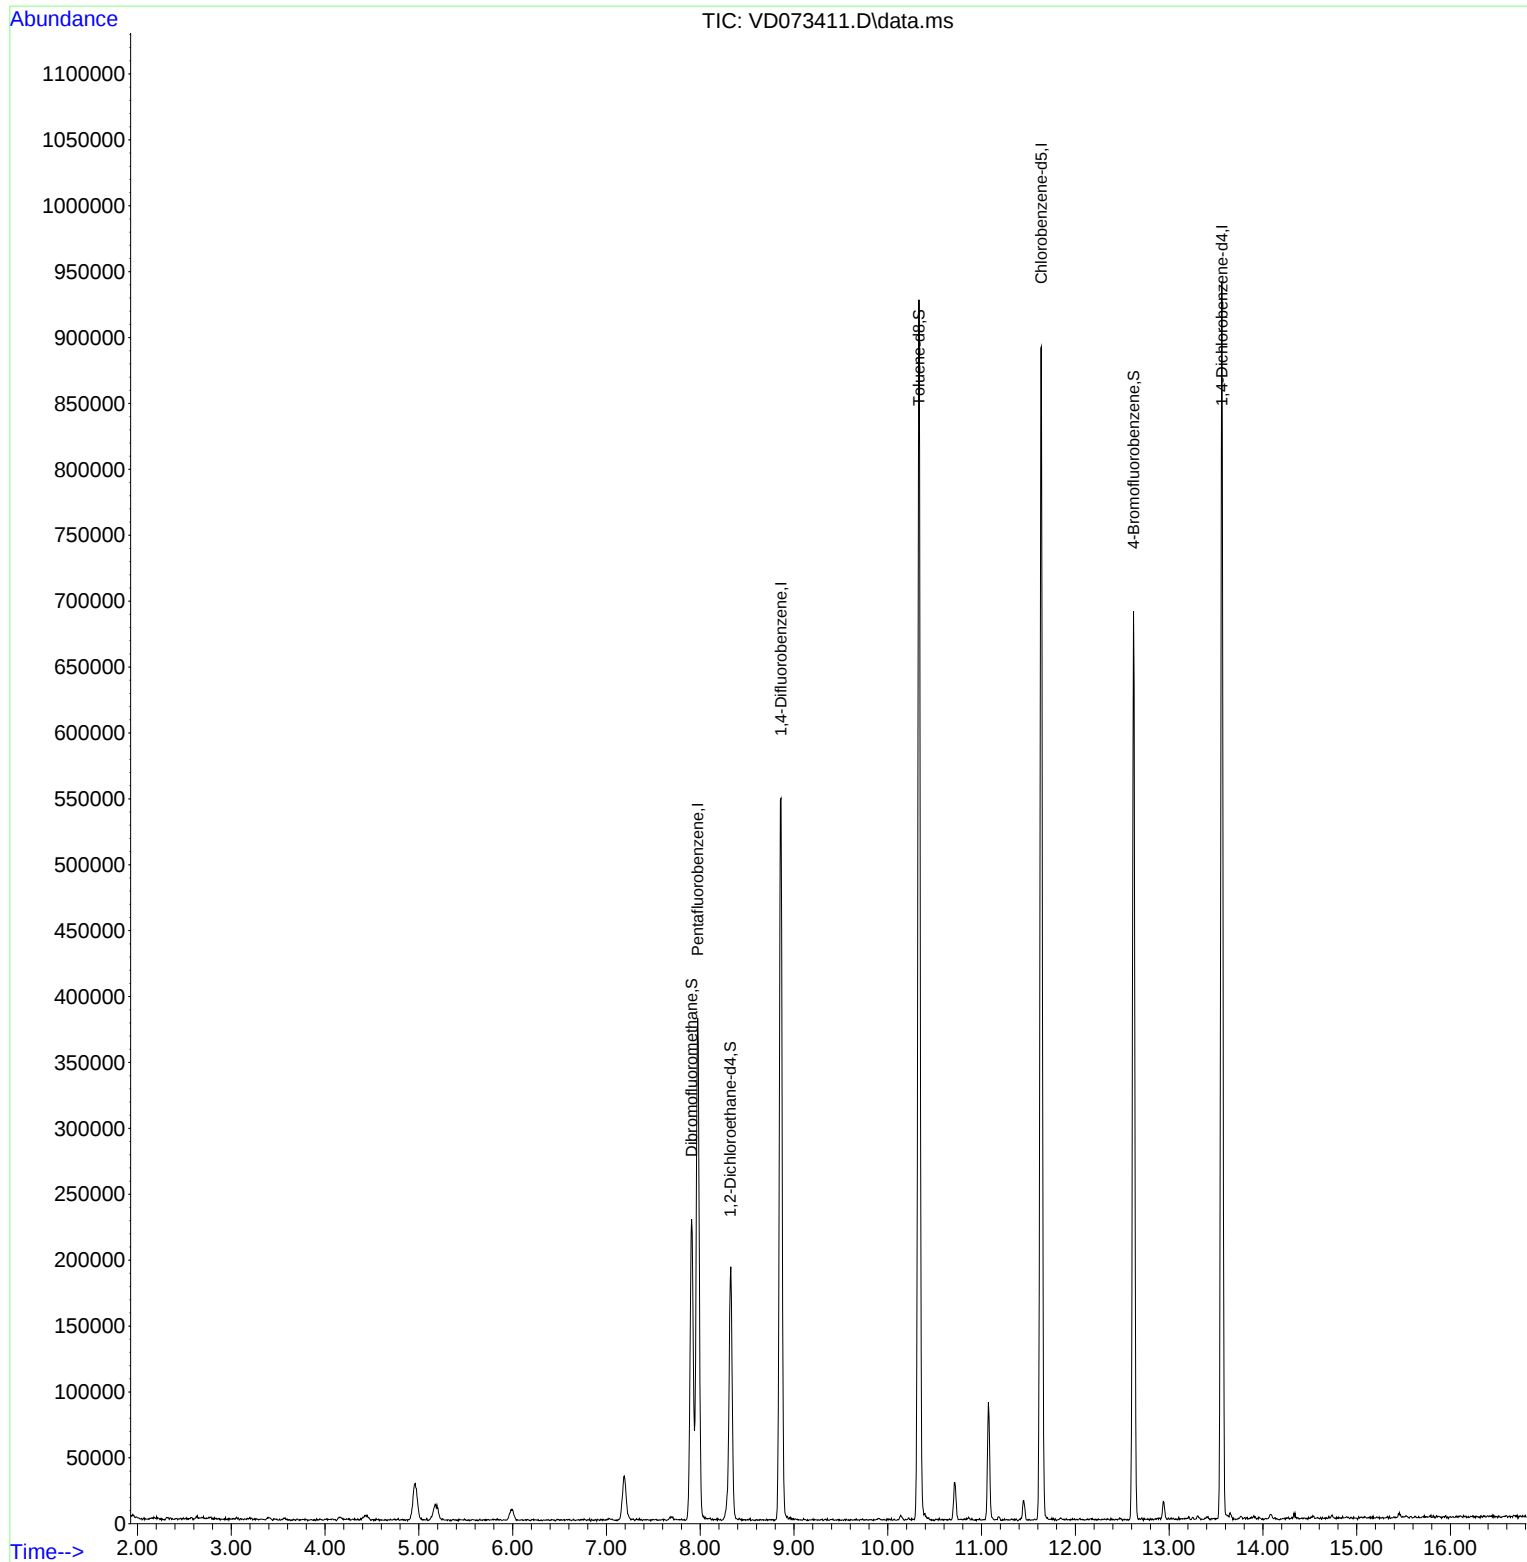

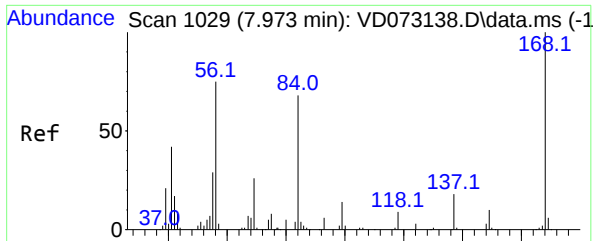

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. 0.000 min

Lab File: VD073411.D

Acq: 27 May 2022 15:11

Instrument :

MSVOA_D

ClientSampleId :





WC-5

Tgt Ion:168 Resp: 273462

Ion Ratio Lower Upper

168 100

99 59.6 49.8 74.6

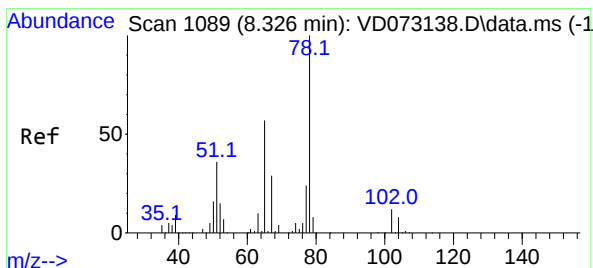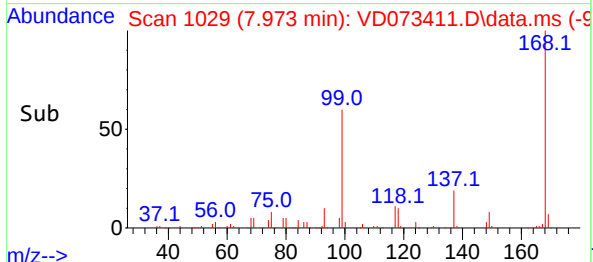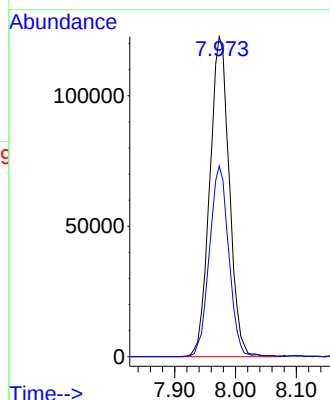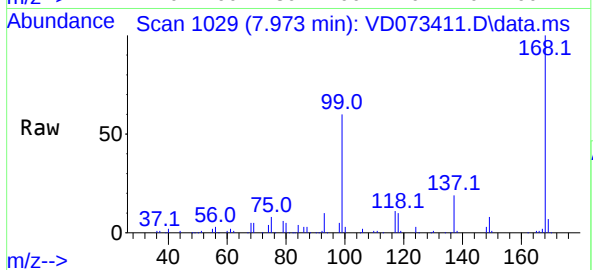

1,2-Dichloroethane-d4

Concen: 49.567 ug/l

RT: 8.320 min Scan# 1088

Delta R.T. -0.006 min

Lab File: VD073411.D




Acq: 27 May 2022 15:11


Tgt Ion: 65 Resp: 149800

Ion Ratio Lower Upper

65 100

67 53.2 0.0 101.4

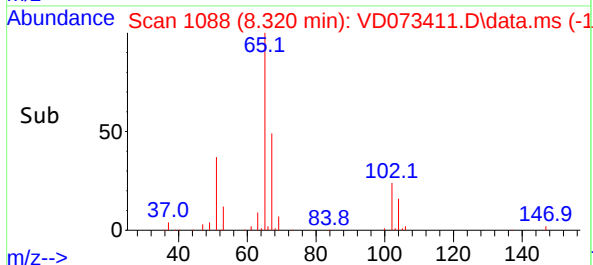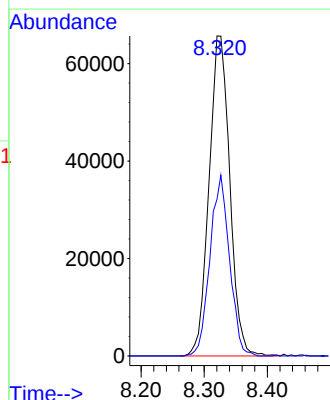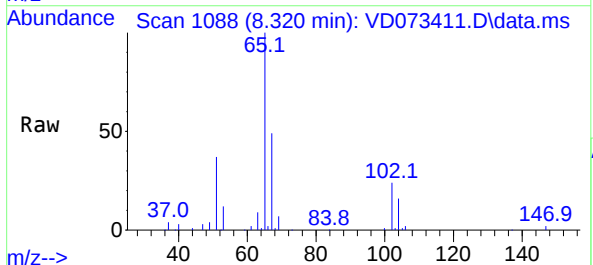

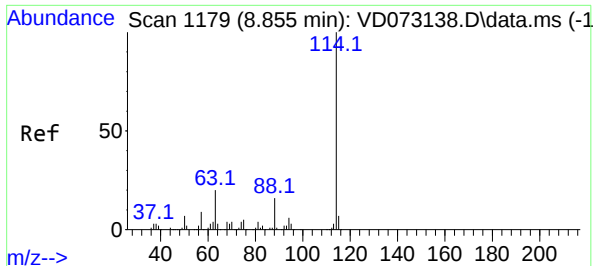

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1179

Delta R.T. 0.006 min

Lab File: VD073411.D

Acq: 27 May 2022 15:11

Instrument :

MSVOA_D

ClientSampleId :

WC-5





Tgt Ion:114 Resp: 490431

Ion Ratio Lower Upper

114 100

63 18.9 0.0 46.6

88 15.5 0.0 33.2

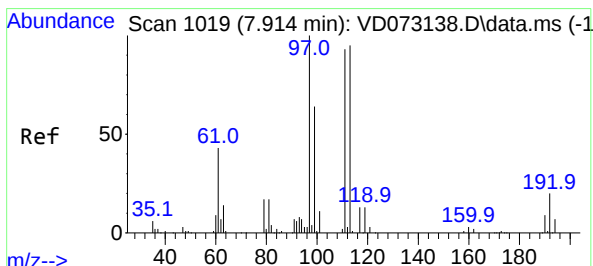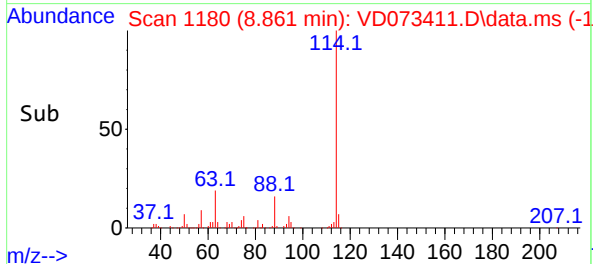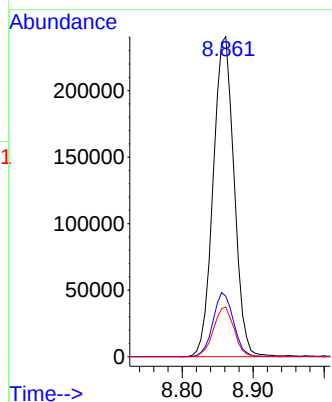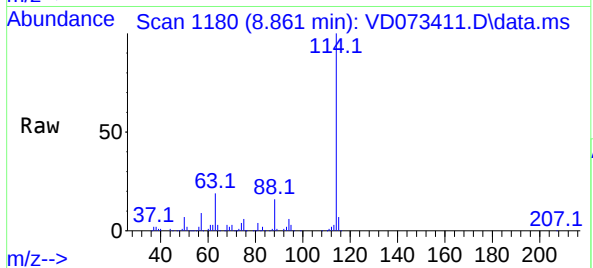

#35

Dibromofluoromethane

Concen: 51.633 ug/l

RT: 7.909 min Scan# 1018

Delta R.T. -0.005 min

Lab File: VD073411.D

Acq: 27 May 2022 15:11




Tgt Ion:113 Resp: 167093

Ion Ratio Lower Upper

113 100

111 104.7 83.8 125.6

192 18.7 14.6 21.8


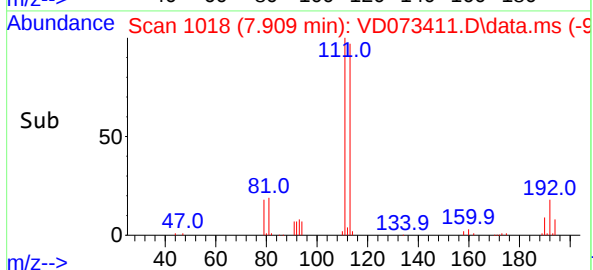
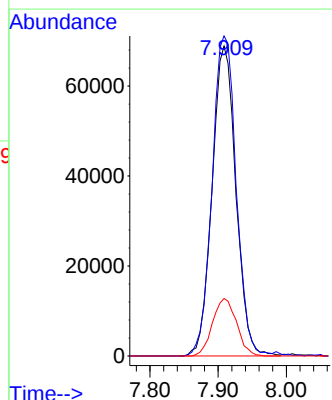
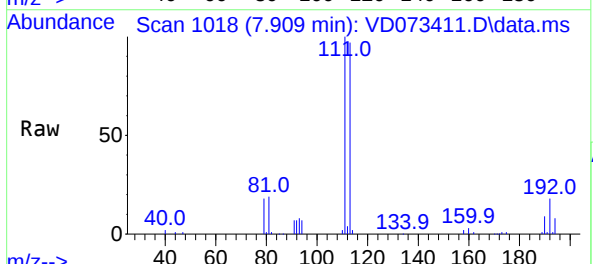




#50
Toluene-d8
Concen: 51.392 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073411.D
Acq: 27 May 2022 15:11




Instrument :
MSVOA_D
ClientSampleId :
WC-5


Tgt Ion: 98 Resp: 613074
Ion Ratio Lower Upper
98 100
100 65.1 52.4 78.6

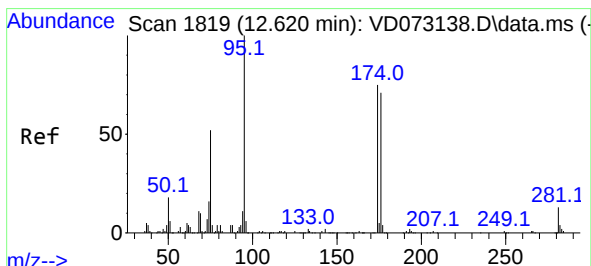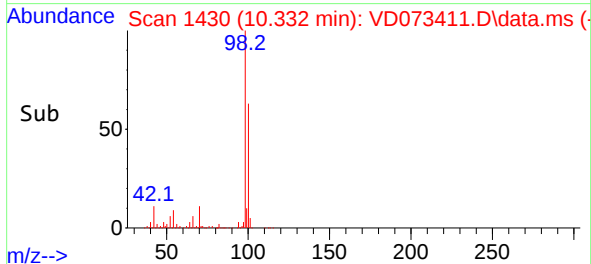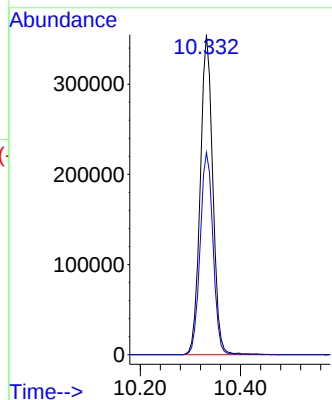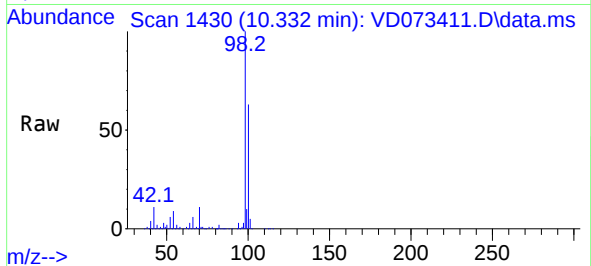

#62
4-Bromofluorobenzene
Concen: 55.593 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073411.D
Acq: 27 May 2022 15:11

Tgt Ion: 95 Resp: 232743
Ion Ratio Lower Upper
95 100
174 78.1 0.0 152.8
176 73.6 0.0 145.4

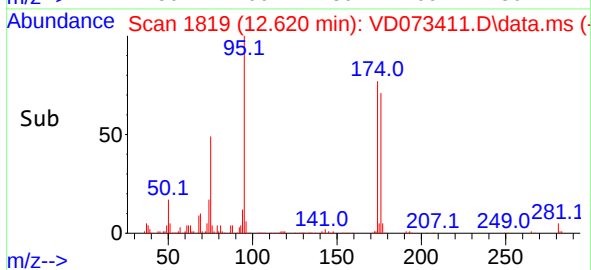
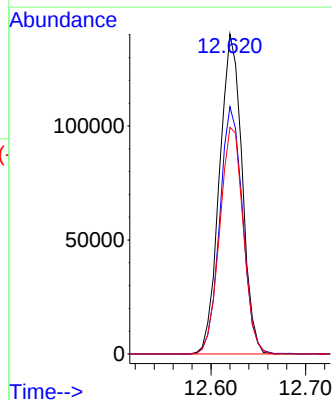
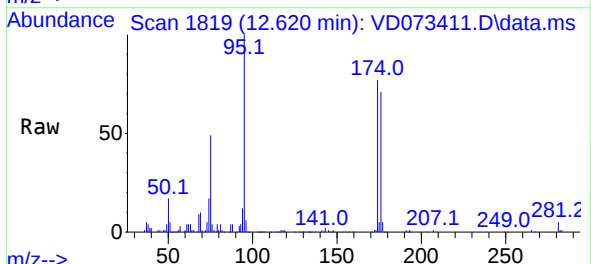


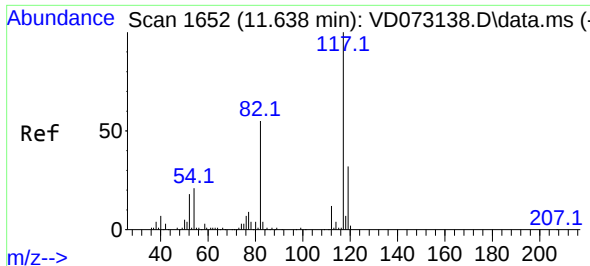

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD073411.D
Acq: 27 May 2022 15:11

Instrument :
MSVOA_D
ClientSampleId :
WC-5

Tgt Ion:117 Resp: 542523
Ion Ratio Lower Upper
117 100
82 51.6 45.3 67.9
119 31.2 26.6 40.0

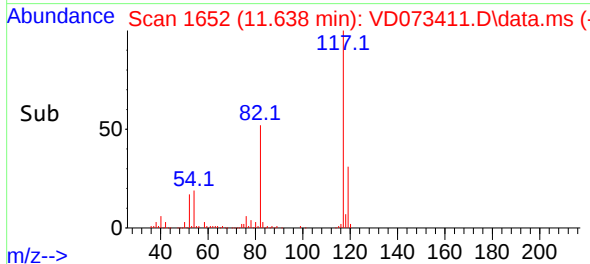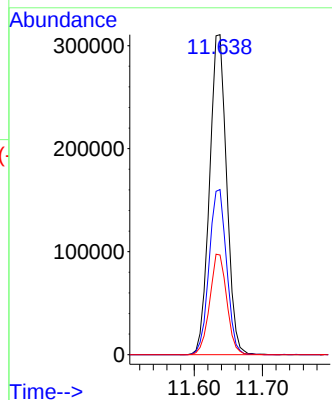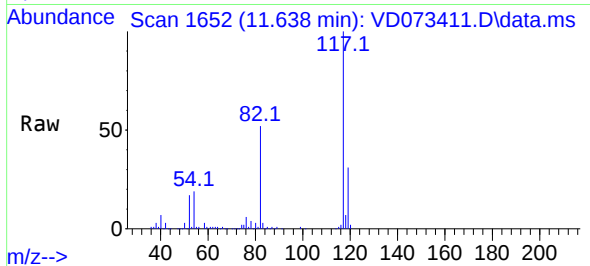

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073411.D
Acq: 27 May 2022 15:11

Tgt Ion:152 Resp: 246112
Ion Ratio Lower Upper
152 100
115 60.2 31.3 93.8
150 159.6 0.0 348.6

