


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD053023\
Data File : VD076270.D
Acq On : 30 May 2023 10:39
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051523S.M
Title : SW846 8260
Last Update : Tue May 16 10:08:53 2023

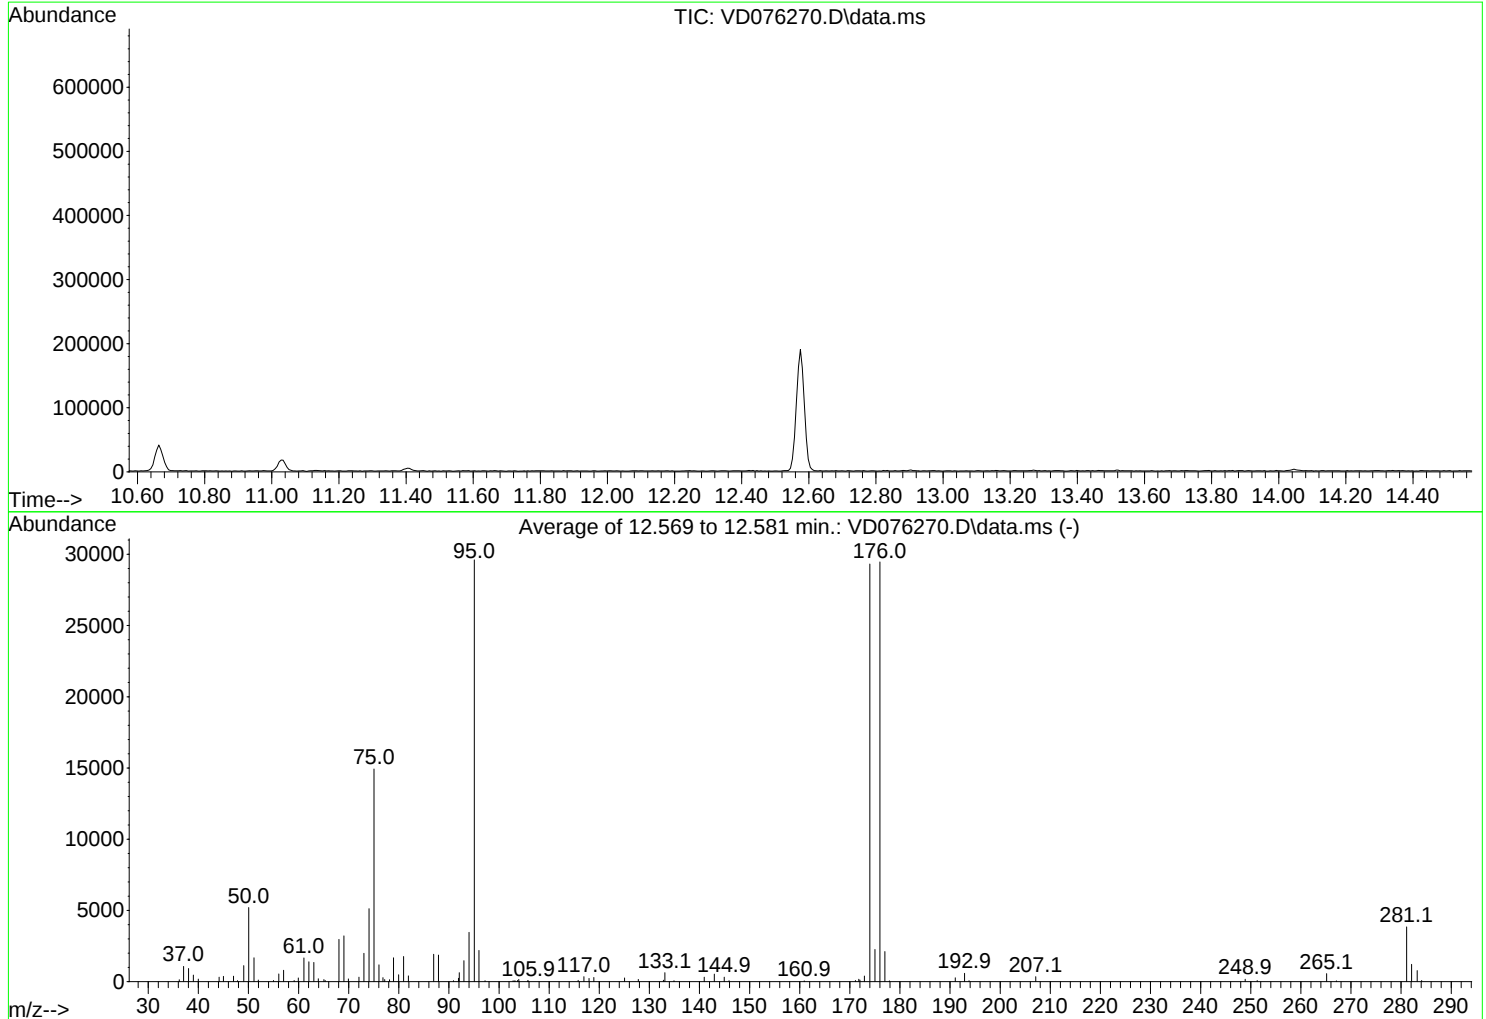

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	5198	PASS
75	95	30	60	50.4	14923	PASS
95	95	100	100	100.0	29611	PASS
96	95	5	9	7.4	2191	PASS
173	174	0.00	2	1.3	389	PASS
174	95	50	100	99.0	29320	PASS
175	174	5	9	7.7	2253	PASS
176	174	95	101	100.5	29461	PASS
177	176	5	9	7.2	2116	PASS