


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD060419\
Data File : VD062596.D
Acq On : 4 Jun 2019 13:16
Operator : FY/SY
Sample : BFB
Misc : 5.00µ/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D053019S.M
Title : SW846 8260
Last Update : Fri May 31 02:08:29 2019

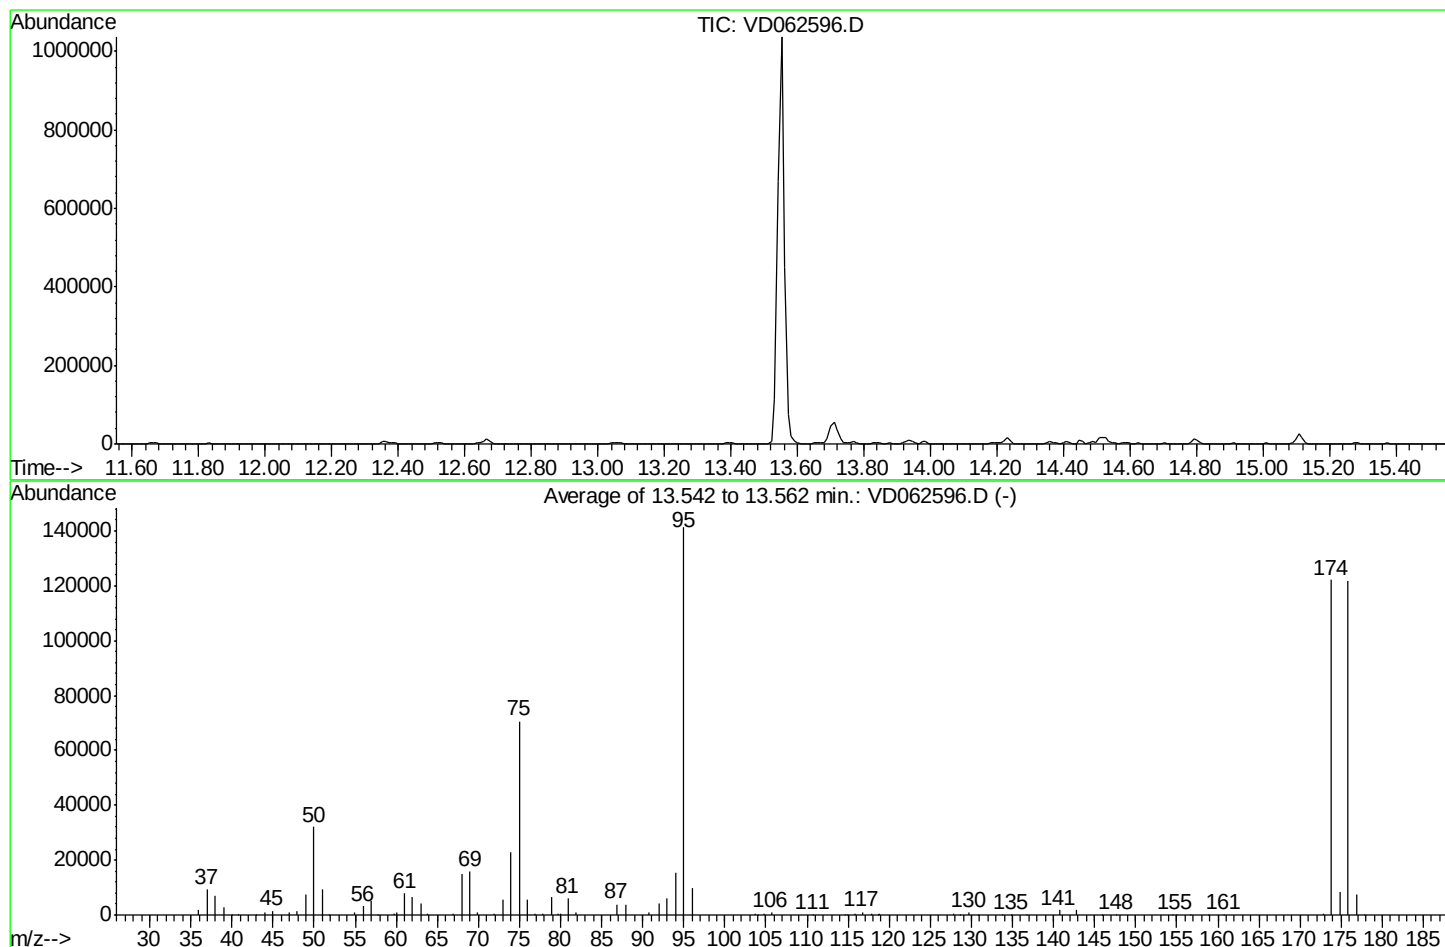

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	32127	PASS
75	95	30	60	49.9	70528	PASS
95	95	100	100	100.0	141349	PASS
96	95	5	9	6.9	9815	PASS
173	174	0.00	2	0.3	315	PASS
174	95	50	100	86.4	122069	PASS
175	174	5	9	6.9	8415	PASS
176	174	95	101	99.7	121696	PASS
177	176	5	9	6.1	7442	PASS