

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060823\
 Data File : VD076382.D
 Acq On : 08 Jun 2023 19:31
 Operator : KP/SY
 Sample : 03074-04
 Misc : 6.85G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 GT-04

Quant Time: Jun 09 01:25:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060523S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 06 02:52:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	238151	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	442488	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	370329	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.522	152	174760	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	146442	68.629	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	137.260%
35) Dibromofluoromethane	7.804	113	187631	66.784	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	133.560%
50) Toluene-d8	10.269	98	342895	30.654	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	61.300%
62) 4-Bromofluorobenzene	12.575	95	161064	54.408	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	108.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060823\
Data File : VD076382.D
Acq On : 08 Jun 2023 19:31
Operator : KP/SY
Sample : 03074-04
Misc : 6.85G/5.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
GT-04

Quant Time: Jun 09 01:25:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060523S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 06 02:52:23 2023
Response via : Initial Calibration




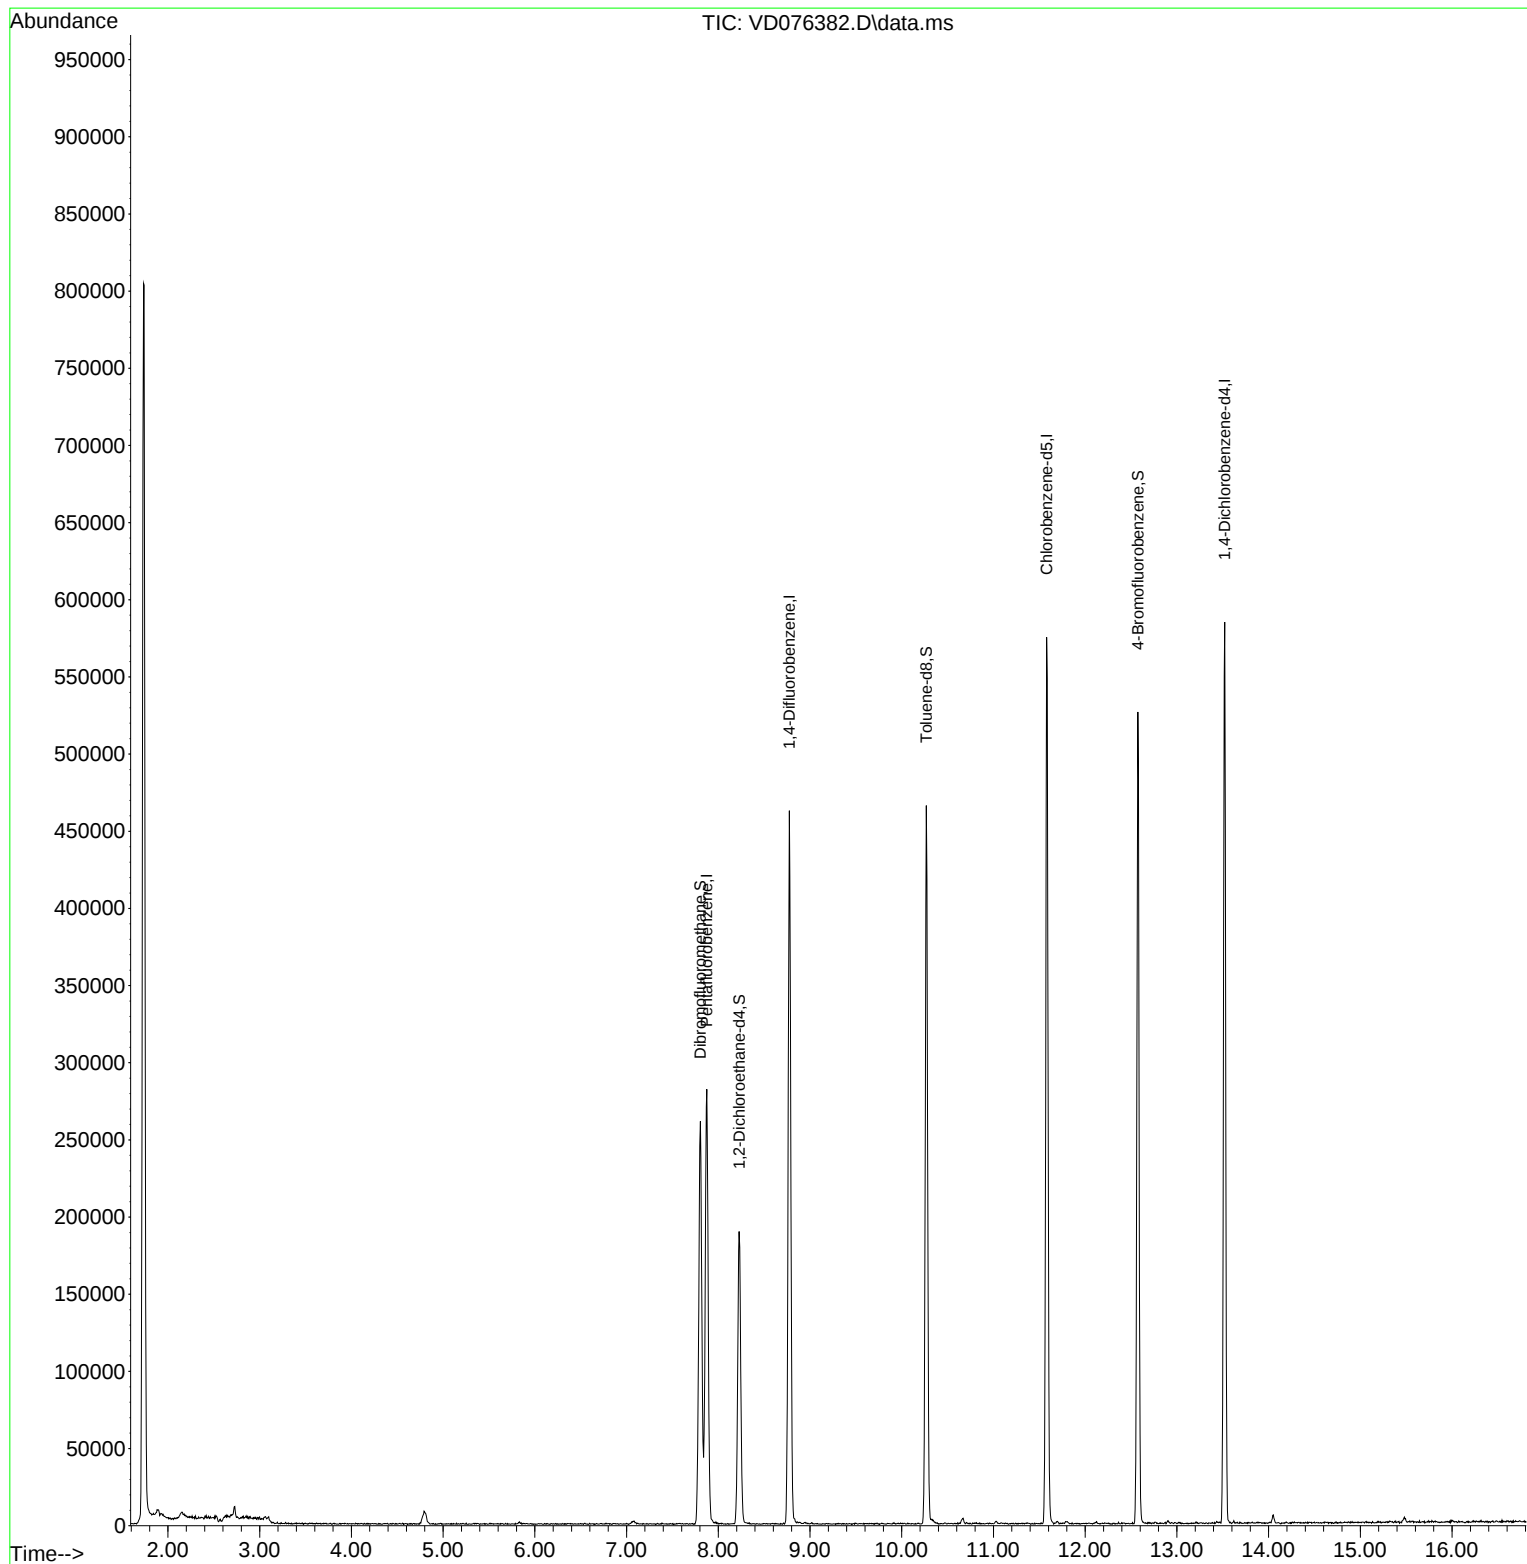


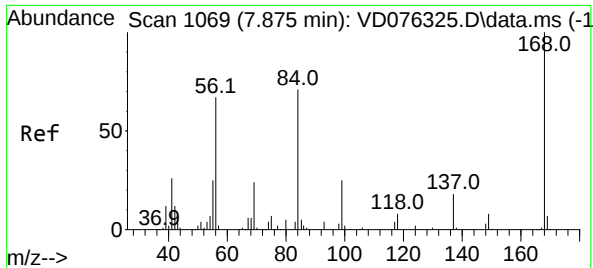

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31




Instrument :
MSVOA_D
ClientSampleId :
GT-04


Tgt Ion:168 Resp: 238151
Ion Ratio Lower Upper
168 100
99 44.5 36.7 55.1

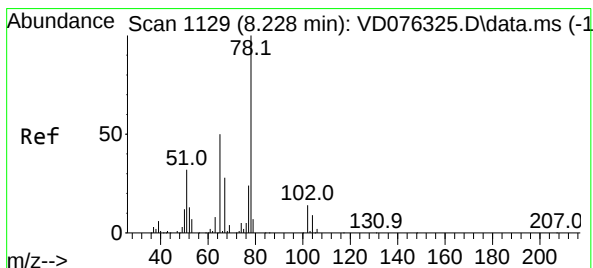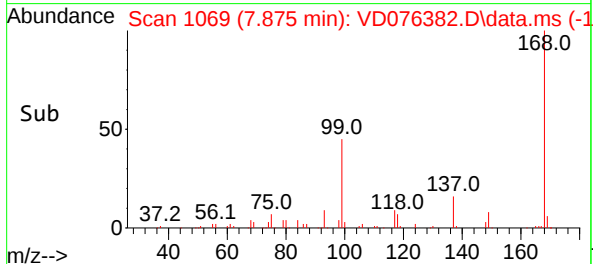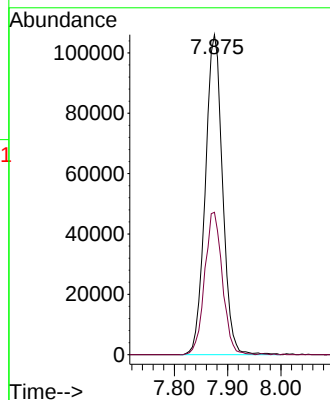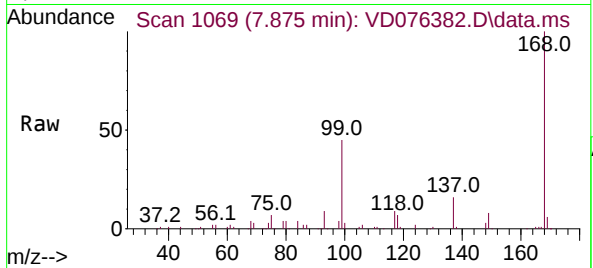

#33
1,2-Dichloroethane-d4
Concen: 68.629 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31

Tgt Ion: 65 Resp: 146442
Ion Ratio Lower Upper
65 100
67 57.3 0.0 115.0

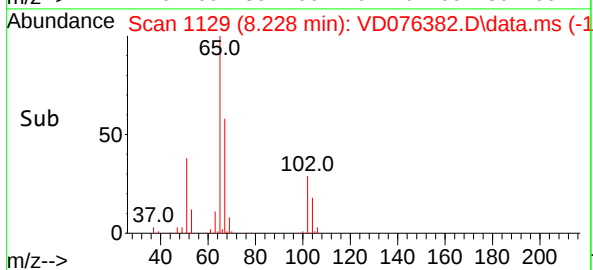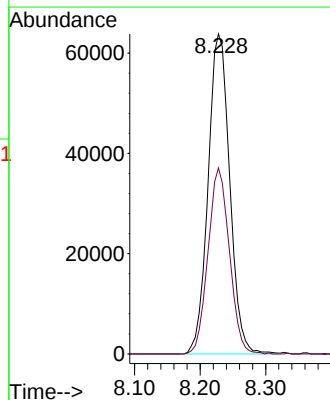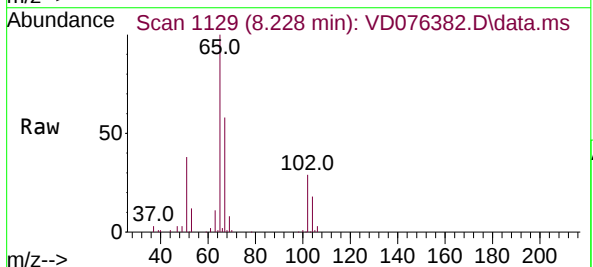

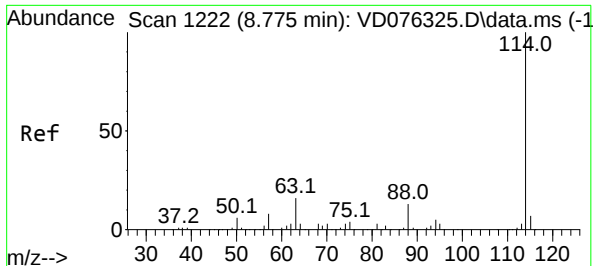

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076382.D

Acq: 08 Jun 2023 19:31

Instrument :

MSVOA_D

ClientSampleId :

GT-04





Tgt Ion:114 Resp: 442488

Ion Ratio Lower Upper

114 100

63 15.4 0.0 33.4

88 13.1 0.0 26.2

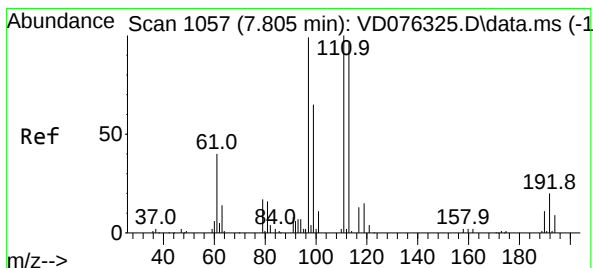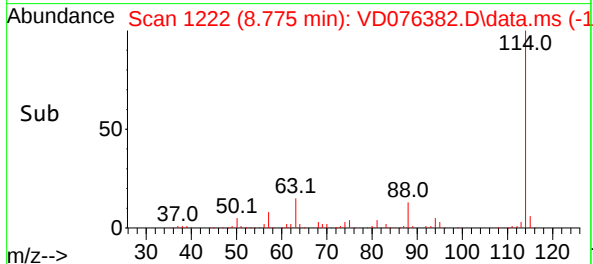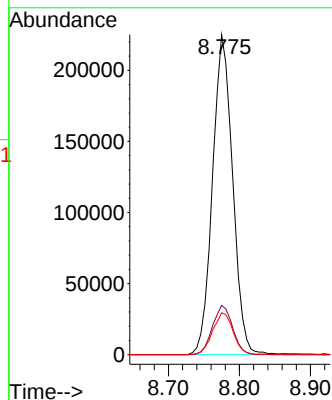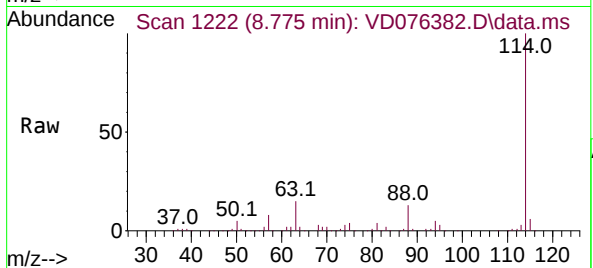

#35

Dibromofluoromethane

Concen: 66.784 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076382.D

Acq: 08 Jun 2023 19:31




Tgt Ion:113 Resp: 187631


Ion Ratio Lower Upper

113 100

111 102.4 84.7 127.1

192 21.4 16.8 25.2


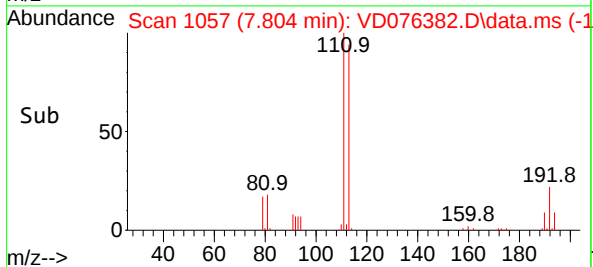
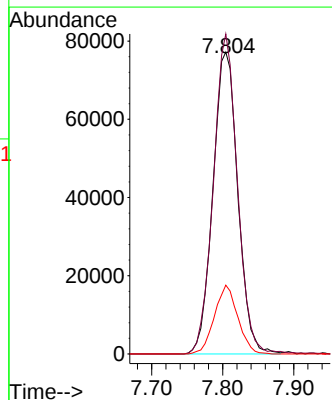
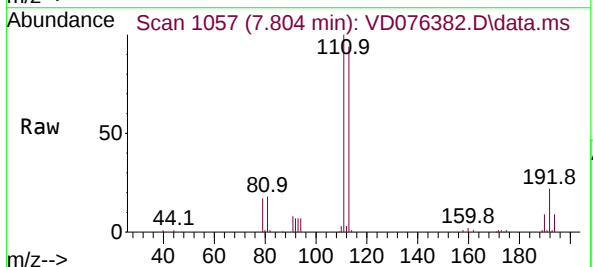


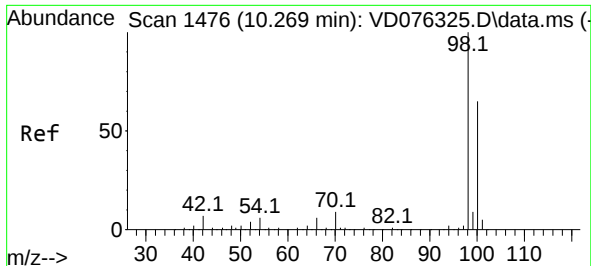

#50
Toluene-d8
Concen: 30.654 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31




Instrument :
MSVOA_D
ClientSampleId :
GT-04


Tgt Ion: 98 Resp: 342895
Ion Ratio Lower Upper
98 100
100 63.0 50.3 75.5

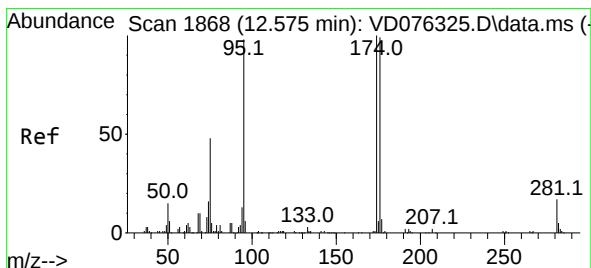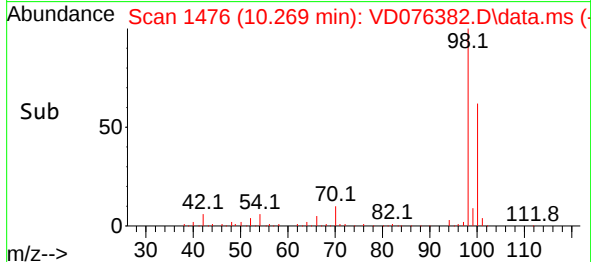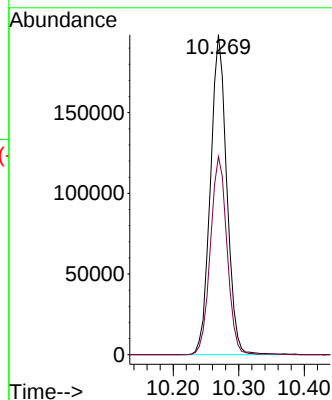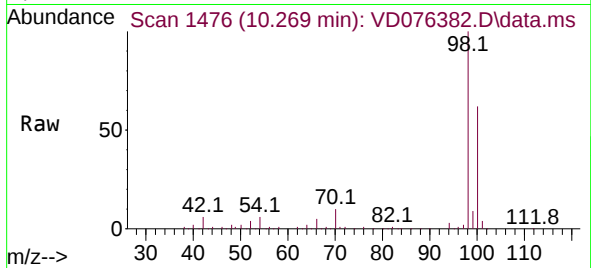

#62
4-Bromofluorobenzene
Concen: 54.408 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31

Tgt Ion: 95 Resp: 161064
Ion Ratio Lower Upper
95 100
174 97.3 0.0 201.8
176 94.9 0.0 191.8


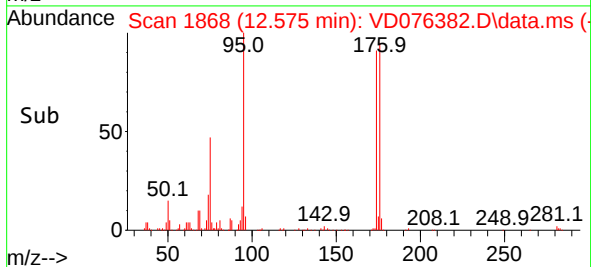
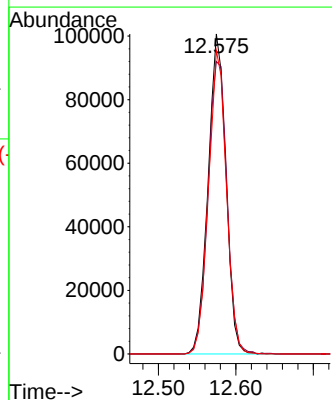
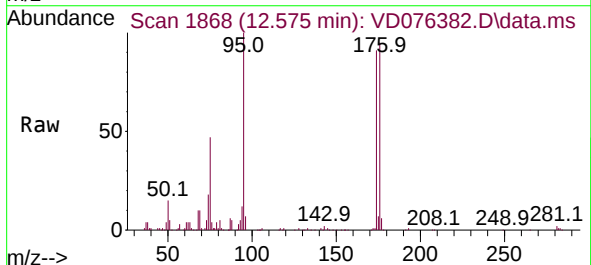


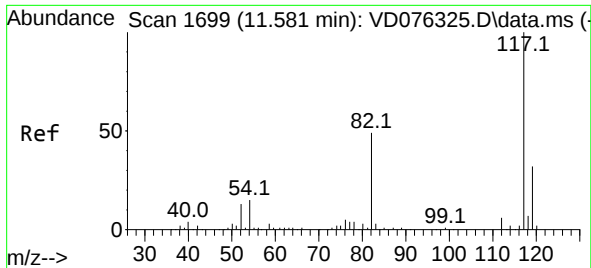

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31

Instrument :
MSVOA_D
ClientSampleId :
GT-04

Tgt Ion:117 Resp: 370329
Ion Ratio Lower Upper
117 100
82 48.4 38.3 57.5
119 32.0 25.0 37.4

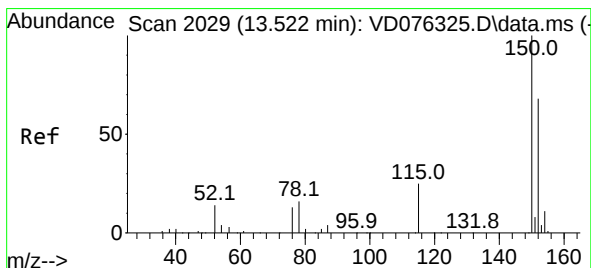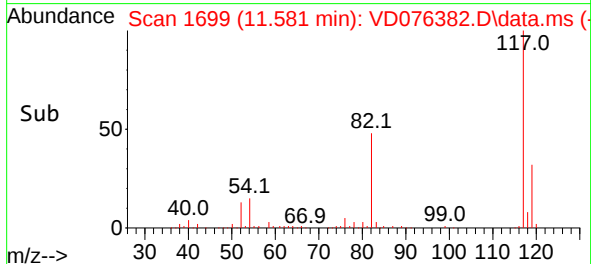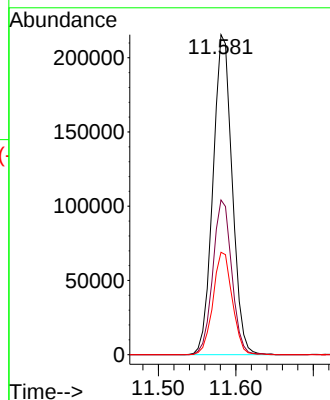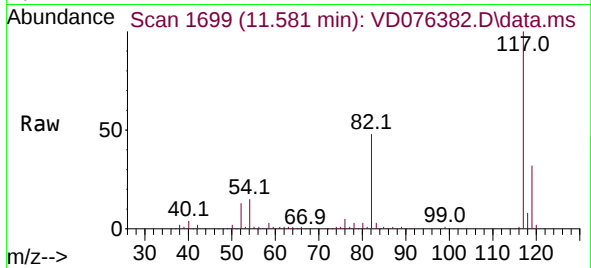

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.522 min Scan# 2029
Delta R.T. -0.000 min
Lab File: VD076382.D
Acq: 08 Jun 2023 19:31

Tgt Ion:152 Resp: 174760
Ion Ratio Lower Upper
152 100
115 51.9 27.1 81.3
150 155.2 0.0 353.6

