
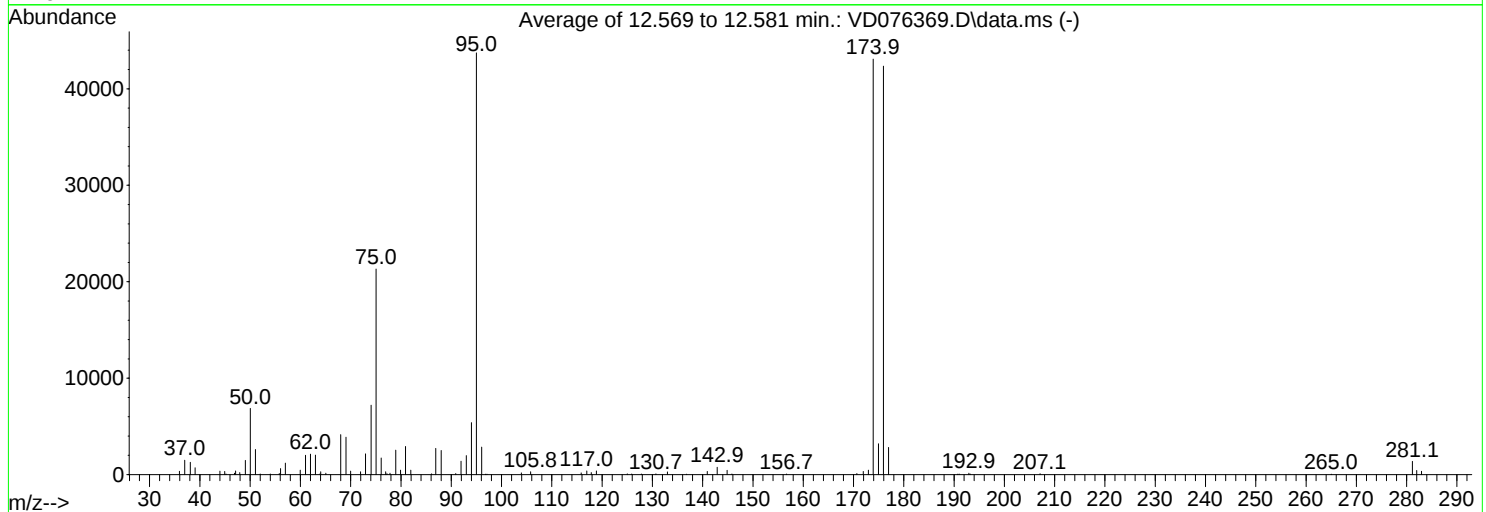


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060823\
Data File : VD076369.D
Acq On : 08 Jun 2023 12:24
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060523S.M
Title : SW846 8260
Last Update : Tue Jun 06 02:52:23 2023

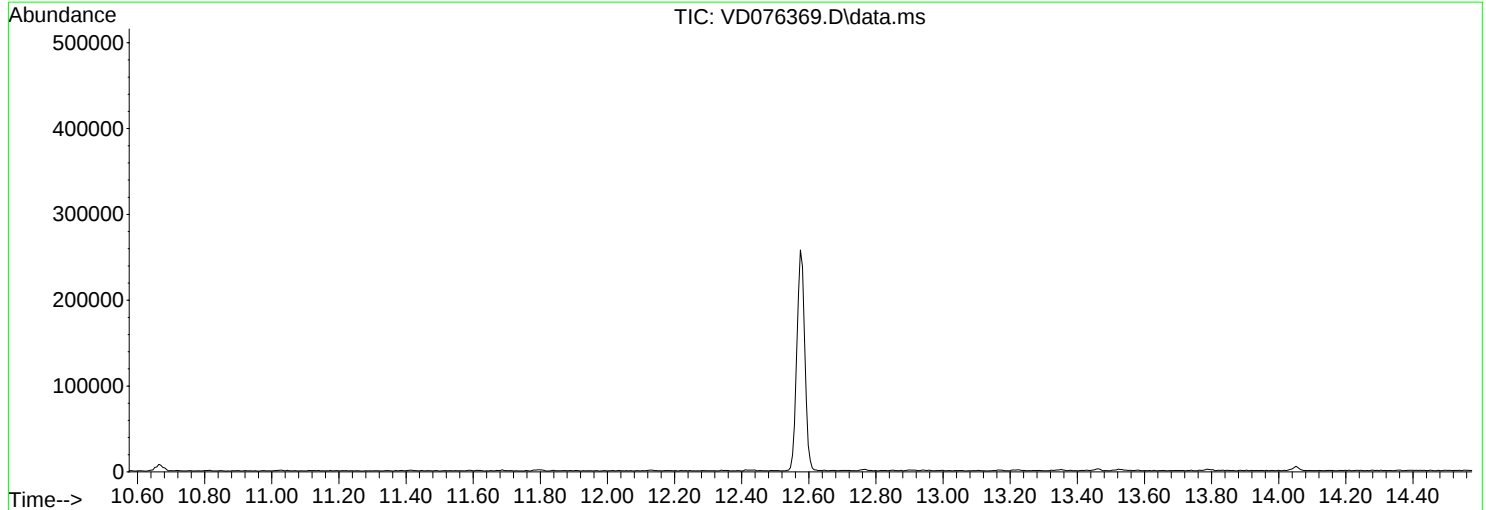

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	6866	PASS
75	95	30	60	48.7	21312	PASS
95	95	100	100	100.0	43728	PASS
96	95	5	9	6.5	2859	PASS
173	174	0.00	2	1.1	464	PASS
174	95	50	100	98.5	43085	PASS
175	174	5	9	7.4	3206	PASS
176	174	95	101	98.3	42341	PASS
177	176	5	9	6.7	2816	PASS