

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062321\
 Data File : VD069539.D
 Acq On : 23 Jun 2021 12:29
 Operator : VA/SY
 Sample : M2816-01
 Misc : 6.01G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 OK-02-062221

Quant Time: Jun 24 06:07:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 22 04:33:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	575146	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	1175159	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	1195000	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	506478	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	427455	59.62	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	119.24%
35) Dibromofluoromethane	7.914	113	407324	51.28	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.56%
50) Toluene-d8	10.338	98	1529250	51.32	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.64%
62) 4-Bromofluorobenzene	12.626	95	568988	58.08	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	116.16%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062321\
Data File : VD069539.D
Acq On : 23 Jun 2021 12:29
Operator : VA/SY
Sample : M2816-01
Misc : 6.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
OK-02-062221

Quant Time: Jun 24 06:07:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 22 04:33:24 2021
Response via : Initial Calibration



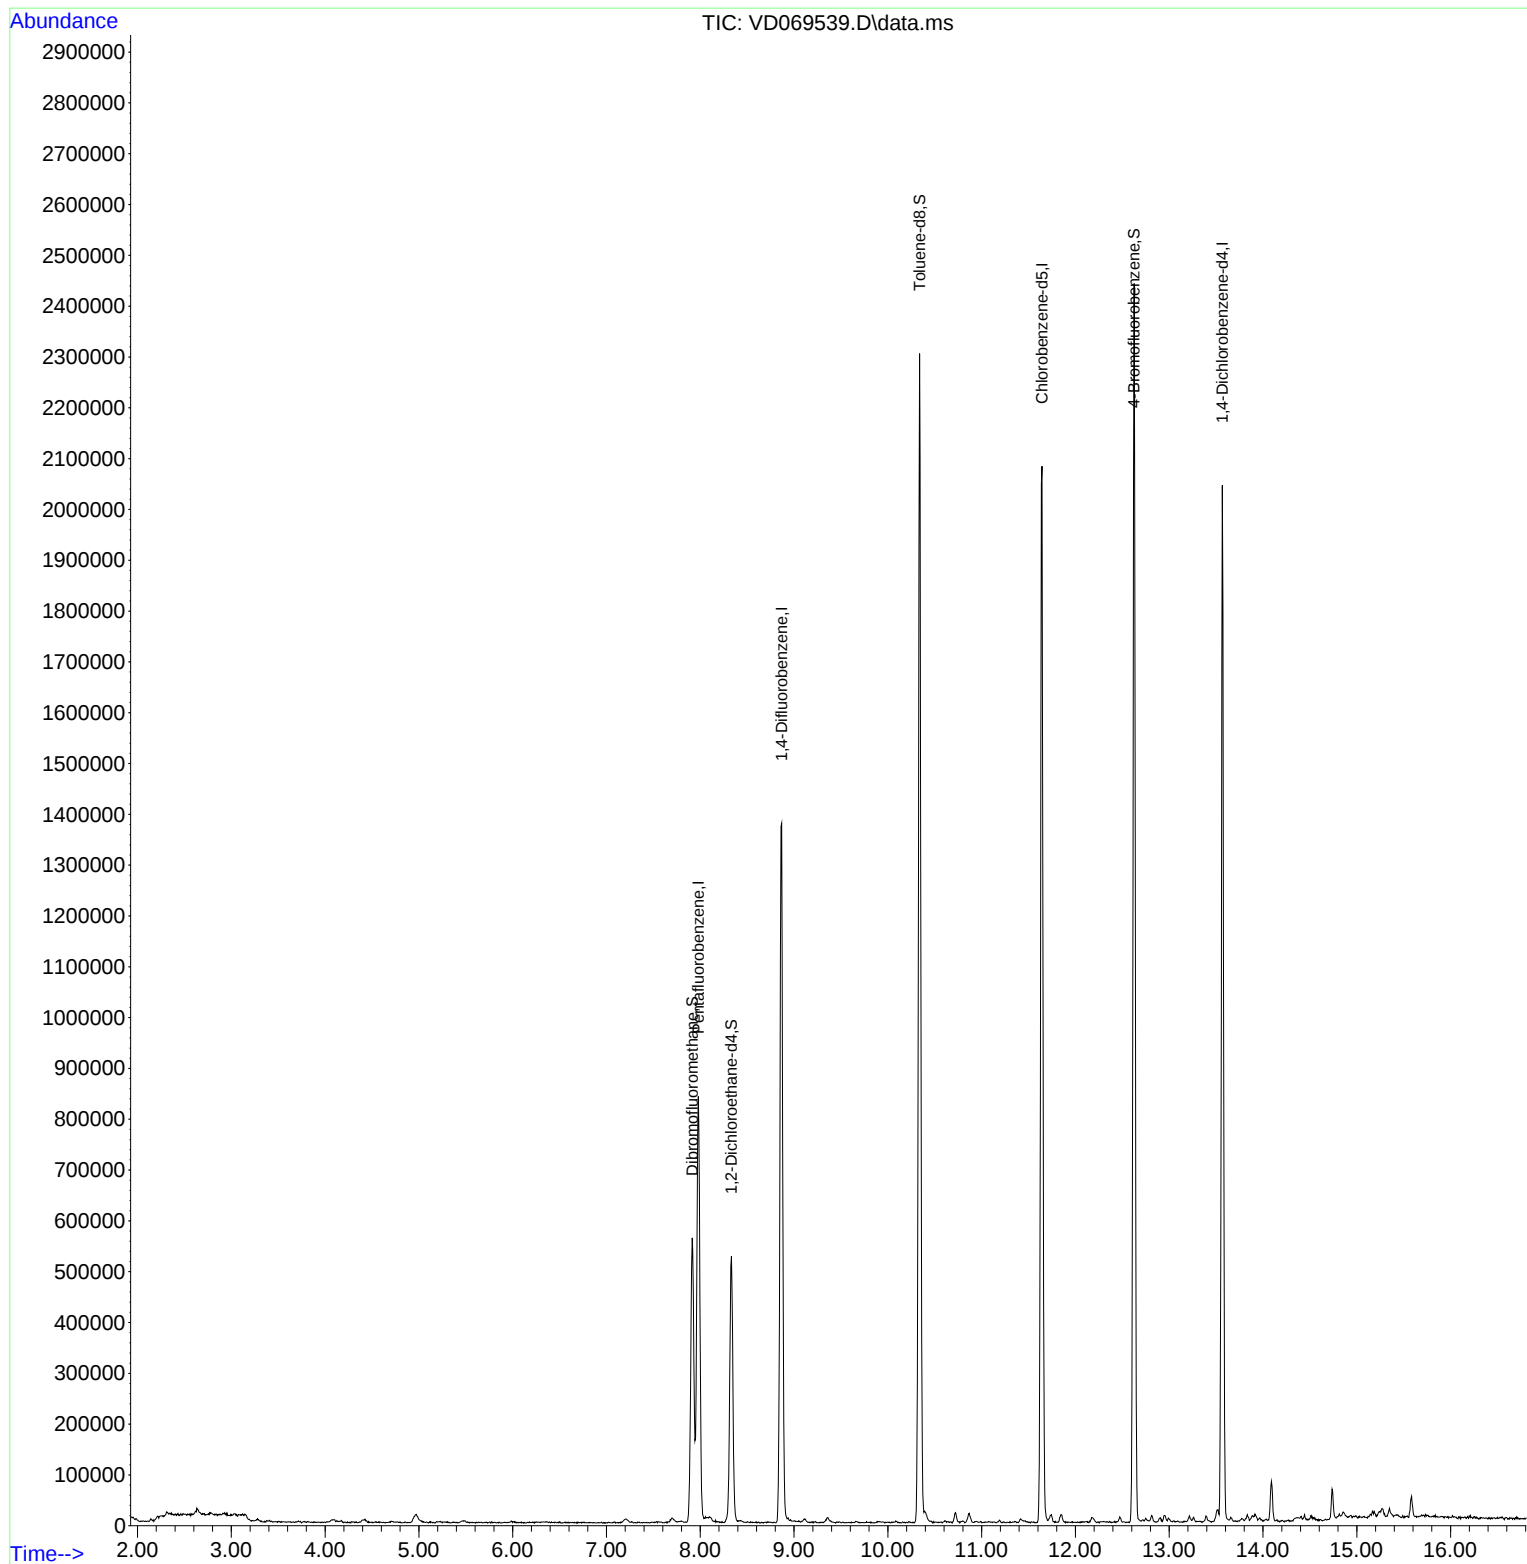


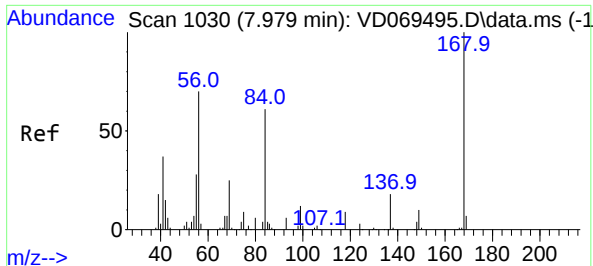

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :
OK-02-062221


Tgt Ion:168 Resp: 575146
Ion Ratio Lower Upper
168 100
99 65.7 49.3 73.9

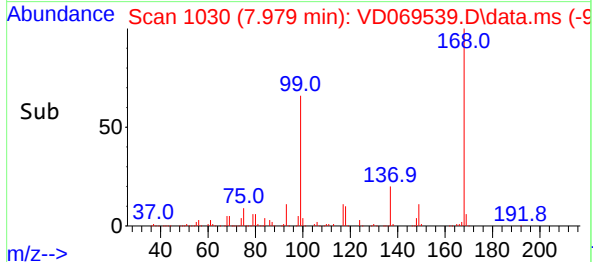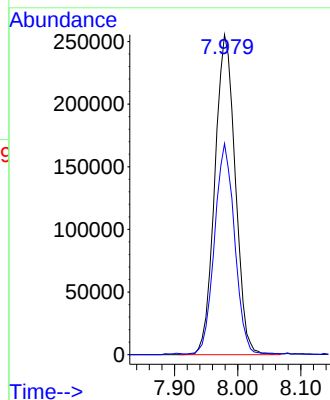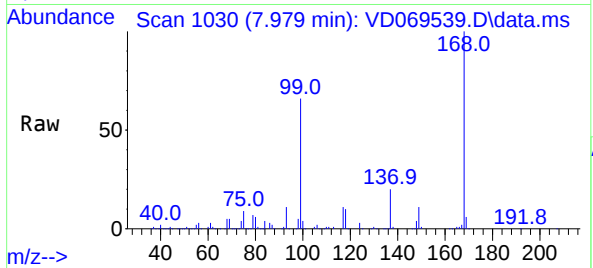

#33
1,2-Dichloroethane-d4
Concen: 59.62 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29

Tgt Ion: 65 Resp: 427455
Ion Ratio Lower Upper
65 100
67 52.8 0.0 105.6

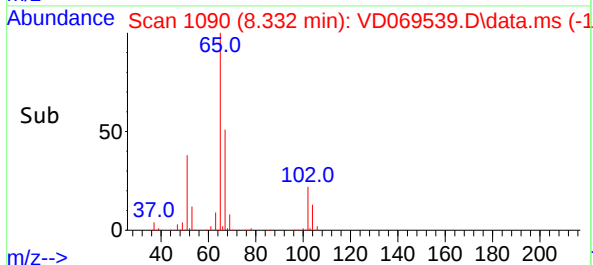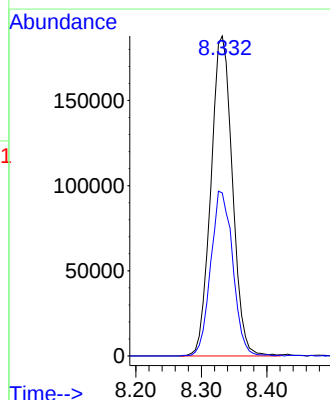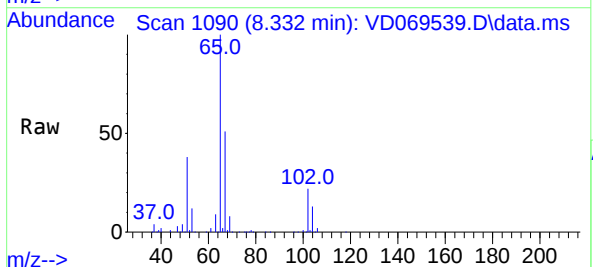




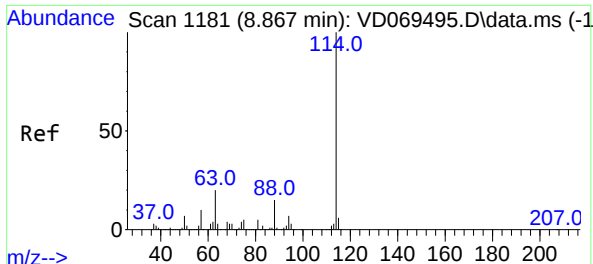


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29

Instrument :
MSVOA_D
ClientSampleId :
OK-02-062221




Tgt Ion:114 Resp: 1175159
Ion Ratio Lower Upper
114 100
63 20.8 0.0 39.6
88 15.9 0.0 29.8

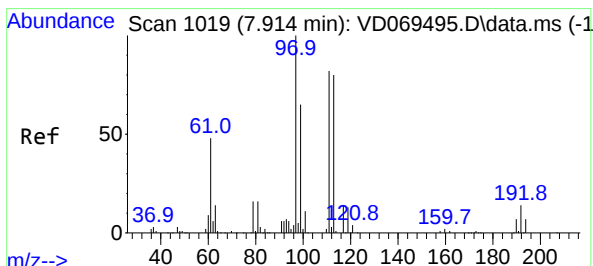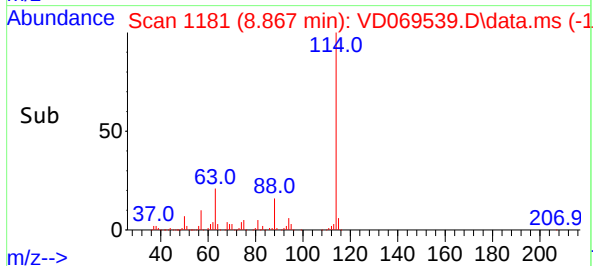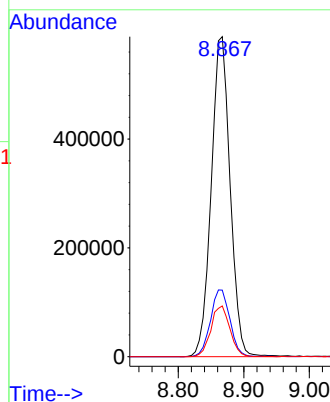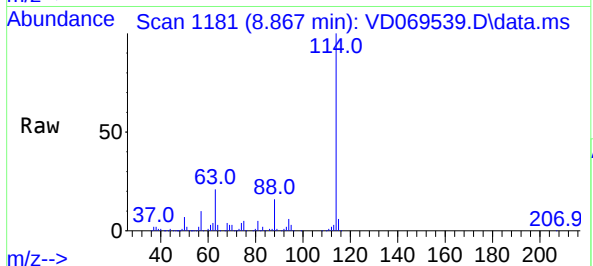


#35

Dibromofluoromethane
Concen: 51.28 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29

Tgt Ion:113 Resp: 407324
Ion Ratio Lower Upper
113 100
111 102.7 81.8 122.8
192 16.8 13.8 20.6


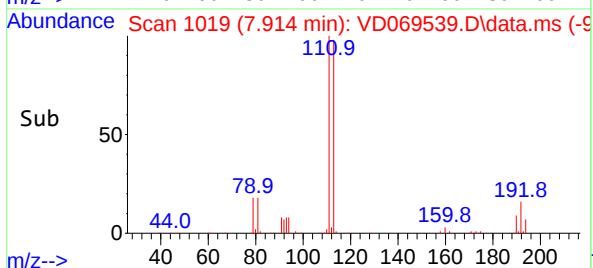
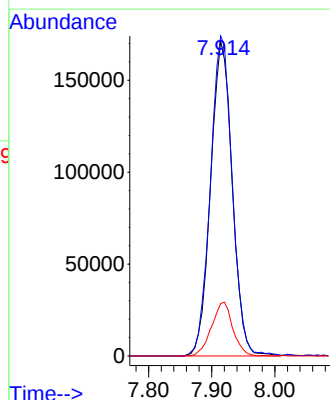
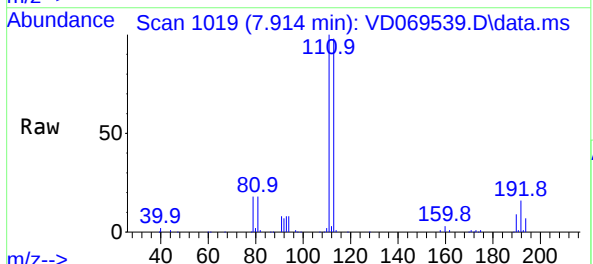


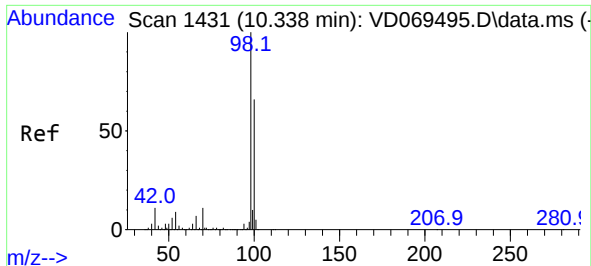

#50
Toluene-d8
Concen: 51.32 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29




Instrument :
MSVOA_D
ClientSampleId :
OK-02-062221


Tgt Ion: 98 Resp: 1529250
Ion Ratio Lower Upper
98 100
100 63.8 52.3 78.5

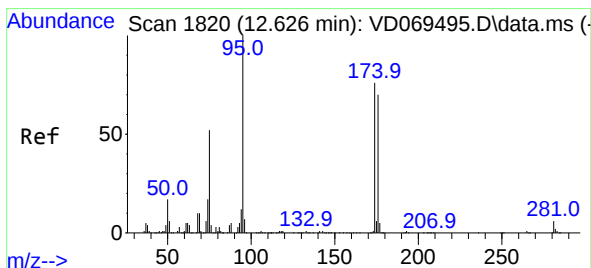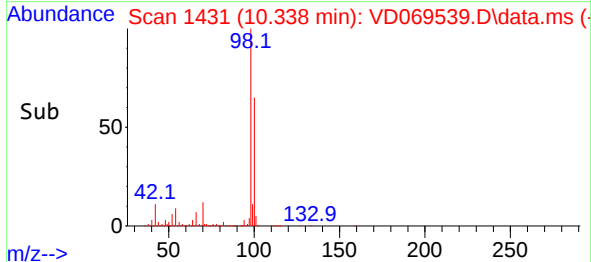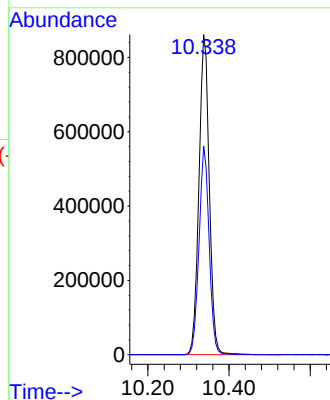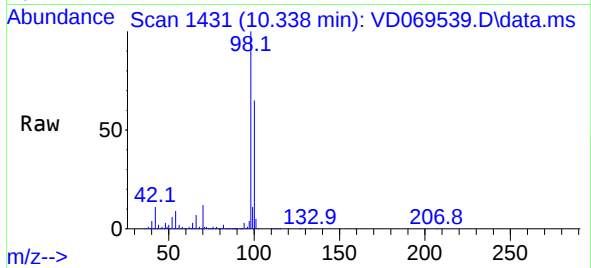

#62
4-Bromofluorobenzene
Concen: 58.08 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29


Tgt Ion: 95 Resp: 568988
Ion Ratio Lower Upper
95 100
174 71.6 0.0 148.0
176 68.8 0.0 139.8

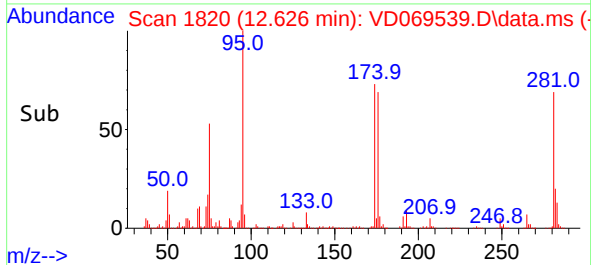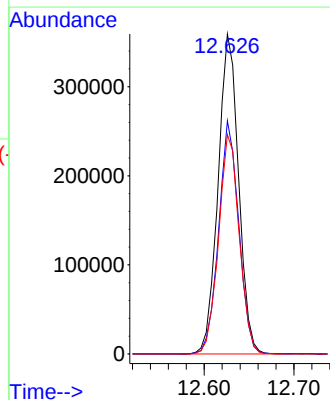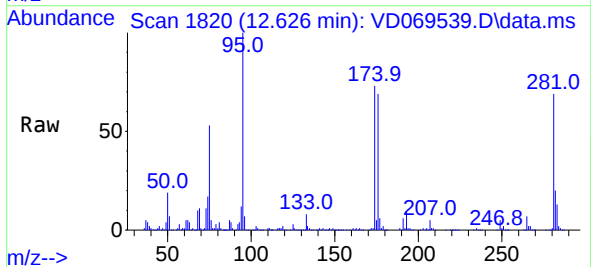

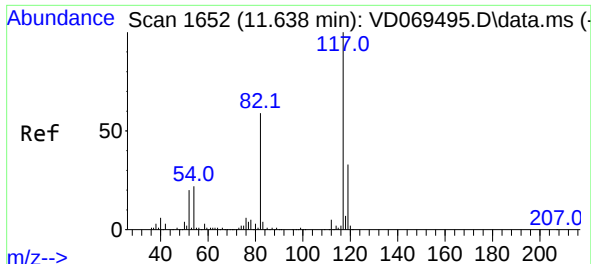




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.006 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29

Instrument :
MSVOA_D
ClientSampleId :
OK-02-062221

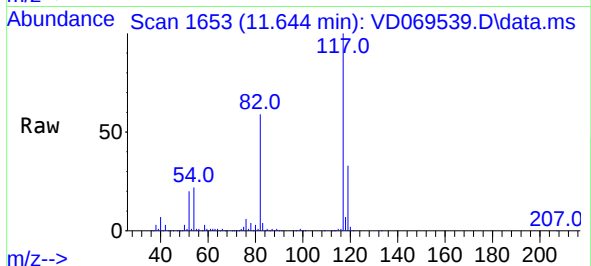


Tgt Ion:117 Resp: 1195000

Ion	Ratio	Lower	Upper
117	100		
82	58.9	46.8	70.2
119	32.8	26.2	39.2

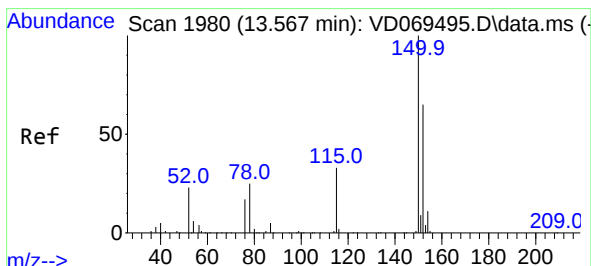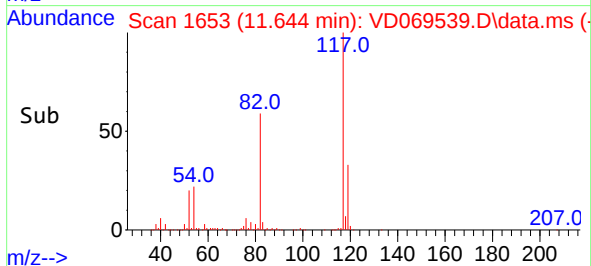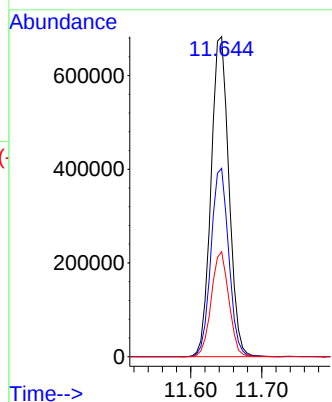

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD069539.D
Acq: 23 Jun 2021 12:29

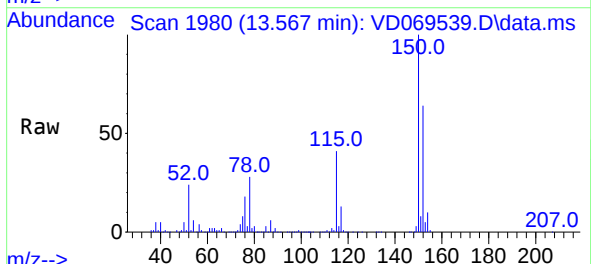

Tgt Ion:152 Resp: 506478

Ion	Ratio	Lower	Upper
152	100		
115	64.1	31.7	95.1
150	158.9	0.0	350.8

